




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040422\
 Data File : VW022390.D
 Acq On : 04 Apr 2022 16:40
 Operator : SY/VA
 Sample : N2179-04
 Misc : 4.43g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0R43

Manual IntegrationsAPPROVED

Quant Time: Apr 05 01:57:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 05 01:44:25 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/05/2022
 Supervised By :Mahesh Dadoda 04/06/2022

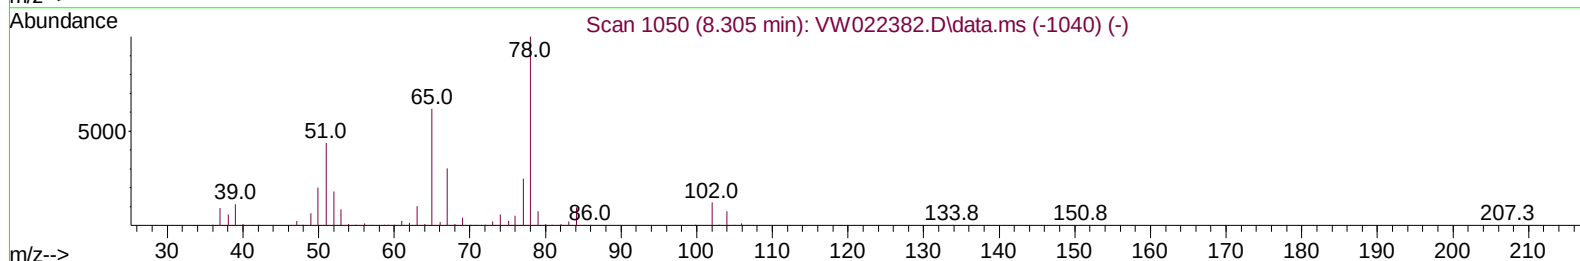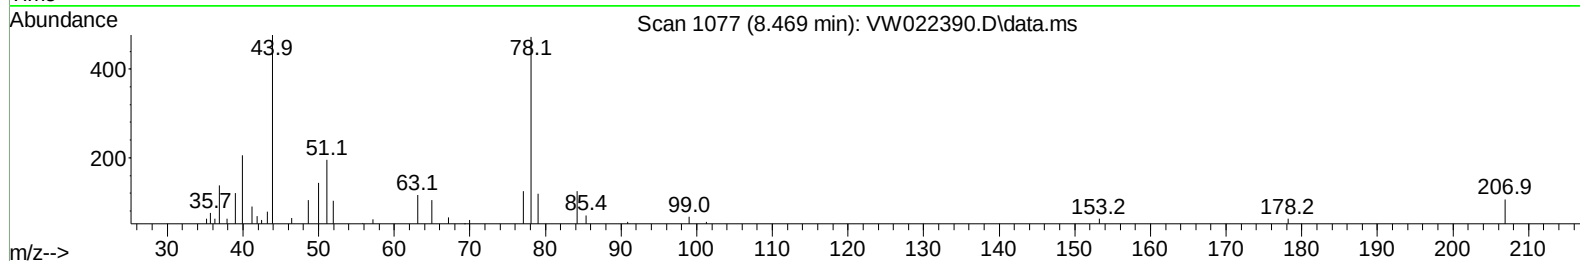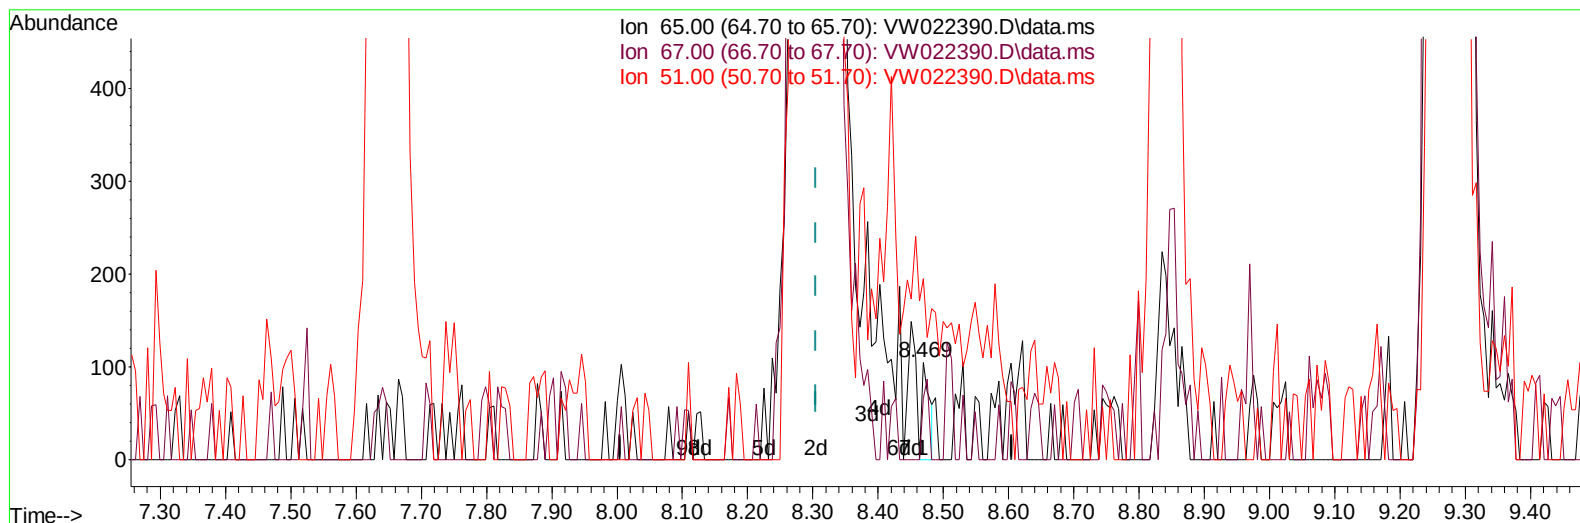

TIC: VW022390.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.469min (+ 0.164) 0.03 ug/L

response 87

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.50	64.37
51.00	90.00	81.61
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040422\
 Data File : VW022390.D
 Acq On : 04 Apr 2022 16:40
 Operator : SY/VA
 Sample : N2179-04
 Misc : 4.43g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0R43

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/05/2022
 Supervised By :Mahesh Dadoda 04/06/2022

Quant Time: Apr 05 01:57:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 05 01:44:25 2022
 Response via : Initial Calibration

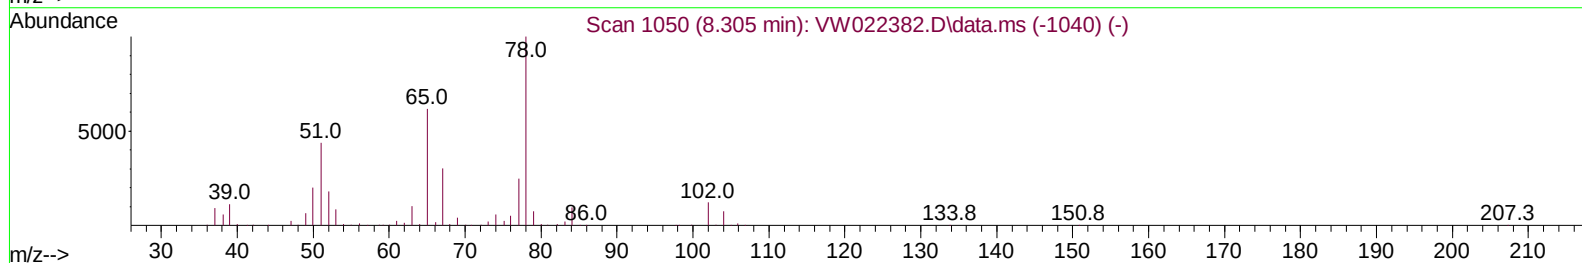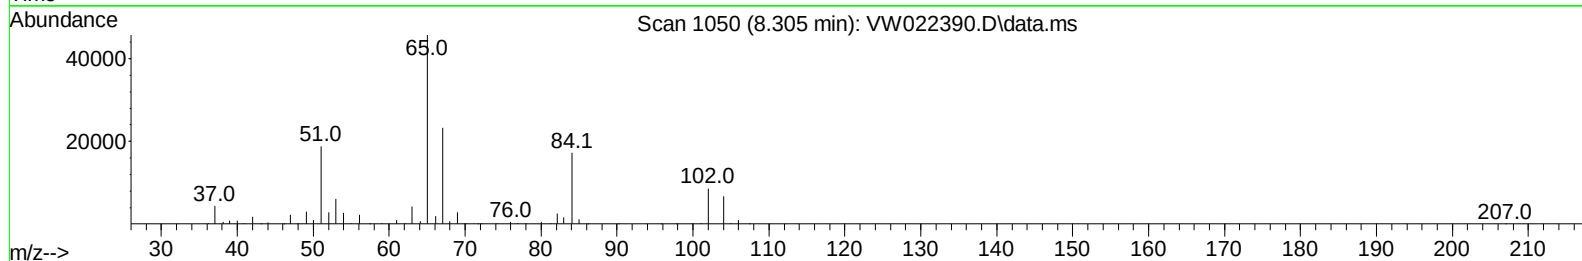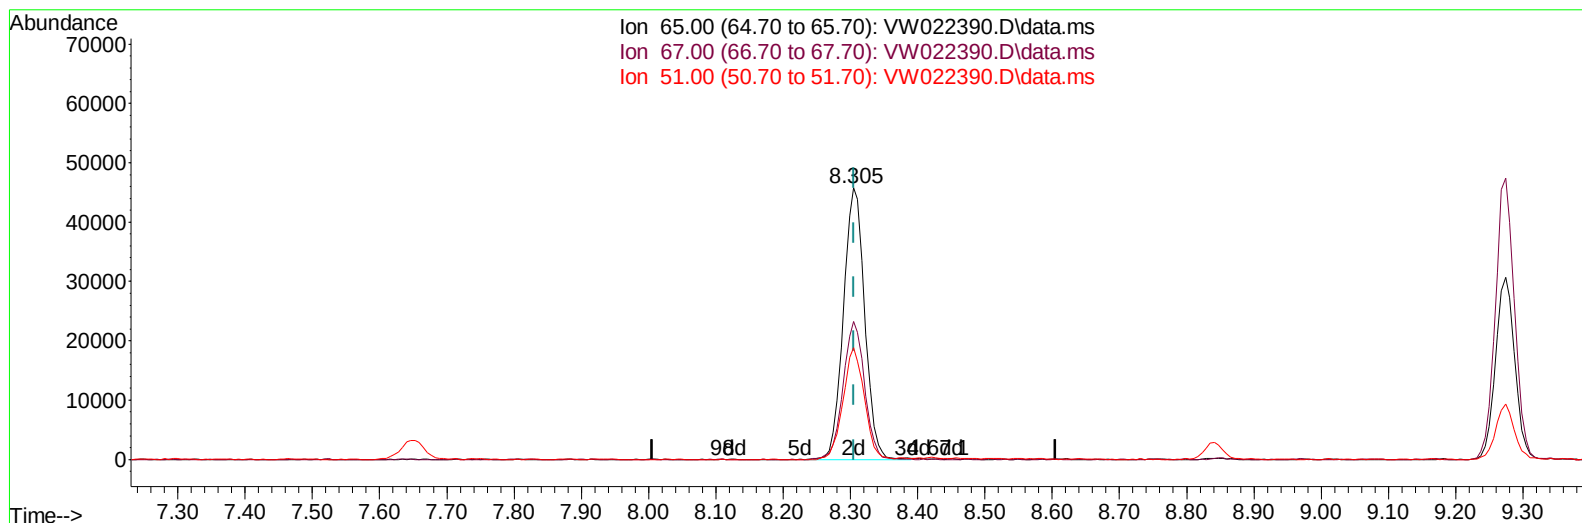

TIC: VW022390.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (-0.000) 29.27 ug/L m

response 100573

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.50	0.06#
51.00	90.00	0.07#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040422\
 Data File : VW022390.D
 Acq On : 04 Apr 2022 16:40
 Operator : SY/VA
 Sample : N2179-04
 Misc : 4.43g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0R43

Manual IntegrationsAPPROVED

Quant Time: Apr 05 01:57:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 05 01:44:25 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/05/2022
 Supervised By :Mahesh Dadoda 04/06/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.841	114		208439	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.633	117		190379	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		76469	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		103329	30.248	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	121.000%	
7) Chloroethane-d5	2.885	69		74717	36.637	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	146.560%	
11) 1,1-Dichloroethene-d2	4.019	63		92138	18.178	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	72.720%	
21) 2-Butanone-d5	7.073	46		49403	59.185	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	118.360%	
24) Chloroform-d	7.646	84		149523	25.727	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	102.920%	
26) 1,2-Dichloroethane-d4	8.305	65		100573m	29.265	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	117.080%	
32) Benzene-d6	8.274	84		311203	29.768	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	119.080%	
36) 1,2-Dichloropropane-d6	9.274	67		93470	29.781	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	119.120%	
41) Toluene-d8	10.323	98		293936	29.553	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	118.200%	
43) trans-1,3-Dichloroprop...	10.579	79		40917	25.925	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	103.680%	
47) 2-Hexanone-d5	10.920	63		43478	67.625	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	135.260%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		80895	30.552	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	122.200%#	
66) 1,2-Dichlorobenzene-d4	13.853	152		71083	28.795	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	115.200%	
Target Compounds							
13) Acetone	4.123	43		22472	39.315	ug/L	Qvalue 96
22) 2-Butanone	7.171	43		9587	10.633	ug/L	77

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040422\
Data File : VW022390.D
Acq On : 04 Apr 2022 16:40
Operator : SY/VA
Sample : N2179-04
Misc : 4.43g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0R43

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/05/2022
Supervised By :Mahesh Dadoda 04/06/2022

Quant Time: Apr 05 01:57:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Apr 05 01:44:25 2022
Response via : Initial Calibration

