

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040422\
 Data File : VW022386.D
 Acq On : 04 Apr 2022 15:04
 Operator : SY/VA
 Sample : N2225-05
 Misc : 7.99g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGQD4

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/05/2022
 Supervised By :Mahesh Dadoda 04/06/2022

Quant Time: Apr 05 01:56:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Apr 05 01:44:25 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	184856	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	177735	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	93991	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	79760	26.327	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 105.320%			
7) Chloroethane-d5	2.891	69	56557	31.270	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 125.080%			
11) 1,1-Dichloroethene-d2	4.019	63	80455	17.898	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 71.600%			
21) 2-Butanone-d5	7.079	46	50718	68.512	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 137.020%#			
24) Chloroform-d	7.652	84	117349	22.767	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 91.080%			
26) 1,2-Dichloroethane-d4	8.305	65	82421	27.043	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 108.160%			
32) Benzene-d6	8.274	84	245794	25.184	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 100.720%			
36) 1,2-Dichloropropane-d6	9.274	67	73479	25.077	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 100.320%			
41) Toluene-d8	10.323	98	238937	25.732	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 102.920%			
43) trans-1,3-Dichloroprop...	10.579	79	37467	25.428	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 101.720%			
47) 2-Hexanone-d5	10.920	63	41941	69.875	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 139.760%#			
56) 1,1,2,2-Tetrachloroeth...	12.688	84	77903	31.515	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 126.040%#			
66) 1,2-Dichlorobenzene-d4	13.853	152	84026	27.693	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 110.760%			
Target Compounds					Qvalue	
13) Acetone	4.135	43	4099m	8.086	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040422\
Data File : VW022386.D
Acq On : 04 Apr 2022 15:04
Operator : SY/VA
Sample : N2225-05
Misc : 7.99g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1




Instrument :
MSVOA_W
ClientSampleId :
BGQD4

Quant Time: Apr 05 01:56:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Apr 05 01:44:25 2022
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 04/05/2022
Supervised By :Mahesh Dadoda 04/06/2022

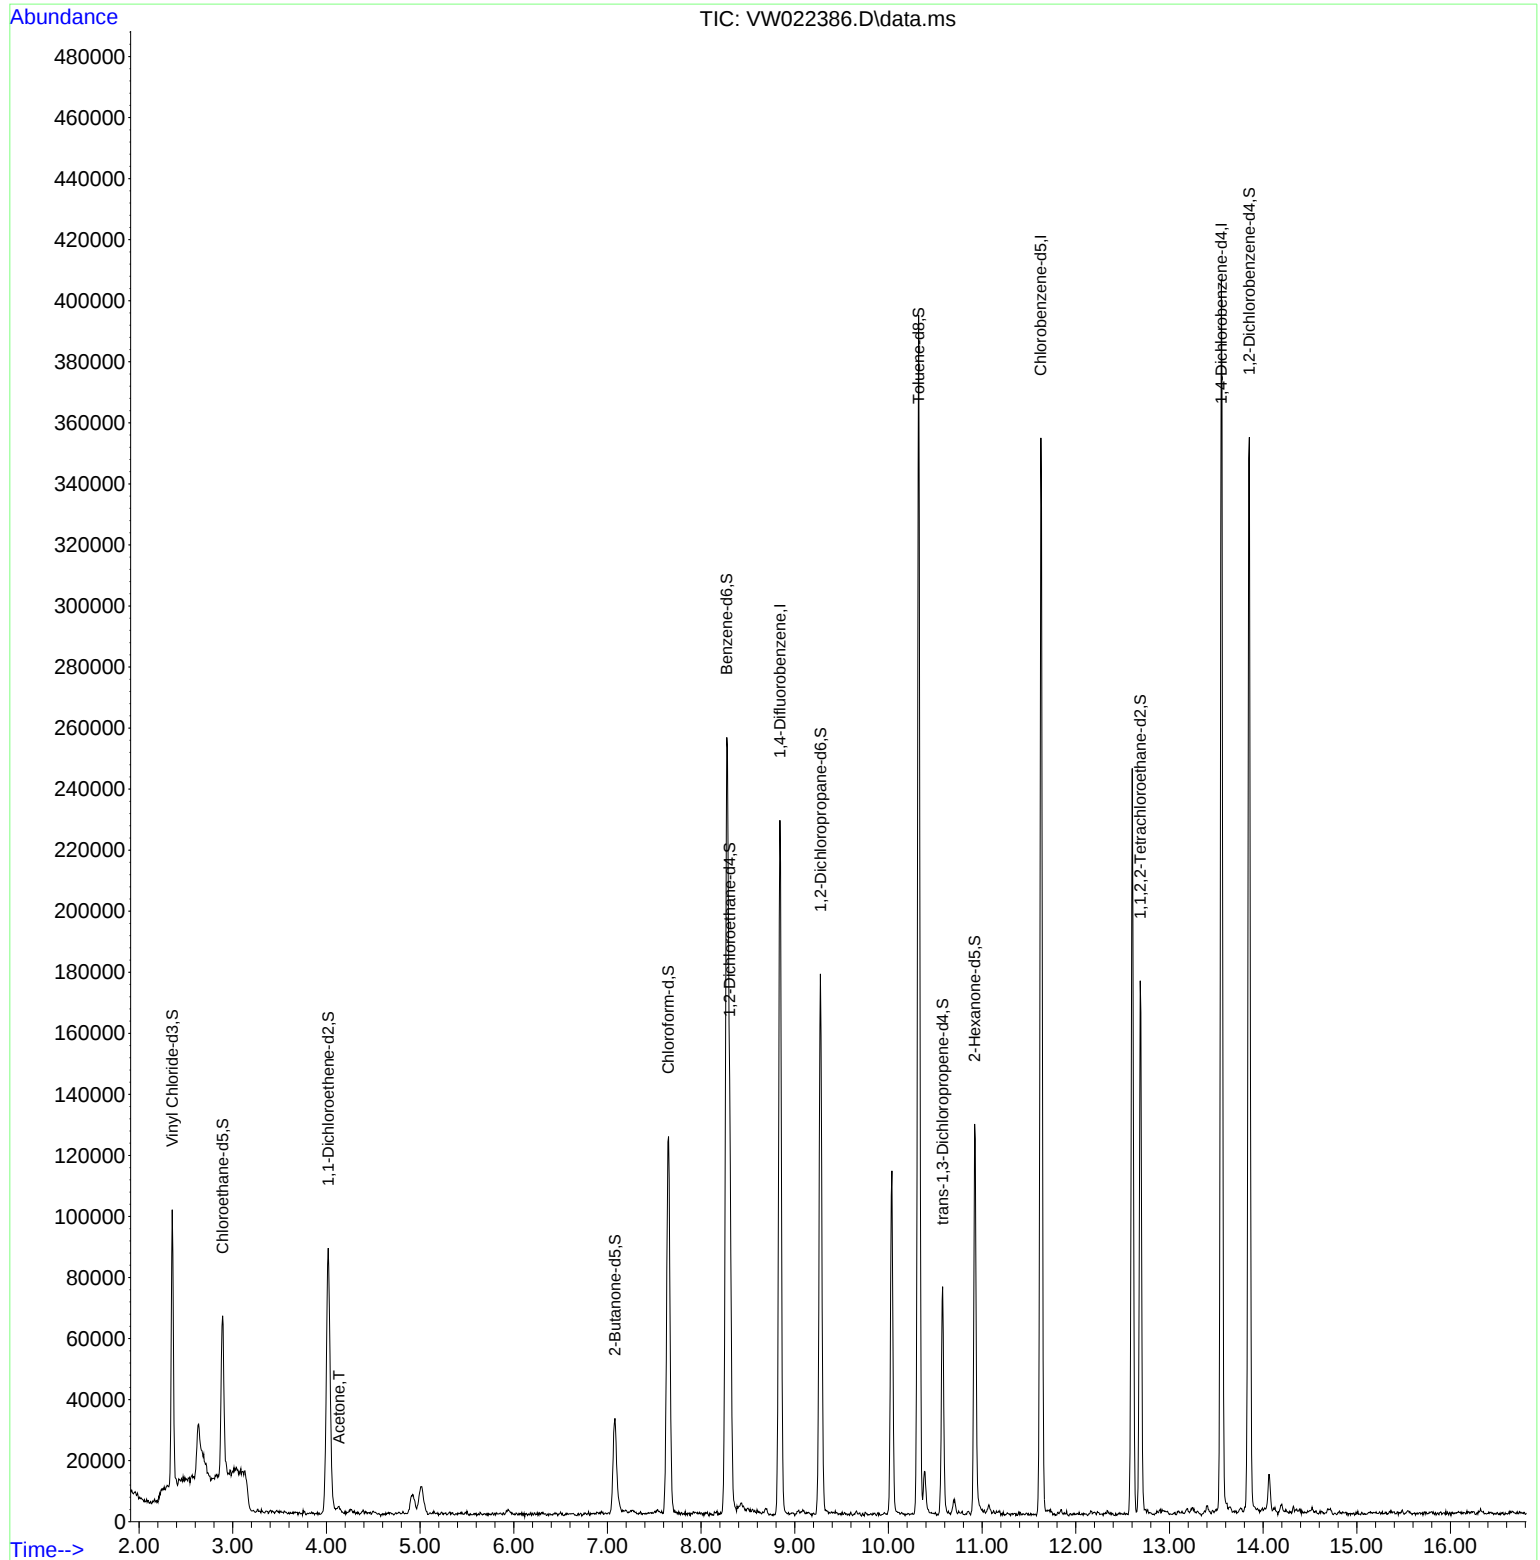

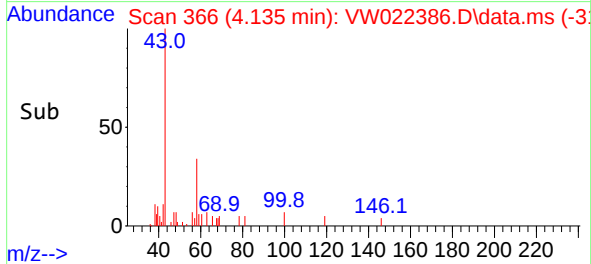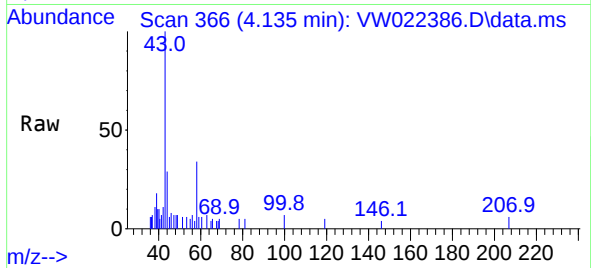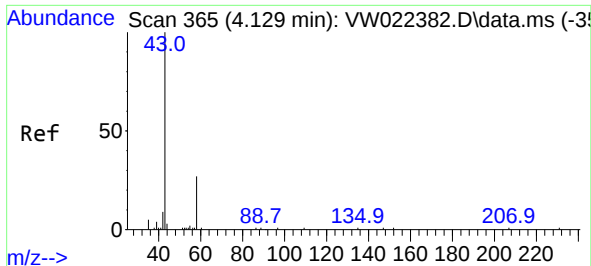

#13
Acetone
Concen: 8.086 ug/L m
RT: 4.135 min Scan# 30
Delta R.T. 0.006 min
Lab File: VW022386.D
Acq: 04 Apr 2022 15:04

Instrument :
MSVOA_W
ClientSampleId :
BGQD4

Tgt Ion: 43 Resp: 4099
Ion Ratio Lower Upper
43 100
58 29.1 0.0 69.2

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 04/05/2022
Supervised By :Mahesh Dadoda 04/06/2022

