
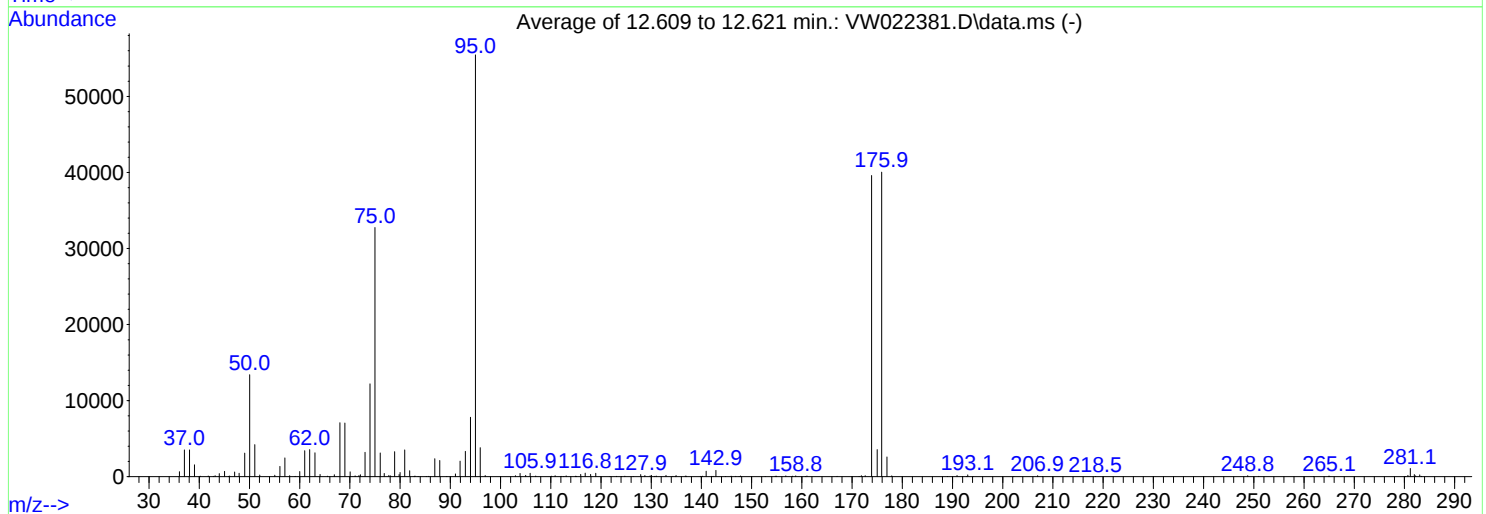


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040422\
 Data File : VW022381.D
 Acq On : 04 Apr 2022 09:58
 Operator : SY/VA
 Sample : BFB526
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB526

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Title : SFAM01.0
 Last Update : Wed Apr 06 02:13:06 2022

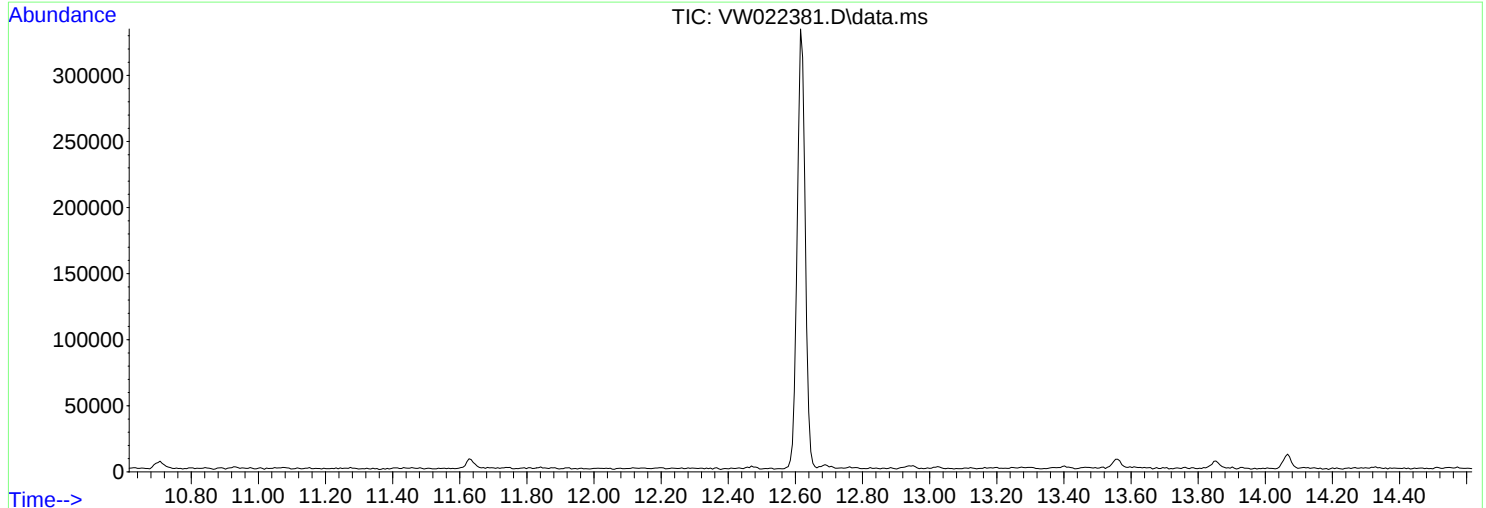

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.2	13406	PASS
75	95	30	80	59.1	32755	PASS
95	95	100	100	100.0	55467	PASS
96	95	5	9	6.9	3817	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.4	39608	PASS
175	174	5	9	9.0	3553	PASS
176	174	95	105	101.1	40048	PASS
177	176	5	10	6.4	2580	PASS

m/z	Abundance
35.50	89.0
37.10	98.0
38.70	81.0
39.90	186.0
40.70	57.0
41.10	70.0
42.00	101.0
44.00	717.0
45.10	67.0
46.30	137.0
47.40	56.0
49.30	105.0
50.10	107.0
52.40	55.0
55.10	117.0
57.30	71.0
95.80	70.0
207.00	101.0
209.20	65.0

Instrument :
MSVOA_W
ClientSampleId :
BFB526

m/z	Abundance
36.10	571.0
37.10	3128.0
38.00	3307.0
39.00	1413.0
39.90	178.0
40.20	184.0
41.90	113.0
42.80	110.0
44.10	996.0
45.00	754.0
46.10	163.0
47.10	522.0
47.90	425.0
49.10	3040.0
50.00	12012.0
51.00	3607.0
52.10	186.0
55.10	213.0
56.00	1305.0
57.10	2100.0
59.10	122.0
60.00	551.0
61.00	2977.0
62.00	3263.0
63.00	2734.0
64.10	258.0
65.60	55.0
66.90	306.0
68.00	5943.0
69.00	5828.0
70.10	449.0
71.10	117.0
72.10	351.0
73.00	3136.0
74.00	11065.0
75.00	28032.0
76.10	2723.0
76.80	358.0
77.70	180.0
78.90	2874.0
79.80	855.0
80.90	3206.0
81.90	741.0
82.80	91.0
83.60	65.0
85.20	69.0
85.70	56.0
86.90	2135.0
87.90	2145.0
89.30	63.0
91.10	329.0
92.00	1906.0
93.00	2906.0
94.00	6446.0
95.00	47976.0
96.00	3667.0
96.90	129.0
103.00	185.0
103.90	396.0
105.10	151.0
105.90	441.0
107.00	75.0
110.90	159.0
113.00	127.0
114.90	133.0
115.90	228.0
116.80	317.0
118.00	284.0
118.90	388.0
121.80	52.0
124.10	60.0
124.70	66.0
127.80	192.0
128.80	108.0
130.10	171.0
130.70	149.0
132.90	292.0
134.30	69.0
134.80	127.0
136.80	87.0
140.90	530.0
142.30	133.0
142.90	578.0
145.90	73.0
146.80	71.0
147.50	76.0
155.00	84.0
156.80	68.0
158.10	67.0
159.00	76.0
161.00	175.0
171.40	94.0

Instrument :
MSVOA_W
ClientSampleId :
BFB526

172.60	392.0
173.90	26440.0
175.00	3024.0
175.90	29144.0
176.90	2082.0
178.00	119.0
189.00	58.0
190.90	243.0
193.10	312.0
194.10	96.0
202.20	90.0
207.00	309.0
207.90	66.0
209.10	66.0
218.50	68.0
248.80	133.0
251.00	69.0
261.90	53.0
264.90	184.0
280.20	59.0
281.10	1573.0
281.90	551.0
283.10	392.0

Instrument :
MSVOA_W
ClientSampleId :
BFB526

m/z	Abundance
36.10	730.0
37.00	4481.0
38.00	3817.0
39.10	1733.0
39.90	146.0
41.20	53.0
41.70	68.0
42.20	55.0
43.20	138.0
44.00	1084.0
45.10	810.0
46.00	123.0
47.00	661.0
48.00	420.0
49.00	3342.0
50.10	14942.0
51.10	4974.0
52.10	252.0
55.00	381.0
56.00	1519.0
57.00	2735.0
58.00	135.0
60.00	806.0
61.00	3509.0
62.00	3859.0
63.10	3489.0
64.00	351.0
65.50	83.0
66.80	243.0
68.00	7860.0
69.00	8266.0
70.00	776.0
71.00	102.0
71.80	470.0
73.00	3397.0
74.00	13713.0
75.00	37816.0
76.00	3534.0
76.90	514.0
77.80	330.0
78.90	3638.0
80.00	887.0
80.90	4087.0
81.90	689.0
83.00	111.0
85.70	102.0
86.90	2776.0
87.90	2373.0
91.00	373.0
91.90	2137.0
93.00	3776.0
94.00	8759.0
95.00	62032.0
96.00	4278.0
97.00	172.0
102.90	122.0
104.00	378.0
105.00	133.0
105.90	520.0
107.00	67.0
110.10	84.0
110.90	122.0
112.00	78.0
112.60	90.0
113.10	86.0
114.90	87.0
116.00	271.0
116.80	506.0
117.90	353.0
119.00	511.0
123.10	66.0
124.70	56.0
126.40	53.0
127.90	267.0
128.70	130.0
129.80	288.0
131.00	141.0
133.00	109.0
134.30	56.0
135.00	236.0
136.80	140.0
139.80	117.0
141.00	905.0
142.00	154.0
142.90	1146.0
147.90	122.0
152.70	50.0
154.90	126.0
156.80	81.0
158.10	89.0
158.80	128.0
161.00	72.0

Instrument :
MSVOA_W
ClientSampleId :
BFB526

167.00	55.0
171.90	196.0
173.90	46176.0
175.00	3727.0
175.90	43384.0
177.00	2875.0
177.90	136.0
190.90	84.0
192.00	56.0
193.00	321.0
207.00	193.0
248.80	131.0
251.00	88.0
265.10	127.0
280.70	486.0
281.20	723.0
282.20	305.0
283.00	200.0

Instrument :
MSVOA_W
ClientSampleId :
BFB526

m/z	Abundance
36.00	673.0
37.10	3259.0
38.10	3403.0
39.10	1556.0
39.90	227.0
41.20	76.0
41.70	57.0
42.10	83.0
43.10	230.0
44.10	1285.0
45.00	718.0
45.80	146.0
47.10	626.0
48.00	464.0
49.00	2870.0
50.00	13586.0
51.10	4025.0
52.00	215.0
55.10	306.0
56.10	1227.0
57.10	2575.0
58.00	237.0
60.00	673.0
61.00	3749.0
62.00	3528.0
63.10	3188.0
64.10	258.0
65.50	54.0
67.00	186.0
68.00	7469.0
69.00	7075.0
70.00	674.0
71.00	71.0
72.10	389.0
73.00	3075.0
74.00	11824.0
75.00	32416.0
76.10	3093.0
76.90	381.0
78.10	347.0
78.90	3335.0
80.00	790.0
80.90	3254.0
81.90	917.0
82.90	125.0
86.90	2190.0
87.90	1893.0
90.90	344.0
92.00	2053.0
93.00	3275.0
94.00	8247.0
95.00	56392.0
96.00	3715.0
97.00	167.0
102.80	55.0
103.80	477.0
104.90	206.0
105.90	366.0
107.00	126.0
110.20	88.0
110.70	101.0
112.10	63.0
113.10	95.0
115.10	124.0
115.90	377.0
116.90	546.0
118.00	264.0
118.90	405.0
123.10	78.0
124.80	62.0
128.00	377.0
128.80	189.0
130.00	309.0
131.00	122.0
132.90	113.0
134.90	229.0
137.00	162.0
140.20	167.0
140.90	691.0
142.90	761.0
144.80	93.0
145.90	92.0
146.90	65.0
147.70	147.0
154.70	170.0
156.80	161.0
158.20	52.0
158.70	123.0
160.70	92.0
167.00	55.0
170.00	66.0
171.80	165.0

Instrument :
MSVOA_W
ClientSampleId :
BFB526

173.90	46208.0
175.00	3909.0
175.90	47616.0
177.00	2783.0
177.80	80.0
190.90	107.0
192.80	86.0
193.20	89.0
206.90	170.0
209.10	84.0
248.80	110.0
265.10	83.0
281.10	955.0
282.00	262.0
283.00	88.0
283.40	129.0

Instrument :
MSVOA_W
ClientSampleId :
BFB526