

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
 Data File : VW022401.D
 Acq On : 05 Apr 2022 17:51
 Operator : SY/VA
 Sample : N2262-04
 Misc : 6.71g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Apr 06 02:15:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 06 02:13:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	174220	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	163033	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	66241	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	96845	33.918	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	135.680%
7) Chloroethane-d5	2.885	69	69724	40.904	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	163.600%#
11) 1,1-Dichloroethene-d2	4.013	63	76202	17.987	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	71.960%
21) 2-Butanone-d5	7.080	46	34473	49.410	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.820%
24) Chloroform-d	7.647	84	119007	24.498	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.000%
26) 1,2-Dichloroethane-d4	8.305	65	74180	25.825	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	103.280%
32) Benzene-d6	8.275	84	249419	27.860	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	111.440%
36) 1,2-Dichloropropane-d6	9.275	67	73690	27.417	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	109.680%
41) Toluene-d8	10.323	98	236730	27.793	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	111.160%
43) trans-1,3-Dichloroprop...	10.573	79	31782	23.514	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	94.040%
47) 2-Hexanone-d5	10.921	63	29597	53.756	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	107.520%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	61415	27.085	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	108.360%
66) 1,2-Dichlorobenzene-d4	13.847	152	61087	28.567	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	114.280%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	3436	0.810	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
Data File : VW022401.D
Acq On : 05 Apr 2022 17:51
Operator : SY/VA
Sample : N2262-04
Misc : 6.71g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Apr 06 02:15:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 06 02:13:06 2022
Response via : Initial Calibration

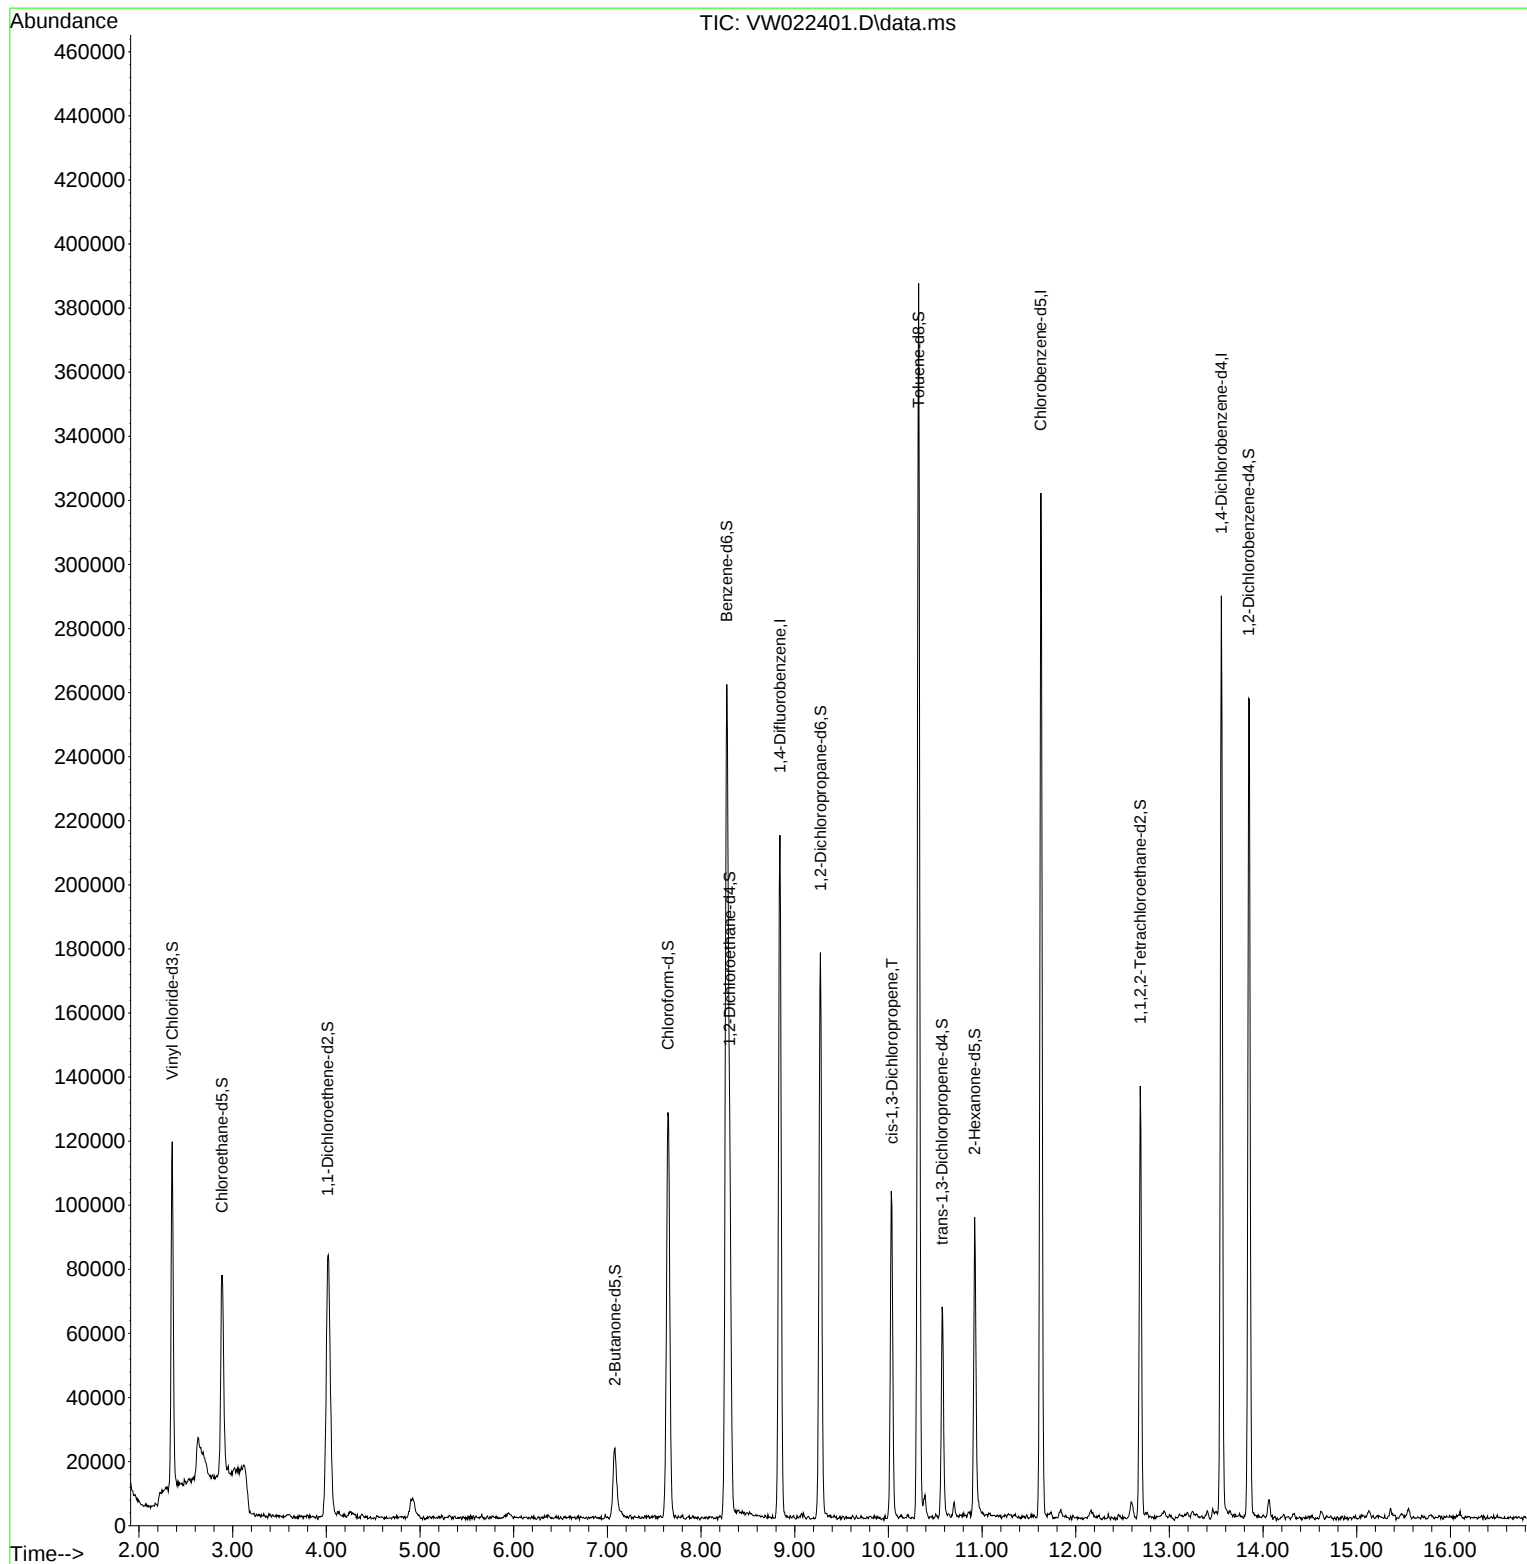

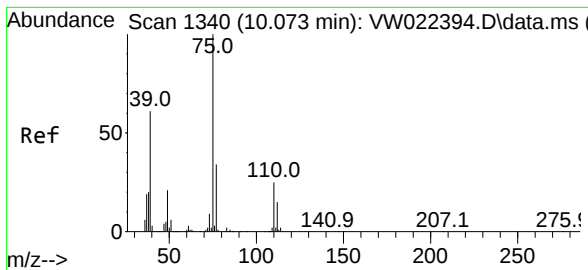

#39
 cis-1,3-Dichloropropene
 Concen: 0.810 ug/L
 RT: 10.037 min Scan# 11
 Delta R.T. -0.036 min
 Lab File: VW022401.D
 Acq: 05 Apr 2022 17:51

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 3436
 Ion Ratio Lower Upper
 75 100
 77 31.6 20.6 38.2

