

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
 Data File : VW022404.D
 Acq On : 05 Apr 2022 19:04
 Operator : SY/VA
 Sample : N2262-07
 Misc : 6.91g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Apr 06 02:15:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 06 02:13:06 2022
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		8.841	114	169678	25.000	ug/L	0.00
28) Chlorobenzene-d5		11.628	117	168949	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.554	152	73703	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.355	65	95495	34.340	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	137.360%	
7) Chloroethane-d5		2.885	69	69200	41.683	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	166.720%#	
11) 1,1-Dichloroethene-d2		4.013	63	68627	16.633	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.520%	
21) 2-Butanone-d5		7.080	46	33895	49.882	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.760%	
24) Chloroform-d		7.647	84	114186	24.135	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.560%	
26) 1,2-Dichloroethane-d4		8.305	65	72231	25.819	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	103.280%	
32) Benzene-d6		8.275	84	244102	26.311	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	105.240%	
36) 1,2-Dichloropropane-d6		9.274	67	70533	25.323	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.280%	
41) Toluene-d8		10.323	98	245004	27.758	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	111.040%	
43) trans-1,3-Dichloroprop...		10.579	79	30445	21.737	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.960%	
47) 2-Hexanone-d5		10.926	63	29829	52.281	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.560%	
56) 1,1,2,2-Tetrachloroeth...		12.688	84	58730	24.994	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	99.960%	
66) 1,2-Dichlorobenzene-d4		13.853	152	72507	30.474	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	121.880%#	
Target Compounds							
13) Acetone		4.123	43	1873	4.025	ug/L	Qvalue 76
39) cis-1,3-Dichloropropene		10.036	75	3489	0.794	ug/L #	44


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
Data File : VW022404.D
Acq On : 05 Apr 2022 19:04
Operator : SY/VA
Sample : N2262-07
Misc : 6.91g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Apr 06 02:15:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 06 02:13:06 2022
Response via : Initial Calibration




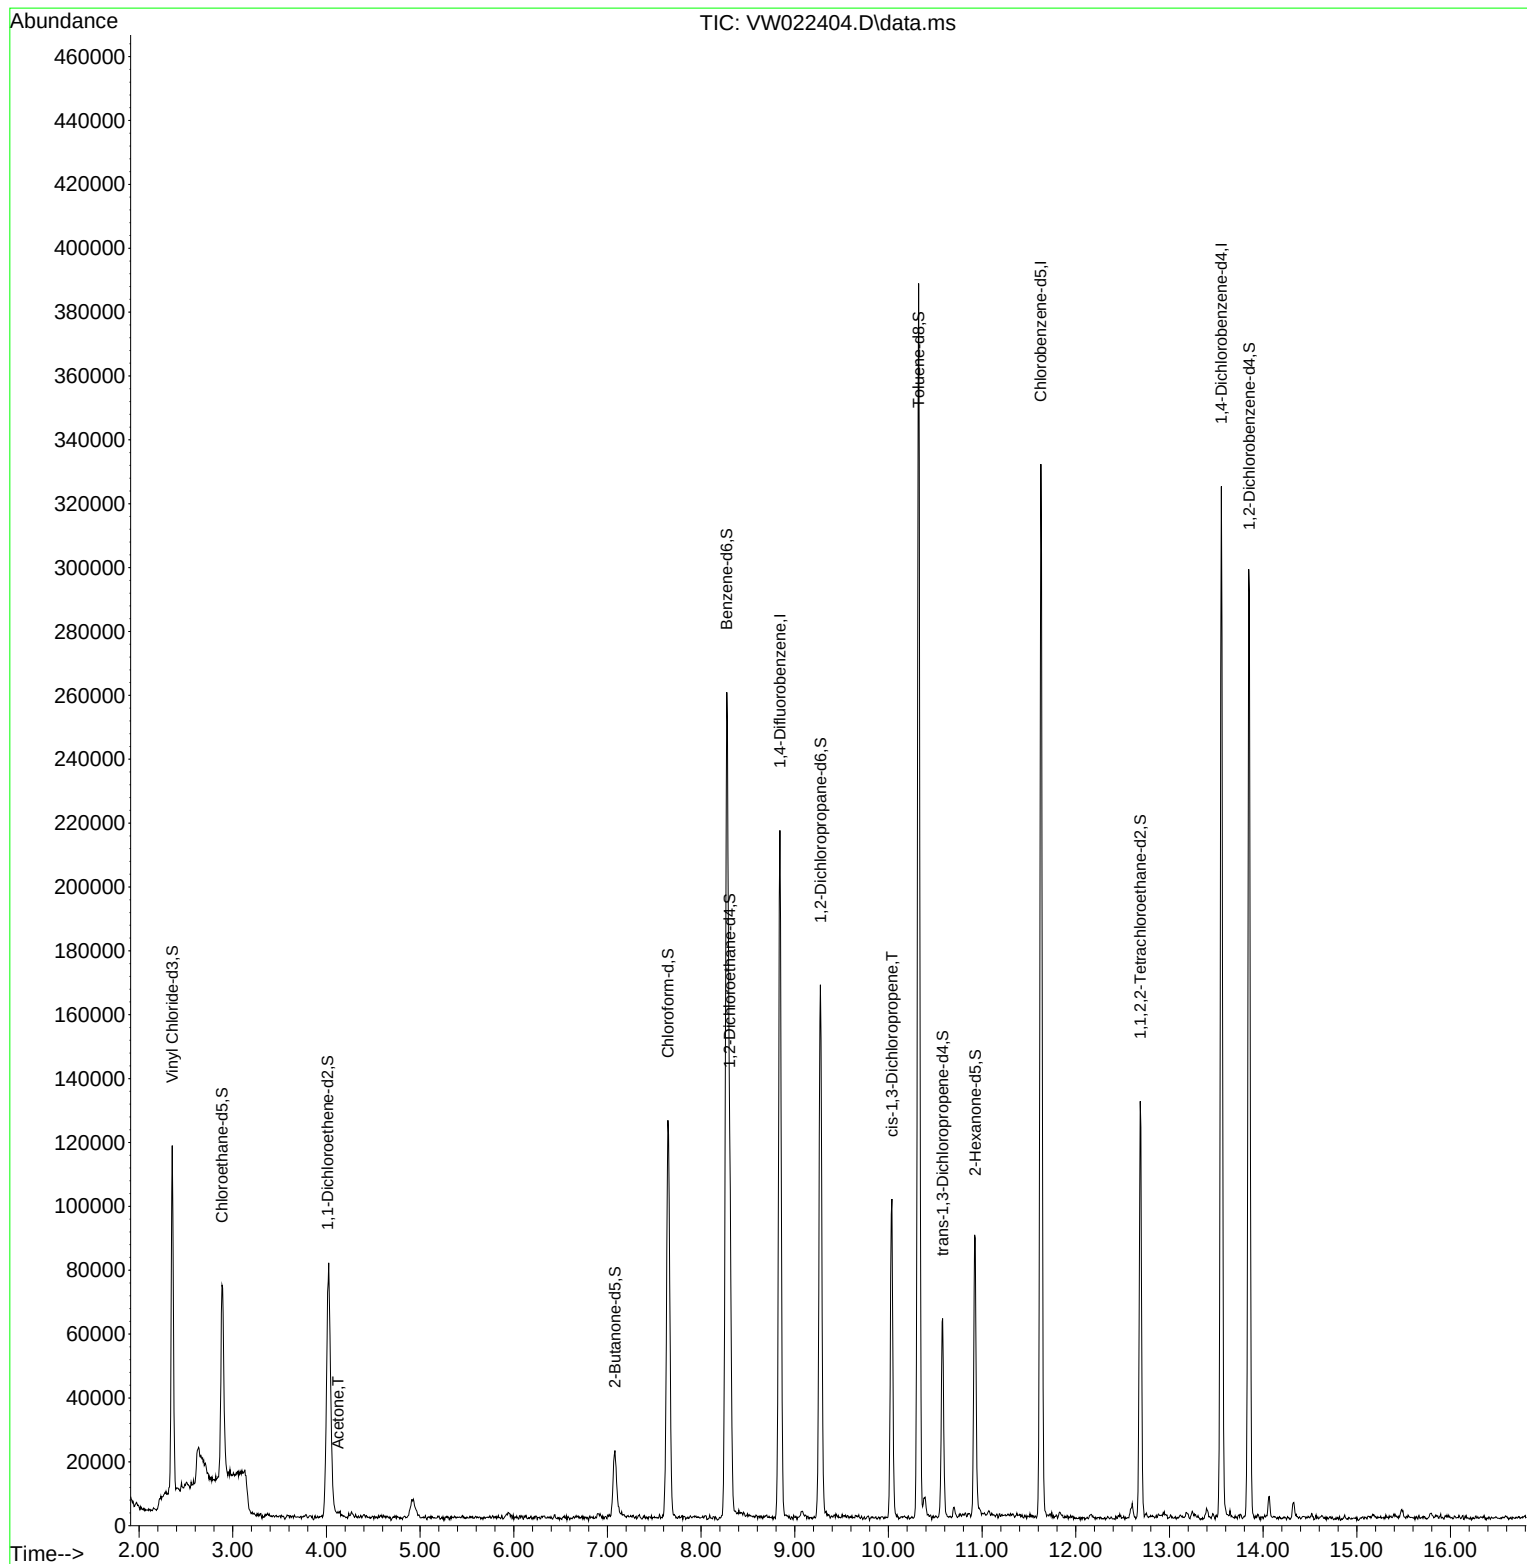


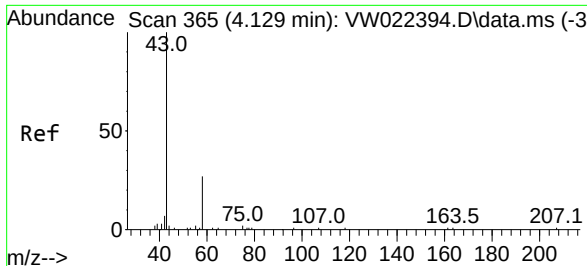

#13
Acetone
Concen: 4.025 ug/L
RT: 4.123 min Scan# 30
Delta R.T. -0.006 min
Lab File: VW022404.D
Acq: 05 Apr 2022 19:04

Instrument :
MSVOA_W
ClientSampleId :

Tgt Ion: 43 Resp: 1873
Ion Ratio Lower Upper
43 100
58 48.4 0.0 69.2

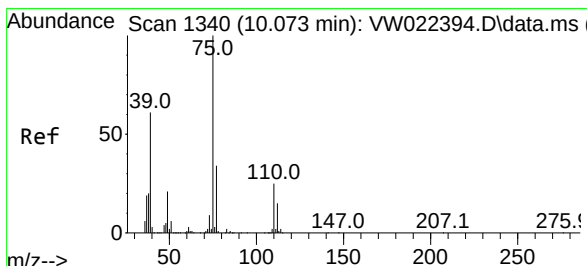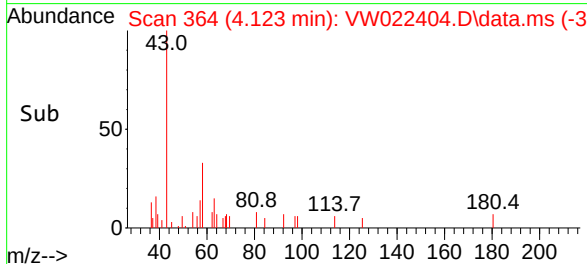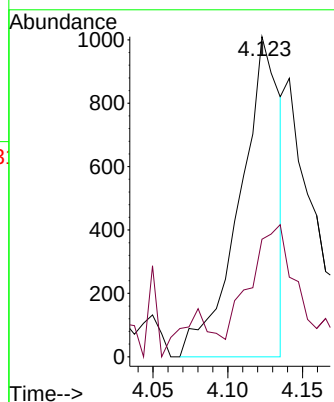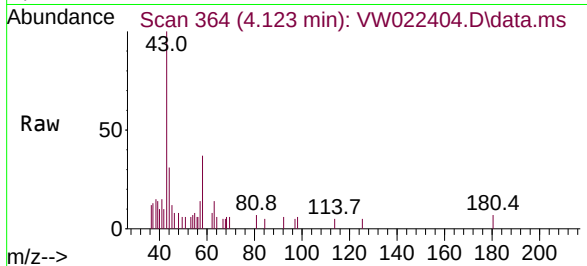

#39
cis-1,3-Dichloropropene
Concen: 0.794 ug/L
RT: 10.036 min Scan# 1334
Delta R.T. -0.037 min
Lab File: VW022404.D
Acq: 05 Apr 2022 19:04

Tgt Ion: 75 Resp: 3489
Ion Ratio Lower Upper
75 100
77 59.6 20.6 38.2#

