




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
 Data File : VW022398.D
 Acq On : 05 Apr 2022 16:39
 Operator : SY/VA
 Sample : N2262-01
 Misc : 6.07g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6K7

Manual IntegrationsAPPROVED

Quant Time: Apr 06 02:14:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 06 02:13:06 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/06/2022
 Supervised By :Mahesh Dadoda 04/07/2022

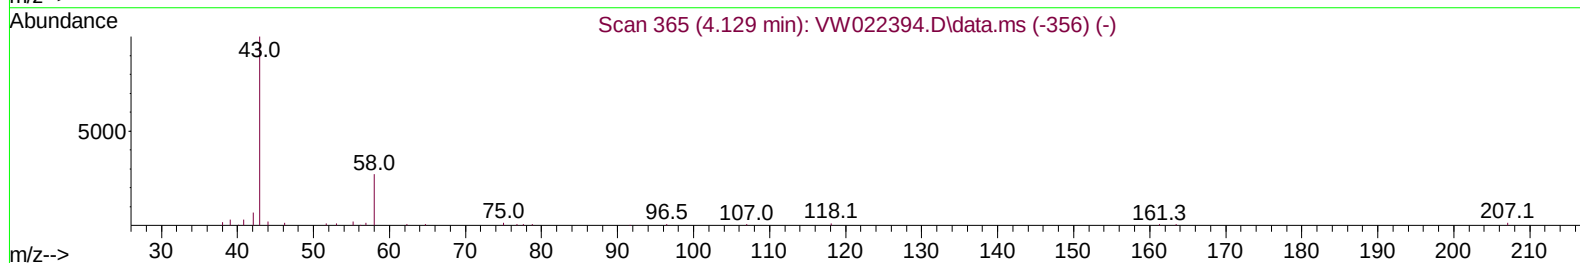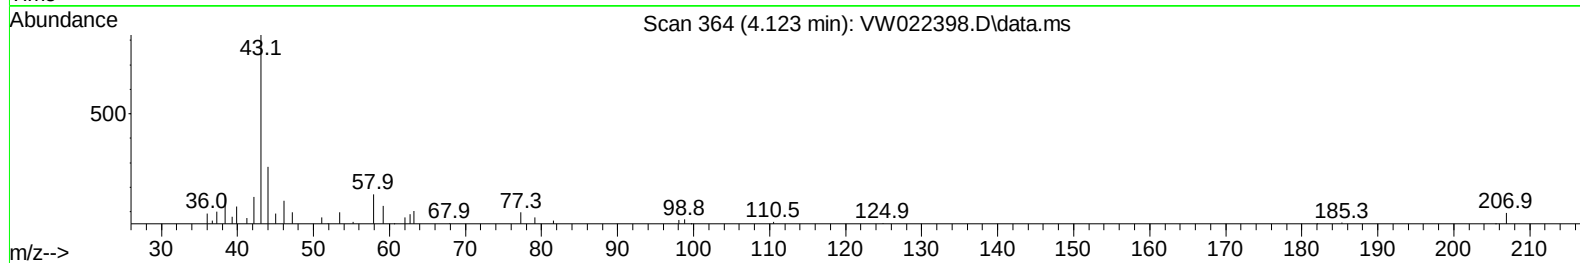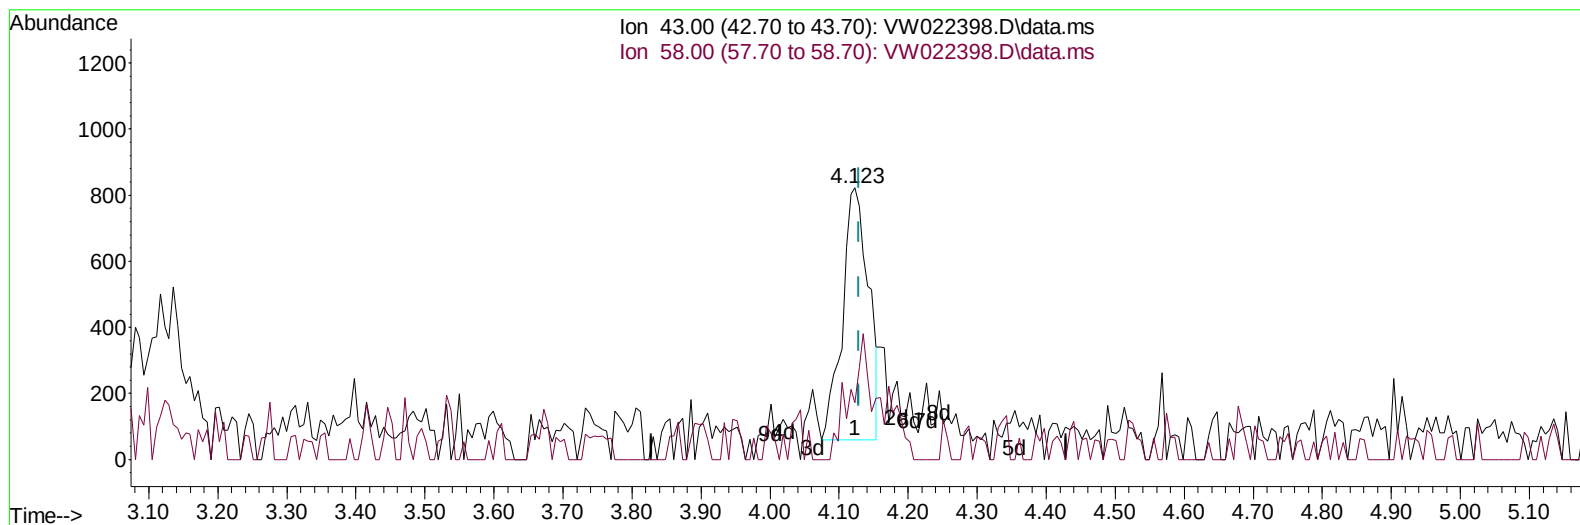

TIC: VW022398.D\data.ms

(13) Acetone (T)

4.123min (-0.006) 4.59 ug/L

response	1995	
Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	13.48
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
 Data File : VW022398.D
 Acq On : 05 Apr 2022 16:39
 Operator : SY/VA
 Sample : N2262-01
 Misc : 6.07g/10mL/MSVOA_W/SoIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6K7

Manual IntegrationsAPPROVED

Quant Time: Apr 06 02:14:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 06 02:13:06 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/06/2022
 Supervised By :Mahesh Dadoda 04/07/2022

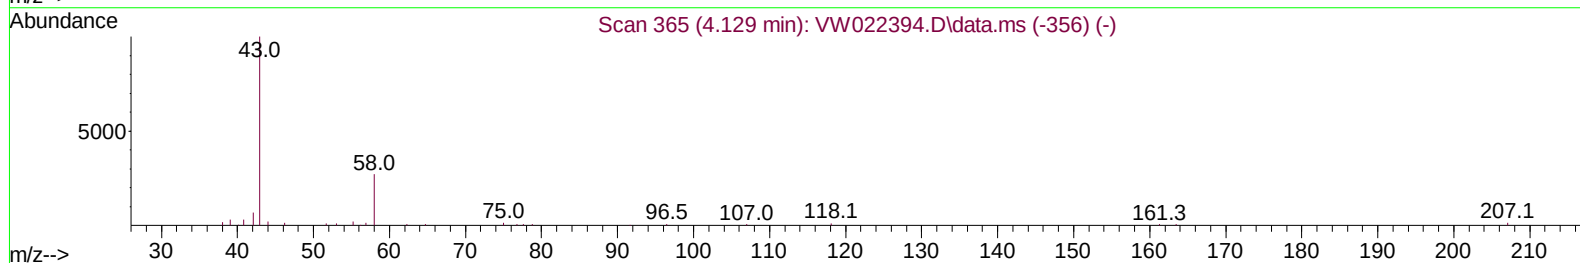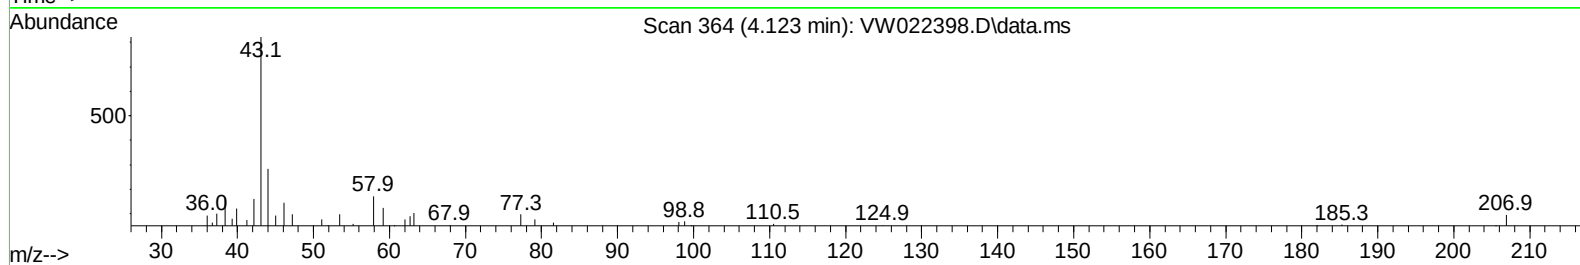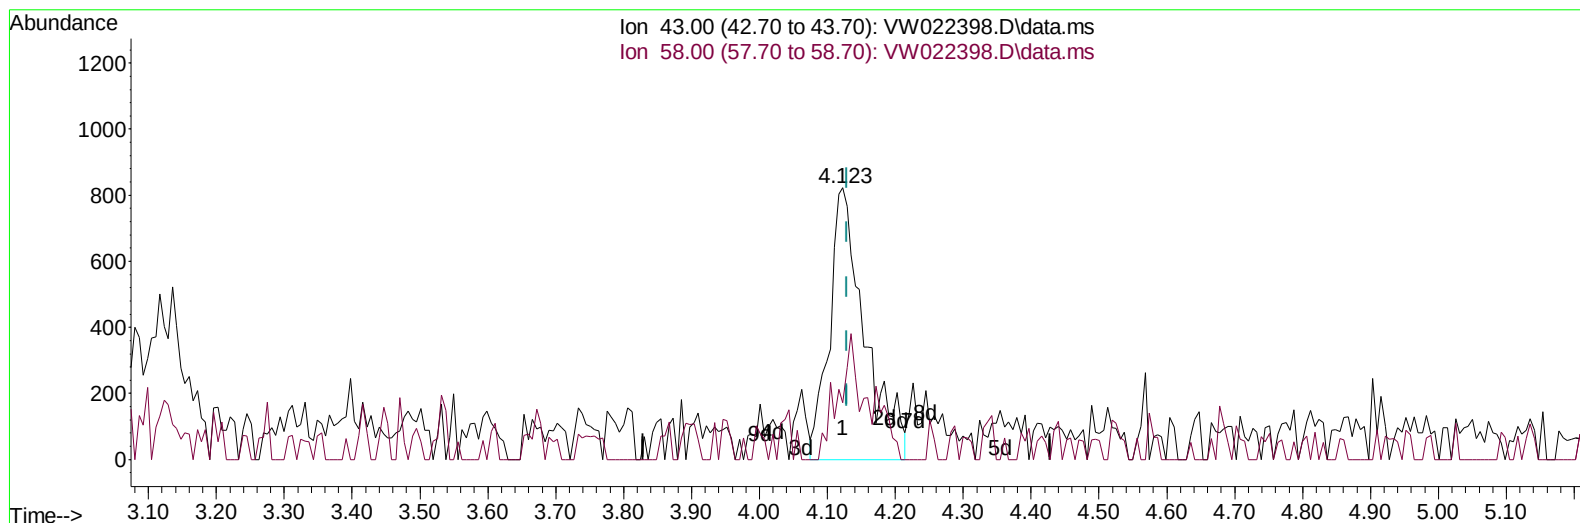

TIC: VW022398.D\data.ms

(13) Acetone (T)

4.123min (-0.006) 6.82 ug/L m

response 2964

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	9.08
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
 Data File : VW022398.D
 Acq On : 05 Apr 2022 16:39
 Operator : SY/VA
 Sample : N2262-01
 Misc : 6.07g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6K7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/06/2022
 Supervised By :Mahesh Dadoda 04/07/2022

Quant Time: Apr 06 02:14:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 06 02:13:06 2022
 Response via : Initial Calibration

Compound		R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards								
1) 1,4-Difluorobenzene		8.842	114		158458	25.000	ug/L	0.00
28) Chlorobenzene-d5		11.628	117		161526	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.554	152		80629	25.000	ug/L	0.00
System Monitoring Compounds								
4) Vinyl Chloride-d3		2.355	65		85398	32.884	ug/L	0.00
Spiked Amount	25.000	Range	30	- 150	Recovery	=	131.520%	
7) Chloroethane-d5		2.885	69		59759	38.545	ug/L	0.00
Spiked Amount	25.000	Range	30	- 150	Recovery	=	154.200%#	
11) 1,1-Dichloroethene-d2		4.013	63		67471	17.510	ug/L	-0.01
Spiked Amount	25.000	Range	45	- 110	Recovery	=	70.040%	
21) 2-Butanone-d5		7.074	46		37574	59.212	ug/L	0.00
Spiked Amount	50.000	Range	20	- 135	Recovery	=	118.420%	
24) Chloroform-d		7.647	84		106476	24.099	ug/L	0.00
Spiked Amount	25.000	Range	40	- 150	Recovery	=	96.400%	
26) 1,2-Dichloroethane-d4		8.305	65		68265	26.130	ug/L	0.00
Spiked Amount	25.000	Range	70	- 130	Recovery	=	104.520%	
32) Benzene-d6		8.275	84		218707	24.657	ug/L	0.00
Spiked Amount	25.000	Range	20	- 135	Recovery	=	98.640%	
36) 1,2-Dichloropropane-d6		9.274	67		64129	24.082	ug/L	0.00
Spiked Amount	25.000	Range	70	- 120	Recovery	=	96.320%	
41) Toluene-d8		10.323	98		218288	25.867	ug/L	0.00
Spiked Amount	25.000	Range	30	- 130	Recovery	=	103.480%	
43) trans-1,3-Dichloroprop...		10.573	79		30650	22.889	ug/L	0.00
Spiked Amount	25.000	Range	30	- 135	Recovery	=	91.560%	
47) 2-Hexanone-d5		10.921	63		31165	57.132	ug/L	0.00
Spiked Amount	50.000	Range	20	- 135	Recovery	=	114.260%	
56) 1,1,2,2-Tetrachloroeth...		12.689	84		61612	27.426	ug/L	0.00
Spiked Amount	25.000	Range	45	- 120	Recovery	=	109.720%	
66) 1,2-Dichlorobenzene-d4		13.853	152		71849	27.604	ug/L	0.00
Spiked Amount	25.000	Range	75	- 120	Recovery	=	110.400%	
Target Compounds								
13) Acetone		4.123	43		2964m	6.821	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
Data File : VW022398.D
Acq On : 05 Apr 2022 16:39
Operator : SY/VA
Sample : N2262-01
Misc : 6.07g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW6K7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/06/2022
Supervised By :Mahesh Dadoda 04/07/2022

Quant Time: Apr 06 02:14:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 06 02:13:06 2022
Response via : Initial Calibration

