




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
 Data File : VW022402.D
 Acq On : 05 Apr 2022 18:15
 Operator : SY/VA
 Sample : N2262-05
 Misc : 4.14g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6K9

Manual IntegrationsAPPROVED

Quant Time: Apr 06 02:15:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 06 02:13:06 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/06/2022
 Supervised By :Mahesh Dadoda 04/07/2022

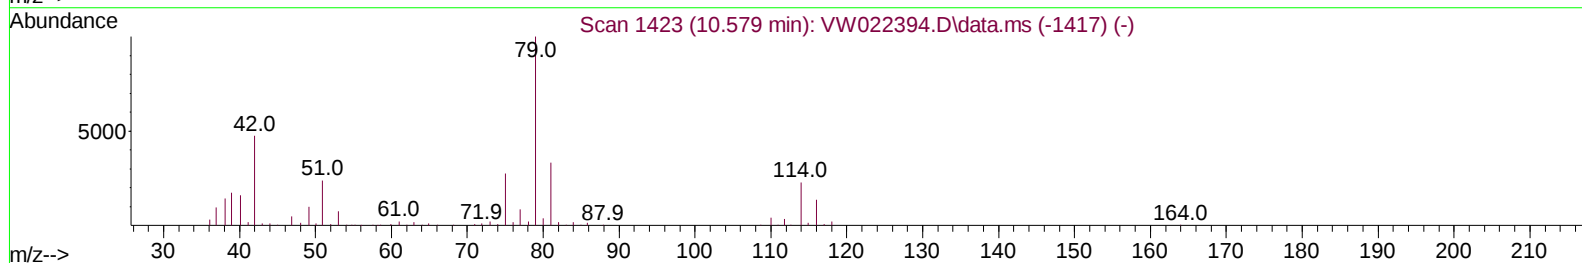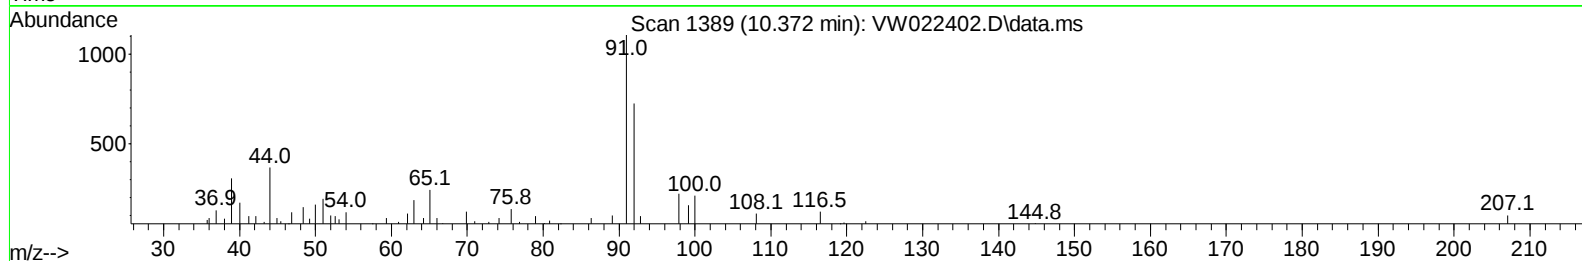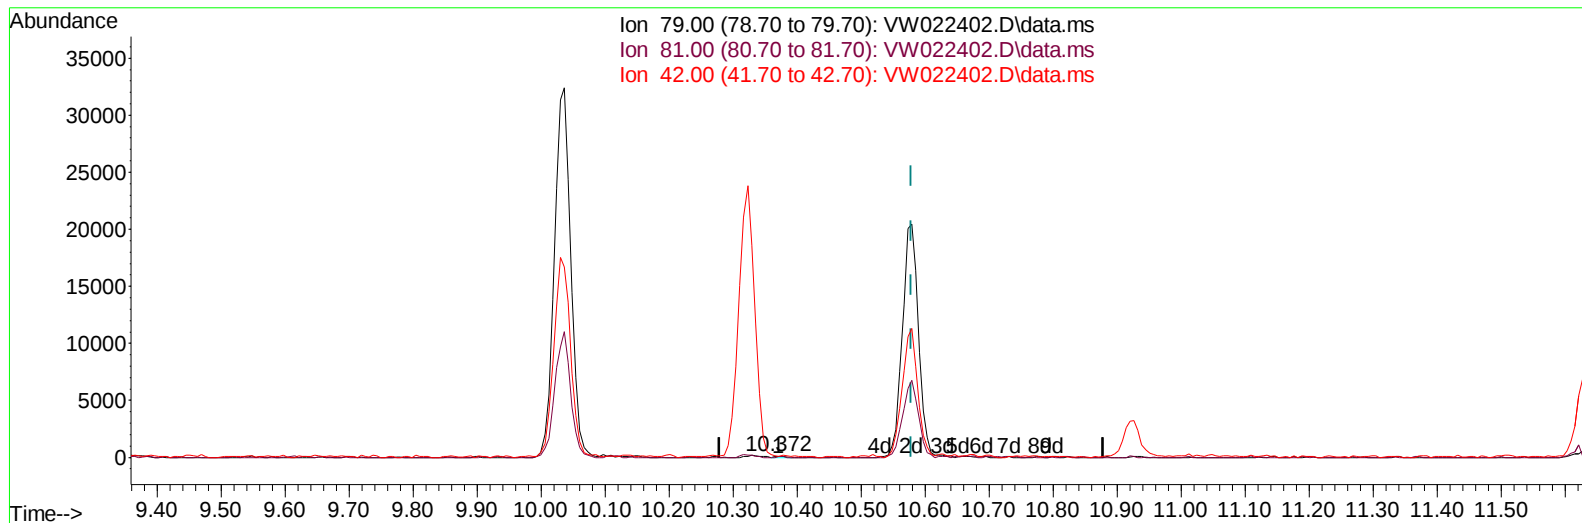

TIC: VW022402.D\data.ms

(43) trans-1,3-Dichloropropene-d4 (S)

10.372min (-0.207) 0.07 ug/L

response 109

Ion	Exp%	Act%
79.00	100.00	100.00
81.00	35.10	44.95
42.00	40.20	49.54
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
 Data File : VW022402.D
 Acq On : 05 Apr 2022 18:15
 Operator : SY/VA
 Sample : N2262-05
 Misc : 4.14g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6K9

Manual IntegrationsAPPROVED

Quant Time: Apr 06 02:15:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 06 02:13:06 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/06/2022
 Supervised By :Mahesh Dadoda 04/07/2022

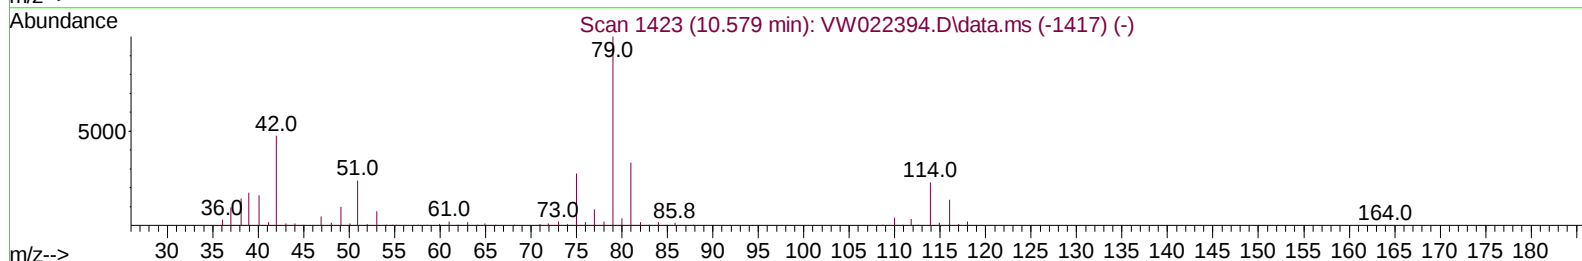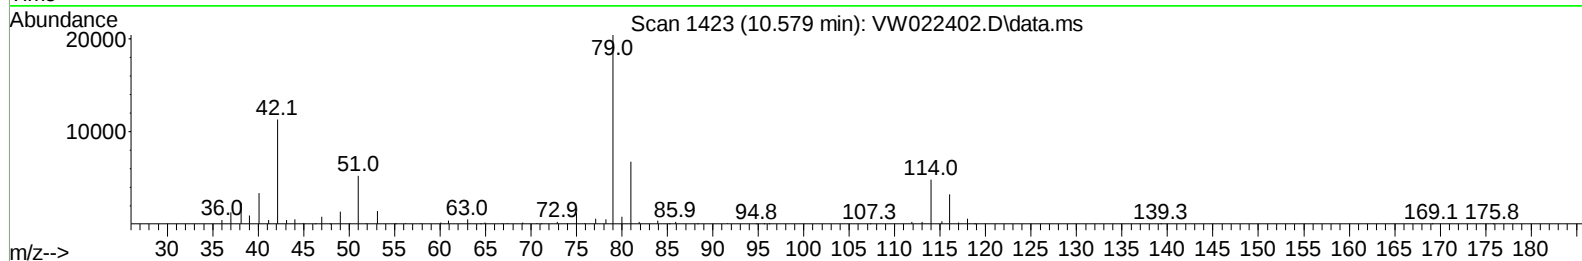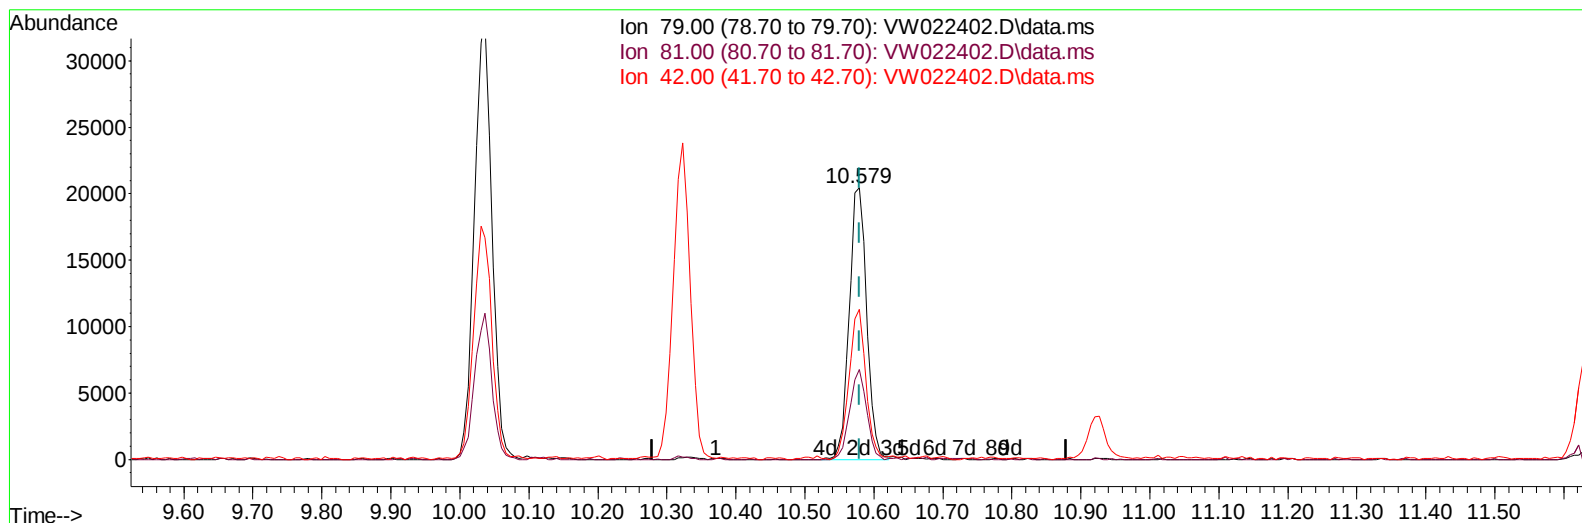

TIC: VW022402.D\data.ms

(43) trans-1,3-Dichloropropene-d4 (S)

10.579min (-0.000) 22.83 ug/L m

response 35742

Ion	Exp%	Act%
79.00	100.00	100.00
81.00	35.10	0.14#
42.00	40.20	0.15#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
 Data File : VW022402.D
 Acq On : 05 Apr 2022 18:15
 Operator : SY/VA
 Sample : N2262-05
 Misc : 4.14g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6K9

Manual IntegrationsAPPROVED

Quant Time: Apr 06 02:15:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 06 02:13:06 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/06/2022
 Supervised By :Mahesh Dadoda 04/07/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	185383	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	188828	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	94569	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	103334	34.011	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 136.040%			
7) Chloroethane-d5	2.891	69	76097	41.955	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 167.800%#			
11) 1,1-Dichloroethene-d2	4.019	63	77448	17.180	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 68.720%			
21) 2-Butanone-d5	7.080	46	37585	50.627	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 101.260%			
24) Chloroform-d	7.647	84	130441	25.235	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 100.960%			
26) 1,2-Dichloroethane-d4	8.305	65	81604	26.699	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 106.800%			
32) Benzene-d6	8.274	84	273993	26.424	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 105.680%			
36) 1,2-Dichloropropane-d6	9.274	67	77461	24.883	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 99.520%			
41) Toluene-d8	10.323	98	274652	27.841	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 111.360%			
43) trans-1,3-Dichloroprop...	10.579	79	35742m	22.832	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 91.320%			
47) 2-Hexanone-d5	10.920	63	31790	49.852	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 99.700%			
56) 1,1,2,2-Tetrachloroeth...	12.694	84	66889	25.470	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 101.880%			
66) 1,2-Dichlorobenzene-d4	13.853	152	86730	28.409	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 113.640%			

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
Data File : VW022402.D
Acq On : 05 Apr 2022 18:15
Operator : SY/VA
Sample : N2262-05
Misc : 4.14g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW6K9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/06/2022
Supervised By :Mahesh Dadoda 04/07/2022

Quant Time: Apr 06 02:15:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 06 02:13:06 2022
Response via : Initial Calibration

