




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
 Data File : VW022404.D
 Acq On : 05 Apr 2022 19:04
 Operator : SY/VA
 Sample : N2262-07
 Misc : 6.91g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6L1

Manual IntegrationsAPPROVED

Quant Time: Apr 06 02:15:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 06 02:13:06 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/06/2022
 Supervised By :Mahesh Dadoda 04/07/2022

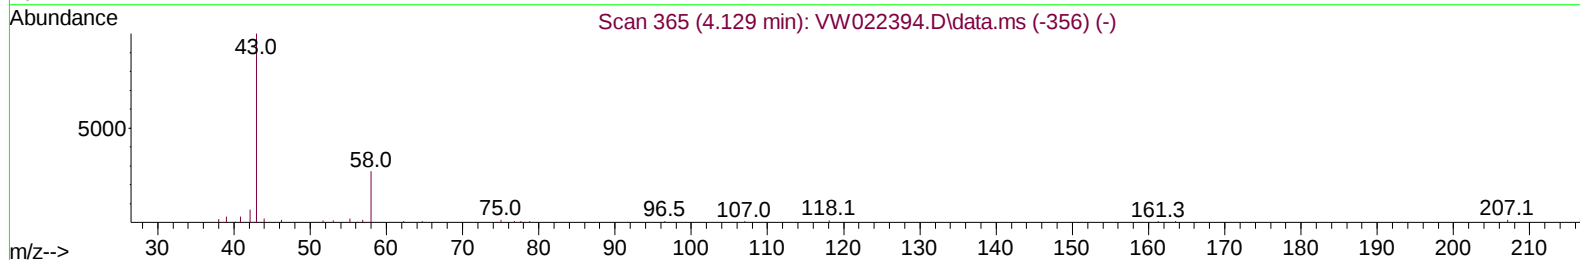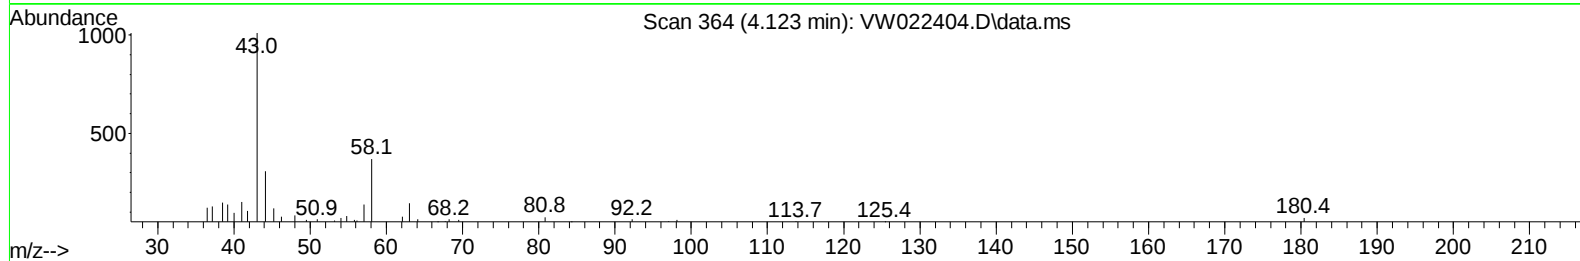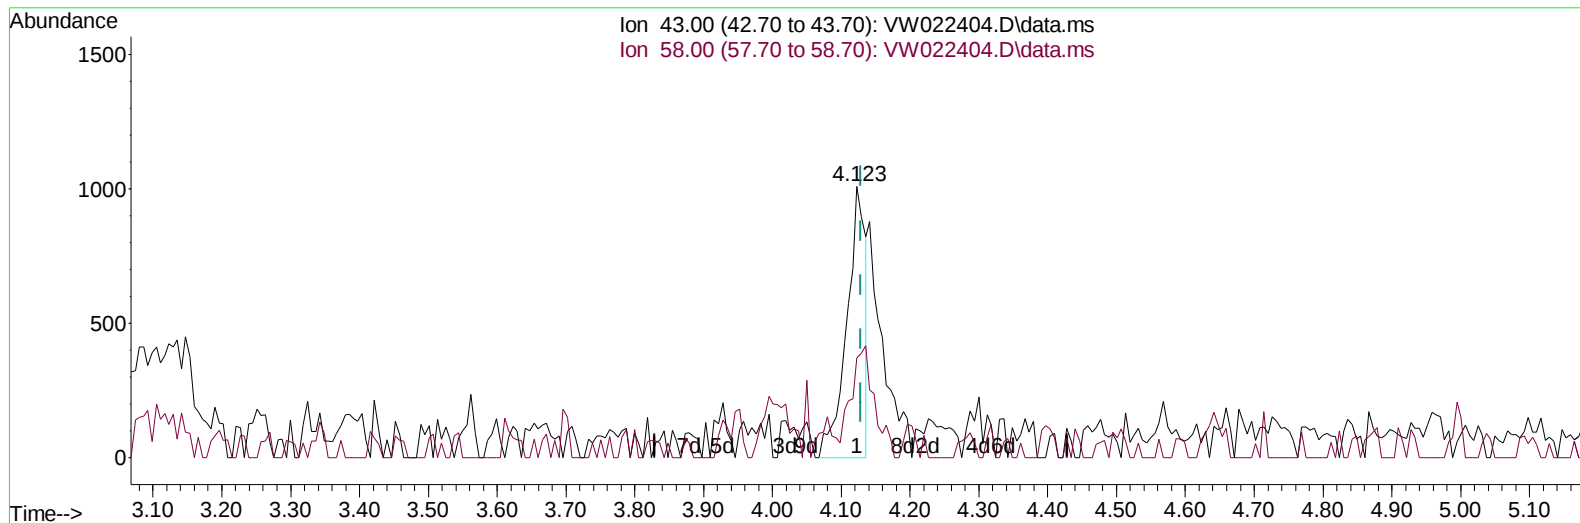

TIC: VW022404.D\data.ms

(13) Acetone (T)

4.123min (-0.006) 4.03 ug/L

response 1873

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	48.37
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
 Data File : VW022404.D
 Acq On : 05 Apr 2022 19:04
 Operator : SY/VA
 Sample : N2262-07
 Misc : 6.91g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6L1

Manual IntegrationsAPPROVED

Quant Time: Apr 06 02:15:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 06 02:13:06 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/06/2022
 Supervised By :Mahesh Dadoda 04/07/2022

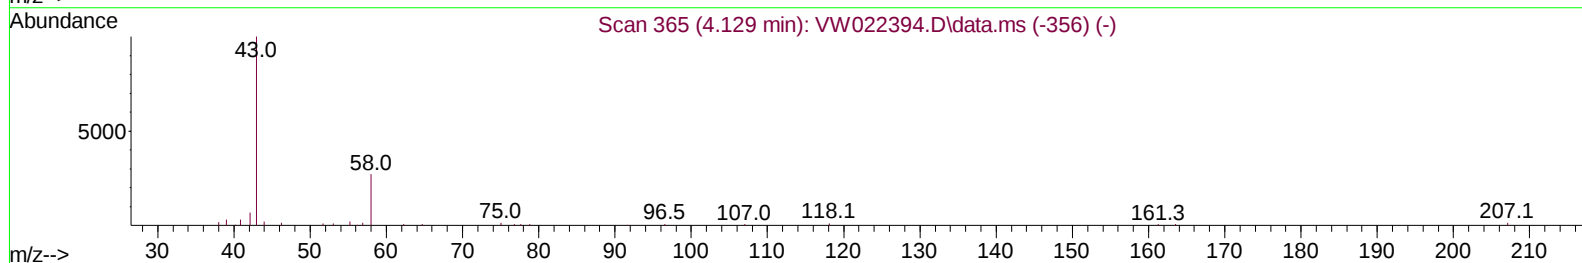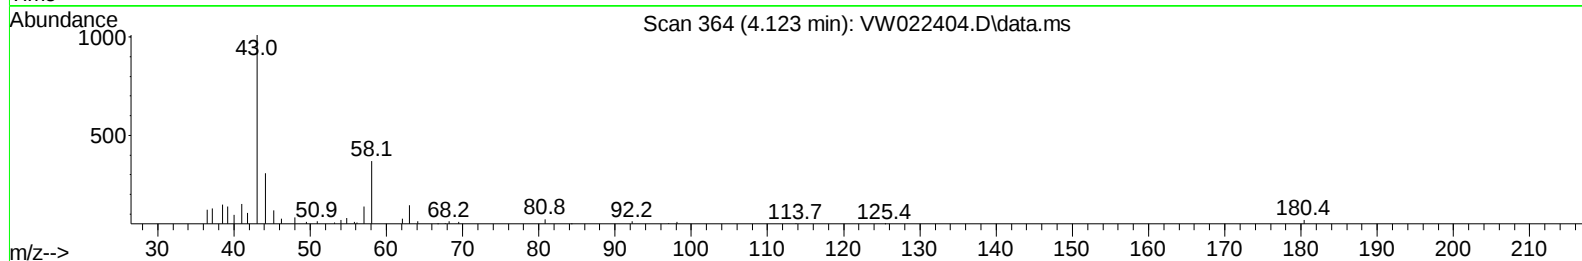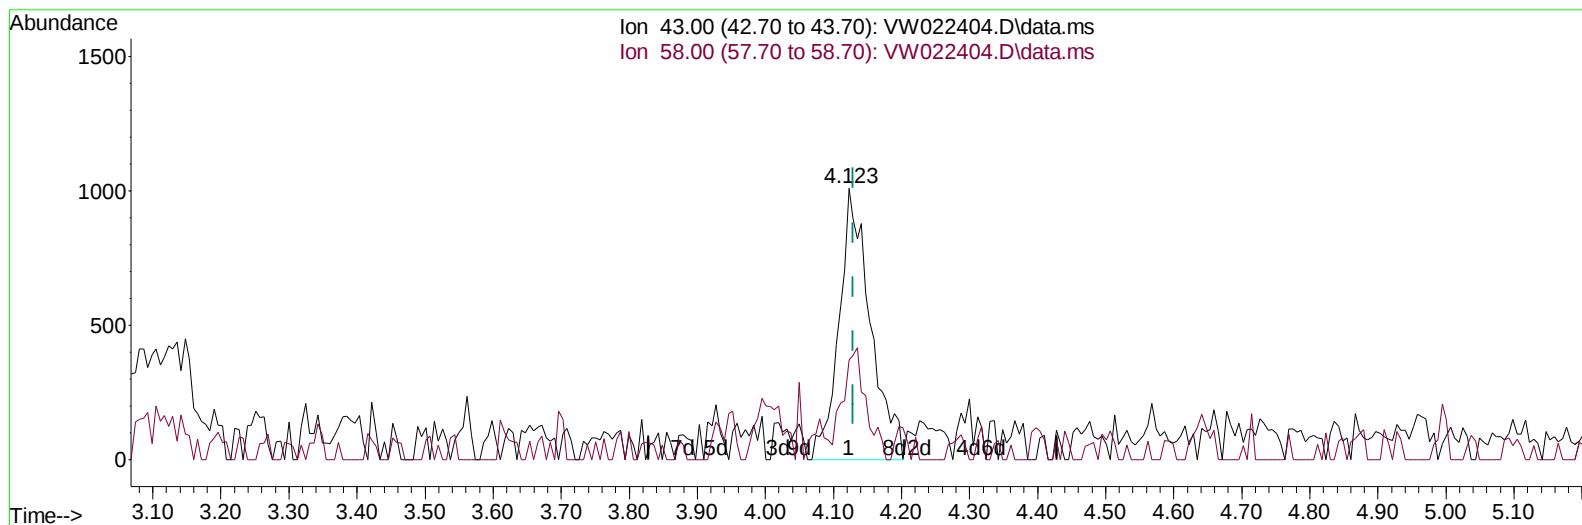

TIC: VW022404.D\data.ms

(13) Acetone (T)

4.123min (-0.006) 6.89 ug/L m

response 3206

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	28.26
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
 Data File : VW022404.D
 Acq On : 05 Apr 2022 19:04
 Operator : SY/VA
 Sample : N2262-07
 Misc : 6.91g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6L1

Manual IntegrationsAPPROVED

Quant Time: Apr 06 02:15:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 06 02:13:06 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/06/2022
 Supervised By :Mahesh Dadoda 04/07/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	169678	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	168949	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	73703	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	95495	34.340	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	137.360%	
7) Chloroethane-d5	2.885	69	69200	41.683	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	166.720%#	
11) 1,1-Dichloroethene-d2	4.013	63	68627	16.633	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	66.520%	
21) 2-Butanone-d5	7.080	46	33895	49.882	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	99.760%	
24) Chloroform-d	7.647	84	114186	24.135	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	96.560%	
26) 1,2-Dichloroethane-d4	8.305	65	72231	25.819	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	103.280%	
32) Benzene-d6	8.275	84	244102	26.311	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	105.240%	
36) 1,2-Dichloropropane-d6	9.274	67	70533	25.323	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	101.280%	
41) Toluene-d8	10.323	98	245004	27.758	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	111.040%	
43) trans-1,3-Dichloroprop...	10.579	79	30445	21.737	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	86.960%	
47) 2-Hexanone-d5	10.926	63	29829	52.281	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	104.560%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	58730	24.994	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	99.960%	
66) 1,2-Dichlorobenzene-d4	13.853	152	72507	30.474	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	121.880%#	
Target Compounds						
13) Acetone	4.123	43	3206m	6.890	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
Data File : VW022404.D
Acq On : 05 Apr 2022 19:04
Operator : SY/VA
Sample : N2262-07
Misc : 6.91g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW6L1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/06/2022
Supervised By :Mahesh Dadoda 04/07/2022

Quant Time: Apr 06 02:15:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 06 02:13:06 2022
Response via : Initial Calibration

