




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
 Data File : VW022405.D
 Acq On : 05 Apr 2022 19:28
 Operator : SY/VA
 Sample : N2262-08
 Misc : 6.70g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6L2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/06/2022
 Supervised By :Mahesh Dadoda 04/07/2022

Quant Time: Apr 06 02:16:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 06 02:13:06 2022
 Response via : Initial Calibration

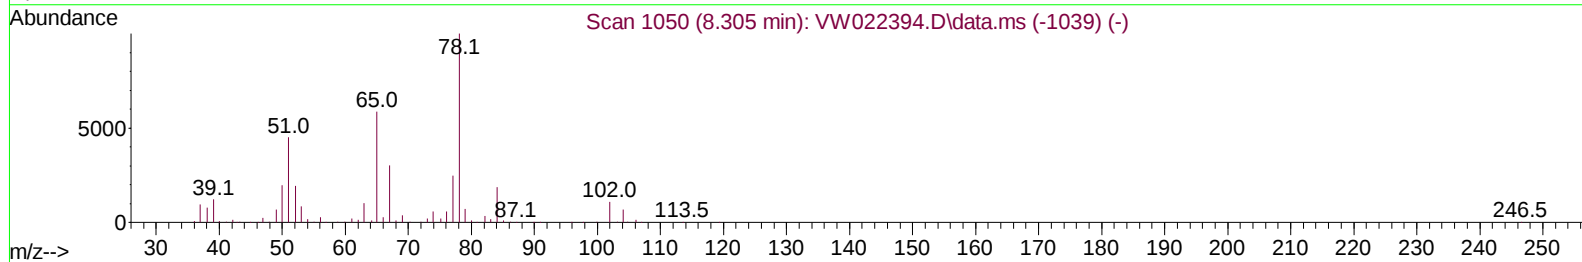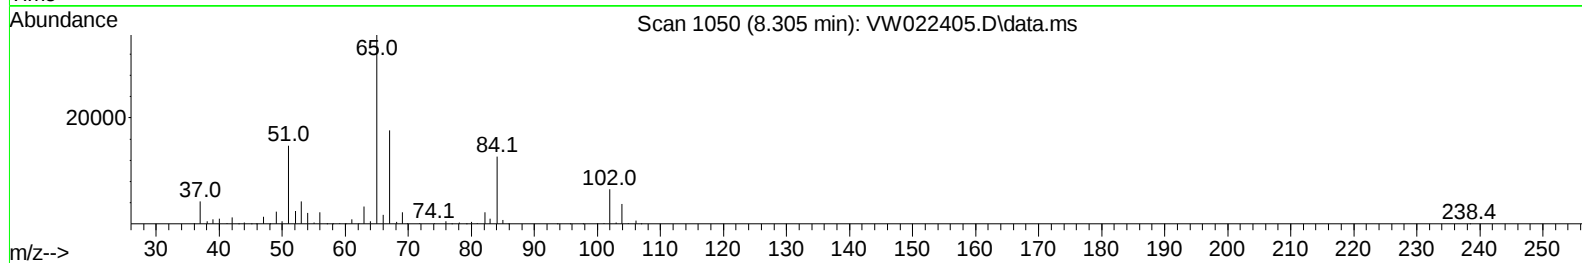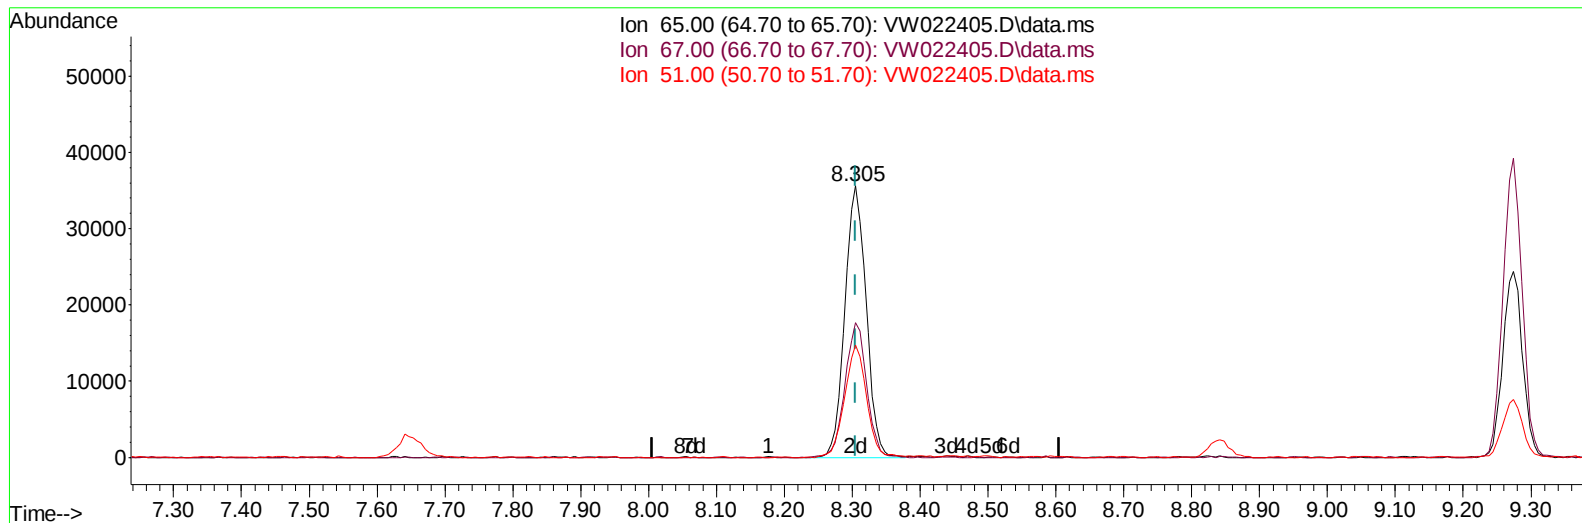

TIC: VW022405.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+ 0.000) 25.17 ug/L m

response 77344

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.50	0.06#
51.00	90.00	0.10#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
 Data File : VW022405.D
 Acq On : 05 Apr 2022 19:28
 Operator : SY/VA
 Sample : N2262-08
 Misc : 6.70g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6L2

Manual IntegrationsAPPROVED

Quant Time: Apr 06 02:16:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 06 02:13:06 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/06/2022
 Supervised By :Mahesh Dadoda 04/07/2022

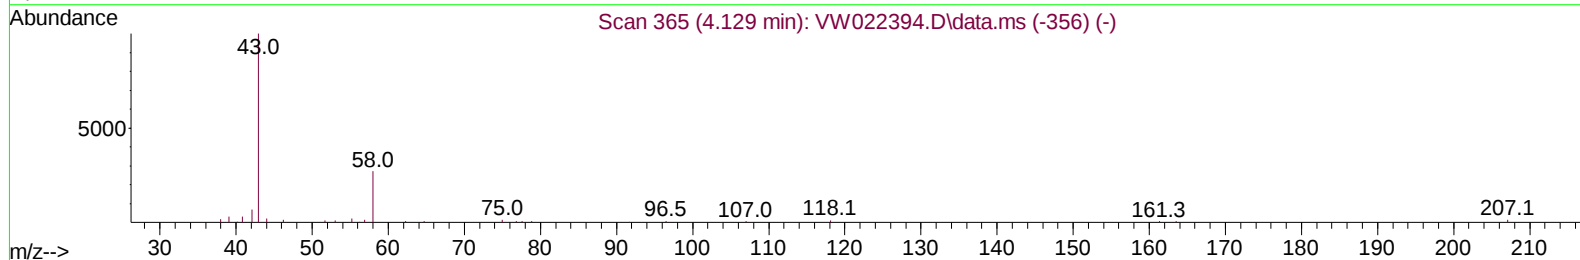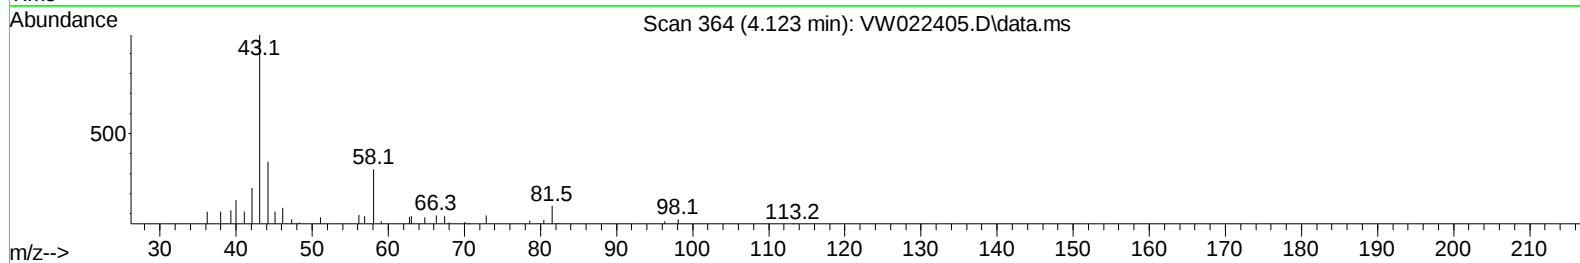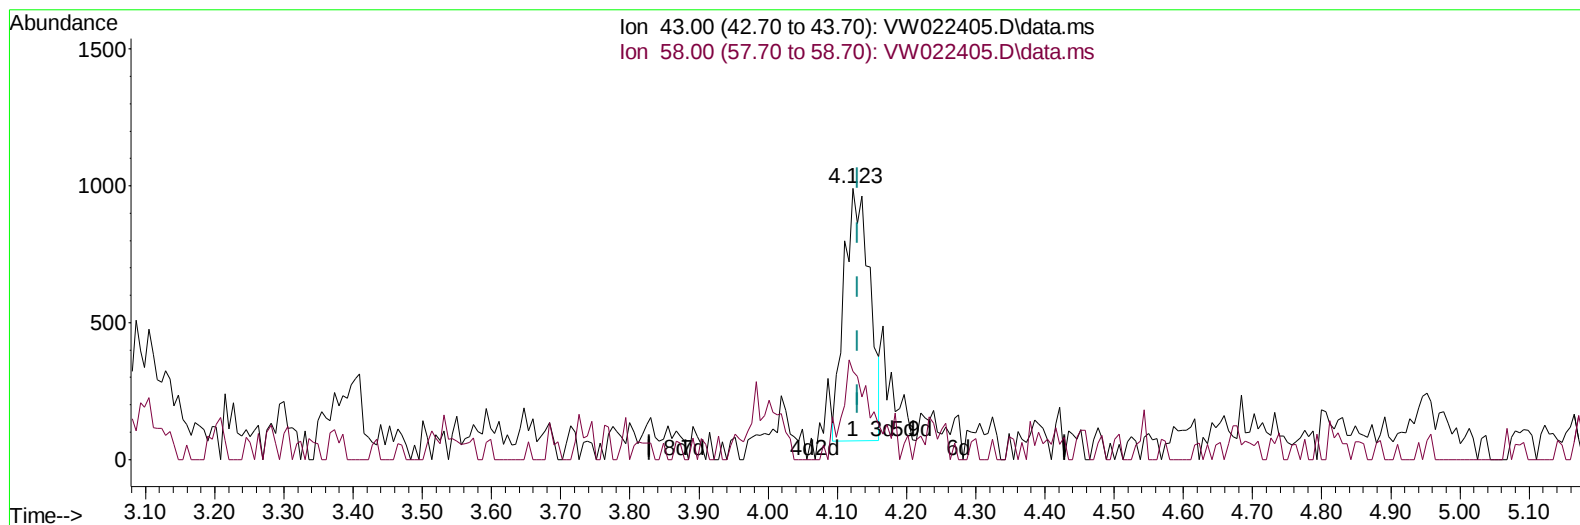

TIC: VW022405.D\data.ms

(13) Acetone (T)

4.123min (-0.006) 4.64 ug/L

response 2371

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	36.78
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
 Data File : VW022405.D
 Acq On : 05 Apr 2022 19:28
 Operator : SY/VA
 Sample : N2262-08
 Misc : 6.70g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6L2

Manual IntegrationsAPPROVED

Quant Time: Apr 06 02:16:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 06 02:13:06 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/06/2022
 Supervised By :Mahesh Dadoda 04/07/2022

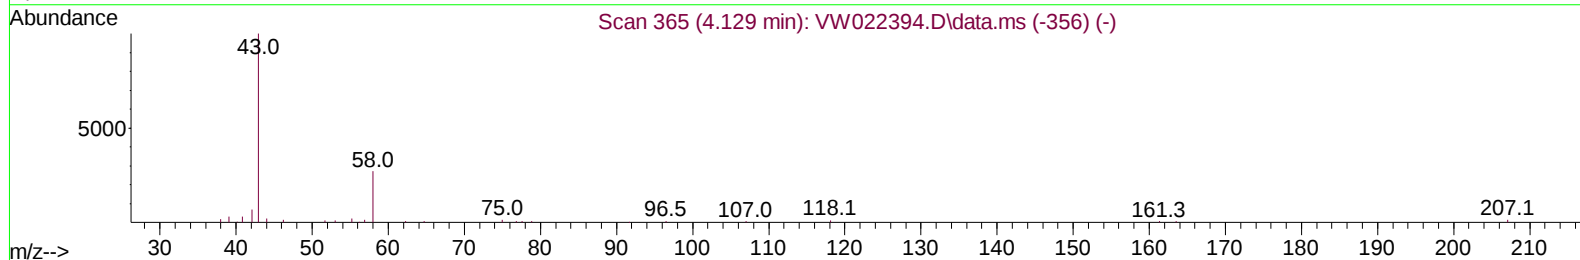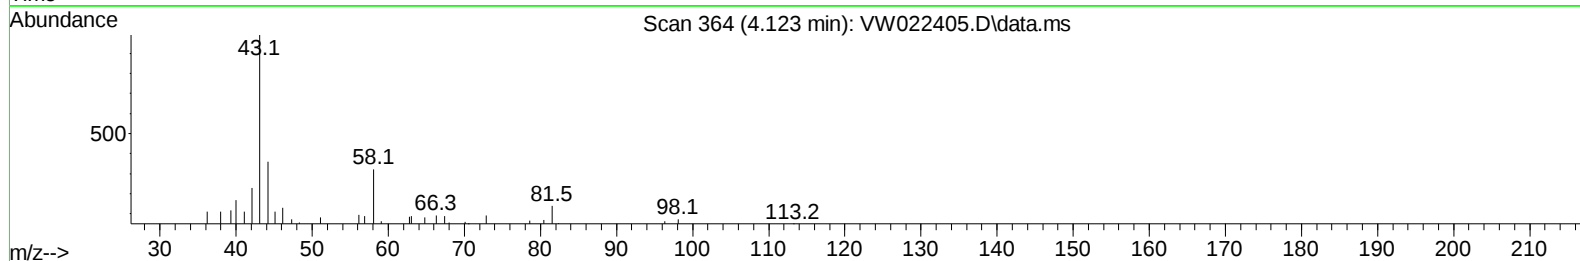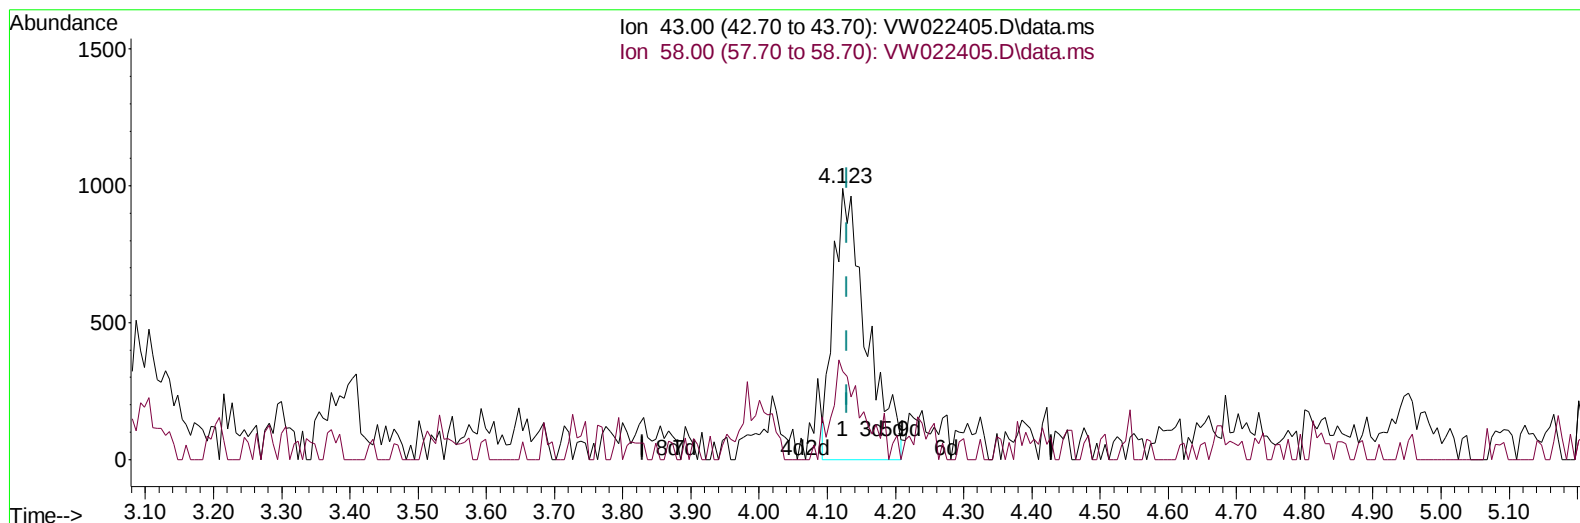

TIC: VW022405.D\data.ms

(13) Acetone (T)

4.123min (-0.006) 6.50 ug/L m

response 3322

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	26.25
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
 Data File : VW022405.D
 Acq On : 05 Apr 2022 19:28
 Operator : SY/VA
 Sample : N2262-08
 Misc : 6.70g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6L2

Manual IntegrationsAPPROVED

Quant Time: Apr 06 02:16:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 06 02:13:06 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/06/2022
 Supervised By :Mahesh Dadoda 04/07/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	186386	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	175857	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	78395	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	107247	35.109	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	140.440%	
7) Chloroethane-d5	2.885	69	77642	42.576	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	170.320%#	
11) 1,1-Dichloroethene-d2	4.019	63	76555	16.891	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	67.560%	
21) 2-Butanone-d5	7.074	46	34109	45.697	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	91.400%	
24) Chloroform-d	7.647	84	127008	24.439	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	97.760%	
26) 1,2-Dichloroethane-d4	8.305	65	77344m	25.169	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	100.680%	
32) Benzene-d6	8.275	84	268868	27.842	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	111.360%	
36) 1,2-Dichloropropane-d6	9.274	67	76707	26.458	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	105.840%	
41) Toluene-d8	10.323	98	267677	29.135	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	116.520%	
43) trans-1,3-Dichloroprop...	10.579	79	33109	22.710	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	90.840%	
47) 2-Hexanone-d5	10.920	63	29204	49.174	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	98.340%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	57256	23.410	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	93.640%	
66) 1,2-Dichlorobenzene-d4	13.853	152	70336	27.793	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	111.160%	
Target Compounds						Qvalue
13) Acetone	4.123	43	3322m	6.499	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
Data File : VW022405.D
Acq On : 05 Apr 2022 19:28
Operator : SY/VA
Sample : N2262-08
Misc : 6.70g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW6L2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/06/2022
Supervised By :Mahesh Dadoda 04/07/2022

Quant Time: Apr 06 02:16:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 06 02:13:06 2022
Response via : Initial Calibration

