




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
 Data File : VW022406.D
 Acq On : 05 Apr 2022 19:52
 Operator : SY/VA
 Sample : N2262-09
 Misc : 7.19g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6L3

Manual IntegrationsAPPROVED

Quant Time: Apr 06 02:16:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 06 02:13:06 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/06/2022
 Supervised By :Mahesh Dadoda 04/07/2022

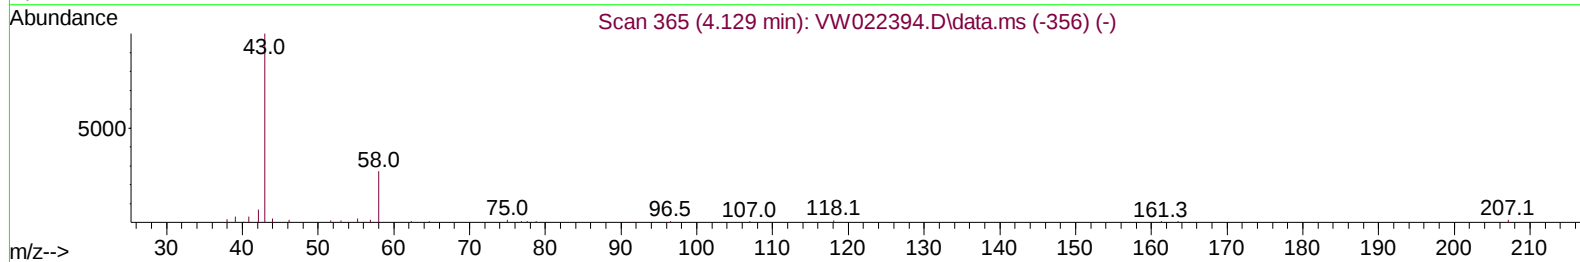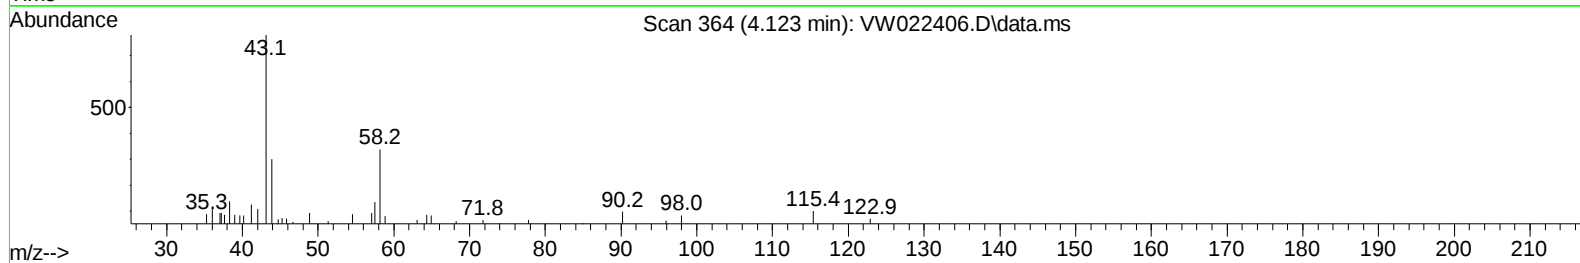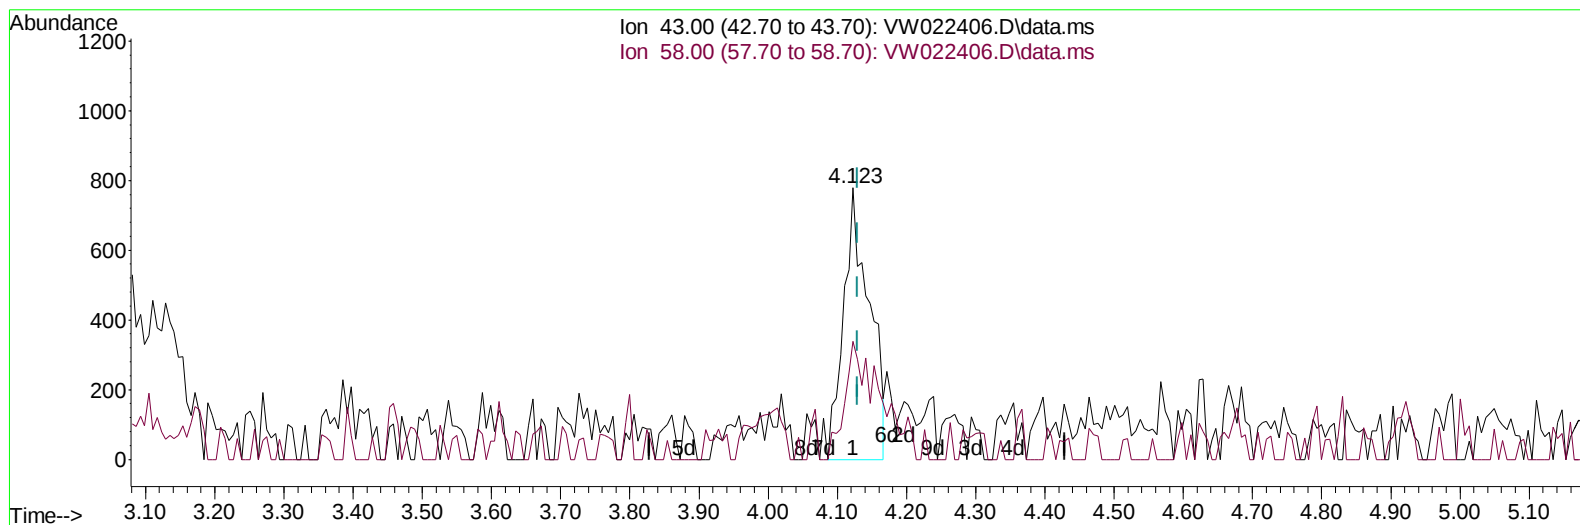

TIC: VW022406.D\data.ms

(13) Acetone (T)

4.123min (-0.006) 4.61 ug/L

response	1993	
Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	24.54
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
 Data File : VW022406.D
 Acq On : 05 Apr 2022 19:52
 Operator : SY/VA
 Sample : N2262-09
 Misc : 7.19g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6L3

Manual IntegrationsAPPROVED

Quant Time: Apr 06 02:16:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 06 02:13:06 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/06/2022
 Supervised By :Mahesh Dadoda 04/07/2022

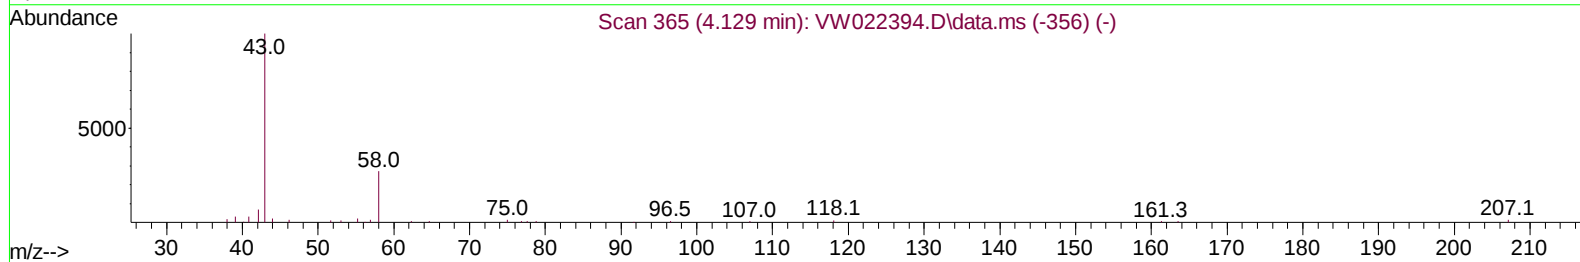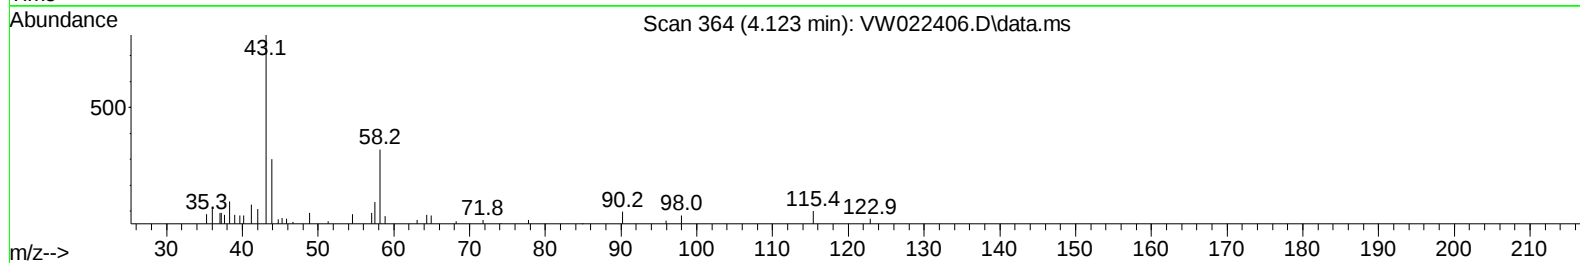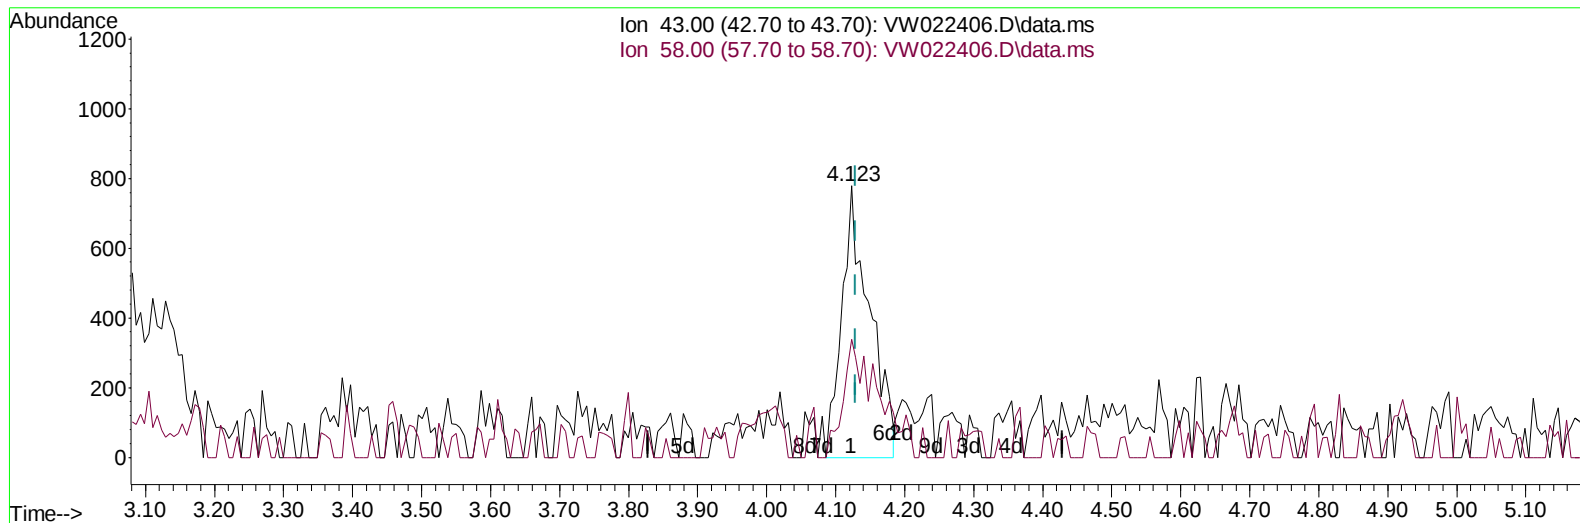

TIC: VW022406.D\data.ms

(13) Acetone (T)

4.123min (-0.006) 5.04 ug/L m

response 2182

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	22.41
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
 Data File : VW022406.D
 Acq On : 05 Apr 2022 19:52
 Operator : SY/VA
 Sample : N2262-09
 Misc : 7.19g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6L3

Manual IntegrationsAPPROVED

Quant Time: Apr 06 02:16:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 06 02:13:06 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/06/2022
 Supervised By :Mahesh Dadoda 04/07/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.841	114		157787	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		140919	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		55897	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		95934	37.098	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	148.400%	
7) Chloroethane-d5	2.885	69		69496	45.016	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	180.080%#	
11) 1,1-Dichloroethene-d2	4.019	63		65837	17.159	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	68.640%	
21) 2-Butanone-d5	7.074	46		30382	48.082	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	96.160%	
24) Chloroform-d	7.647	84		108086	24.568	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	98.280%	
26) 1,2-Dichloroethane-d4	8.305	65		65627	25.227	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	100.920%	
32) Benzene-d6	8.275	84		226140	29.223	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	116.880%	
36) 1,2-Dichloropropane-d6	9.274	67		66440	28.598	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	114.400%	
41) Toluene-d8	10.323	98		215309	29.245	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	117.000%	
43) trans-1,3-Dichloroprop...	10.579	79		25975	22.234	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	88.920%	
47) 2-Hexanone-d5	10.920	63		24449	51.375	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	102.740%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		50353	25.692	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	102.760%	
66) 1,2-Dichlorobenzene-d4	13.853	152		50597	28.040	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	112.160%	
Target Compounds							
13) Acetone	4.123	43		2182m	5.043	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
Data File : VW022406.D
Acq On : 05 Apr 2022 19:52
Operator : SY/VA
Sample : N2262-09
Misc : 7.19g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW6L3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/06/2022
Supervised By :Mahesh Dadoda 04/07/2022

Quant Time: Apr 06 02:16:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 06 02:13:06 2022
Response via : Initial Calibration

