




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
 Data File : VW022407.D
 Acq On : 05 Apr 2022 20:16
 Operator : SY/VA
 Sample : VIBLK411
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK411

Manual IntegrationsAPPROVED

Quant Time: Apr 06 02:16:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 06 02:13:06 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/06/2022
 Supervised By :Mahesh Dadoda 04/07/2022

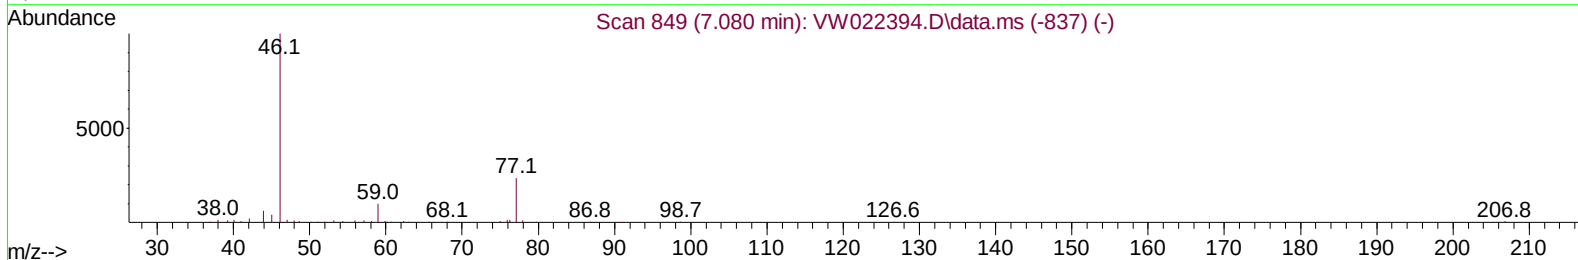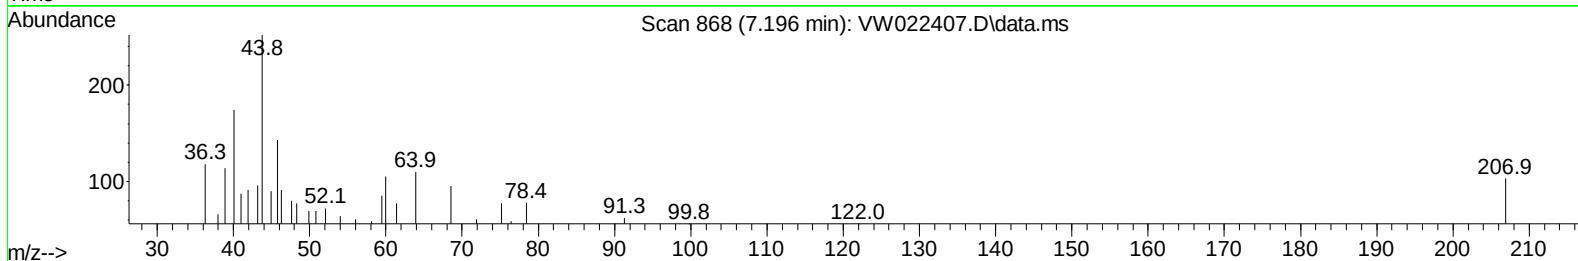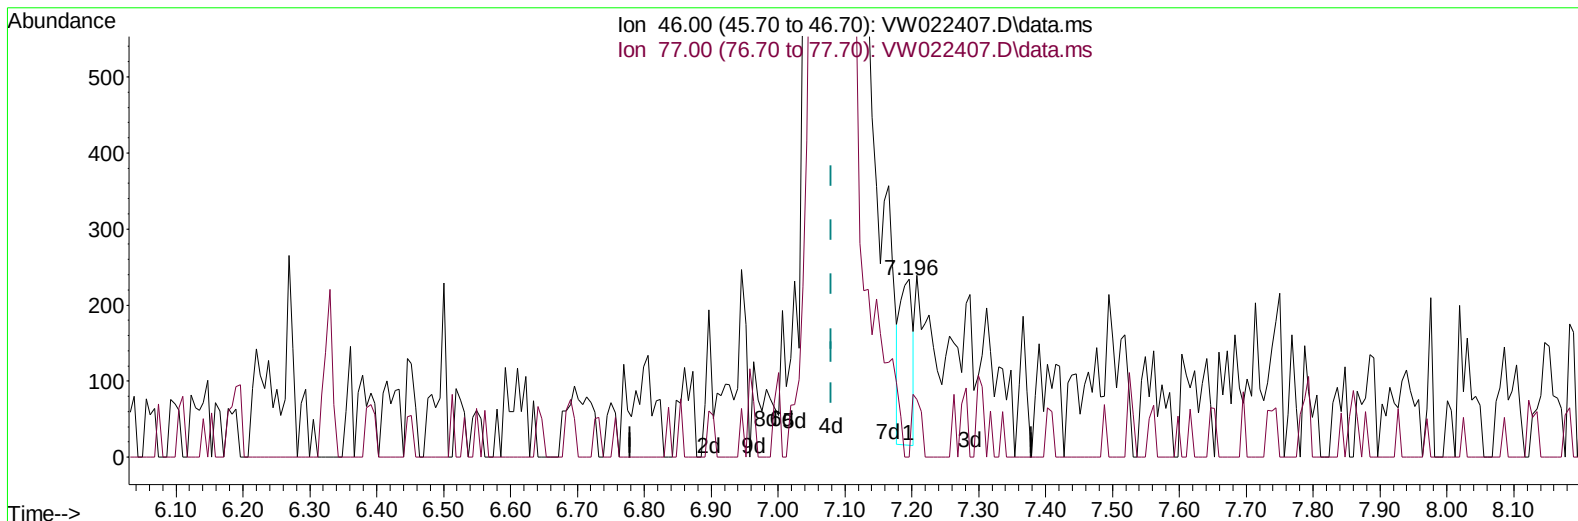

TIC: VW022407.D\data.ms

(21) 2-Butanone-d5 (S)

7.196min (+ 0.116) 0.43 ug/L

response	281	
Ion	Exp%	Act%
46.00	100.00	100.00
77.00	28.10	28.47
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
 Data File : VW022407.D
 Acq On : 05 Apr 2022 20:16
 Operator : SY/VA
 Sample : VIBLK411
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK411

Manual IntegrationsAPPROVED

Quant Time: Apr 06 02:16:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 06 02:13:06 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/06/2022
 Supervised By :Mahesh Dadoda 04/07/2022

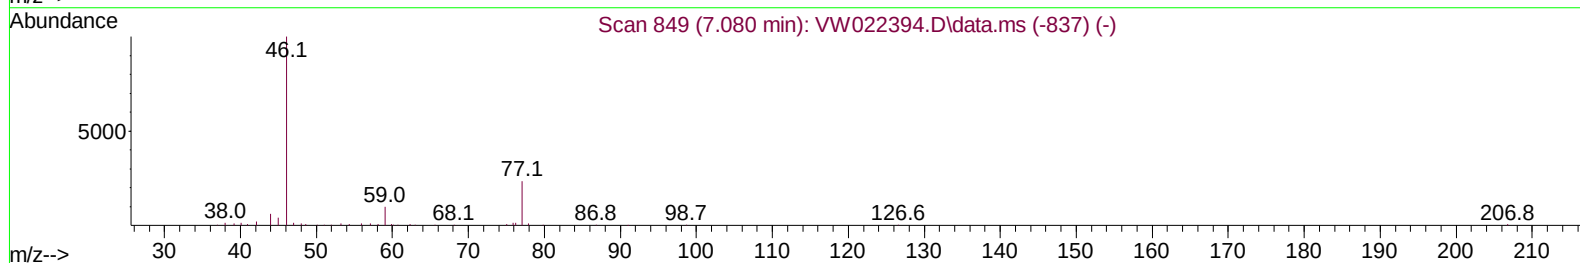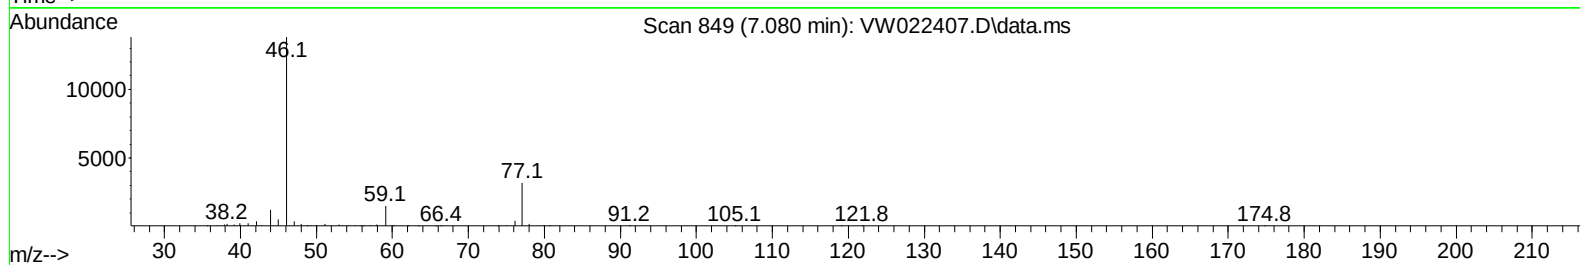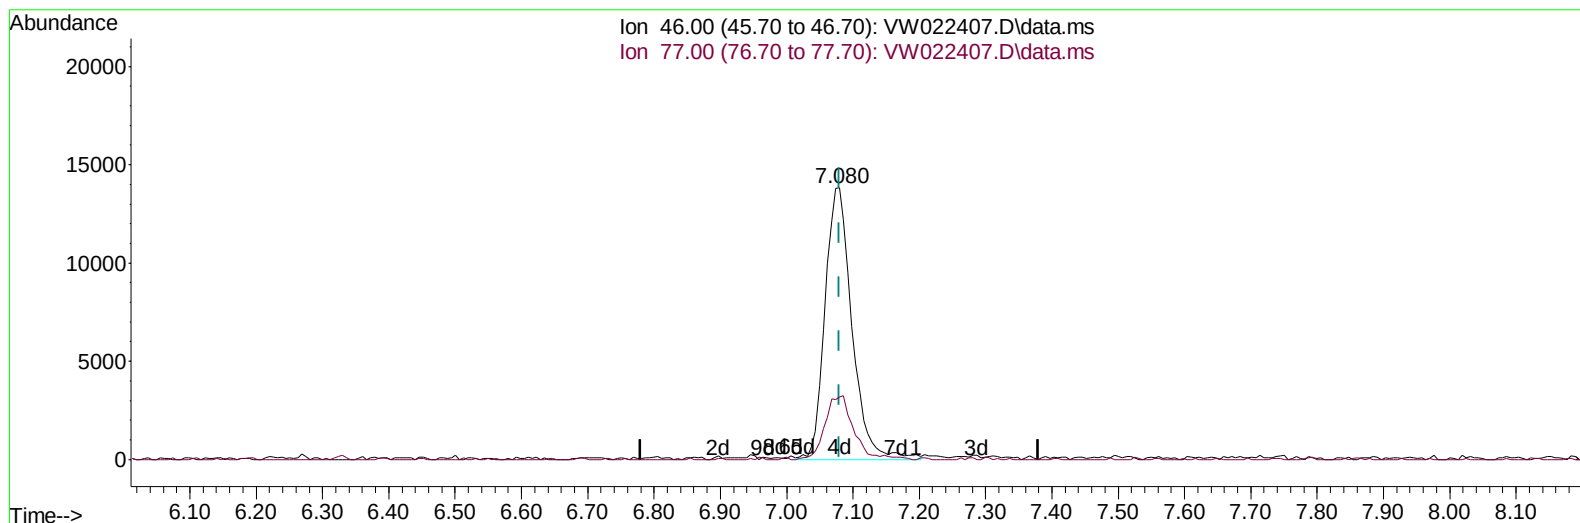

TIC: VW022407.D\data.ms

(21) 2-Butanone-d5 (S)

7.080min (+ 0.000) 60.54 ug/L m

response 39255

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	28.10	0.20#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
 Data File : VW022407.D
 Acq On : 05 Apr 2022 20:16
 Operator : SY/VA
 Sample : VIBLK411
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK411

Manual IntegrationsAPPROVED

Quant Time: Apr 06 02:16:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 06 02:13:06 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/06/2022
 Supervised By :Mahesh Dadoda 04/07/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	161924	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	161476	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	83099	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	98011	36.933	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	147.720%	
7) Chloroethane-d5	2.885	69	69828	44.076	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	176.320%#	
11) 1,1-Dichloroethene-d2	4.025	63	68507	17.399	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	69.600%	
21) 2-Butanone-d5	7.080	46	39255m	60.537	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	121.080%	
24) Chloroform-d	7.647	84	118499	26.246	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	105.000%	
26) 1,2-Dichloroethane-d4	8.305	65	75797	28.392	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	113.560%	
32) Benzene-d6	8.275	84	250528	28.253	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	113.000%	
36) 1,2-Dichloropropane-d6	9.274	67	73208	27.500	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	110.000%	
41) Toluene-d8	10.323	98	251474	29.809	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	119.240%	
43) trans-1,3-Dichloroprop...	10.579	79	33646	25.134	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	100.520%	
47) 2-Hexanone-d5	10.921	63	34076	62.488	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	124.980%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	66423	29.576	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	118.320%	
66) 1,2-Dichlorobenzene-d4	13.847	152	86191	32.130	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	128.520%#	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
Data File : VW022407.D
Acq On : 05 Apr 2022 20:16
Operator : SY/VA
Sample : VIBLK411
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK411

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/06/2022
Supervised By :Mahesh Dadoda 04/07/2022

Quant Time: Apr 06 02:16:25 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 06 02:13:06 2022
Response via : Initial Calibration

