

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
 Data File : VW022398.D
 Acq On : 05 Apr 2022 16:39
 Operator : SY/VA
 Sample : N2262-01
 Misc : 6.07g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6K7

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 04/06/2022
 Supervised By : Mahesh Dadoda 04/07/2022

Quant Time: Apr 06 02:14:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 06 02:13:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	158458	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	161526	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	80629	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	85398	32.884	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	131.520%
7) Chloroethane-d5	2.885	69	59759	38.545	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	154.200%#
11) 1,1-Dichloroethene-d2	4.013	63	67471	17.510	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	70.040%
21) 2-Butanone-d5	7.074	46	37574	59.212	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	118.420%
24) Chloroform-d	7.647	84	106476	24.099	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.400%
26) 1,2-Dichloroethane-d4	8.305	65	68265	26.130	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	104.520%
32) Benzene-d6	8.275	84	218707	24.657	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	98.640%
36) 1,2-Dichloropropane-d6	9.274	67	64129	24.082	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.320%
41) Toluene-d8	10.323	98	218288	25.867	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	103.480%
43) trans-1,3-Dichloroprop...	10.573	79	30650	22.889	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	91.560%
47) 2-Hexanone-d5	10.921	63	31165	57.132	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	114.260%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	61612	27.426	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	109.720%
66) 1,2-Dichlorobenzene-d4	13.853	152	71849	27.604	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	110.400%
Target Compounds					Qvalue	
13) Acetone	4.123	43	2964m	6.821	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
Data File : VW022398.D
Acq On : 05 Apr 2022 16:39
Operator : SY/VA
Sample : N2262-01
Misc : 6.07g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EW6K7

Quant Time: Apr 06 02:14:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 06 02:13:06 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 04/06/2022
Supervised By :Mahesh Dadoda 04/07/2022

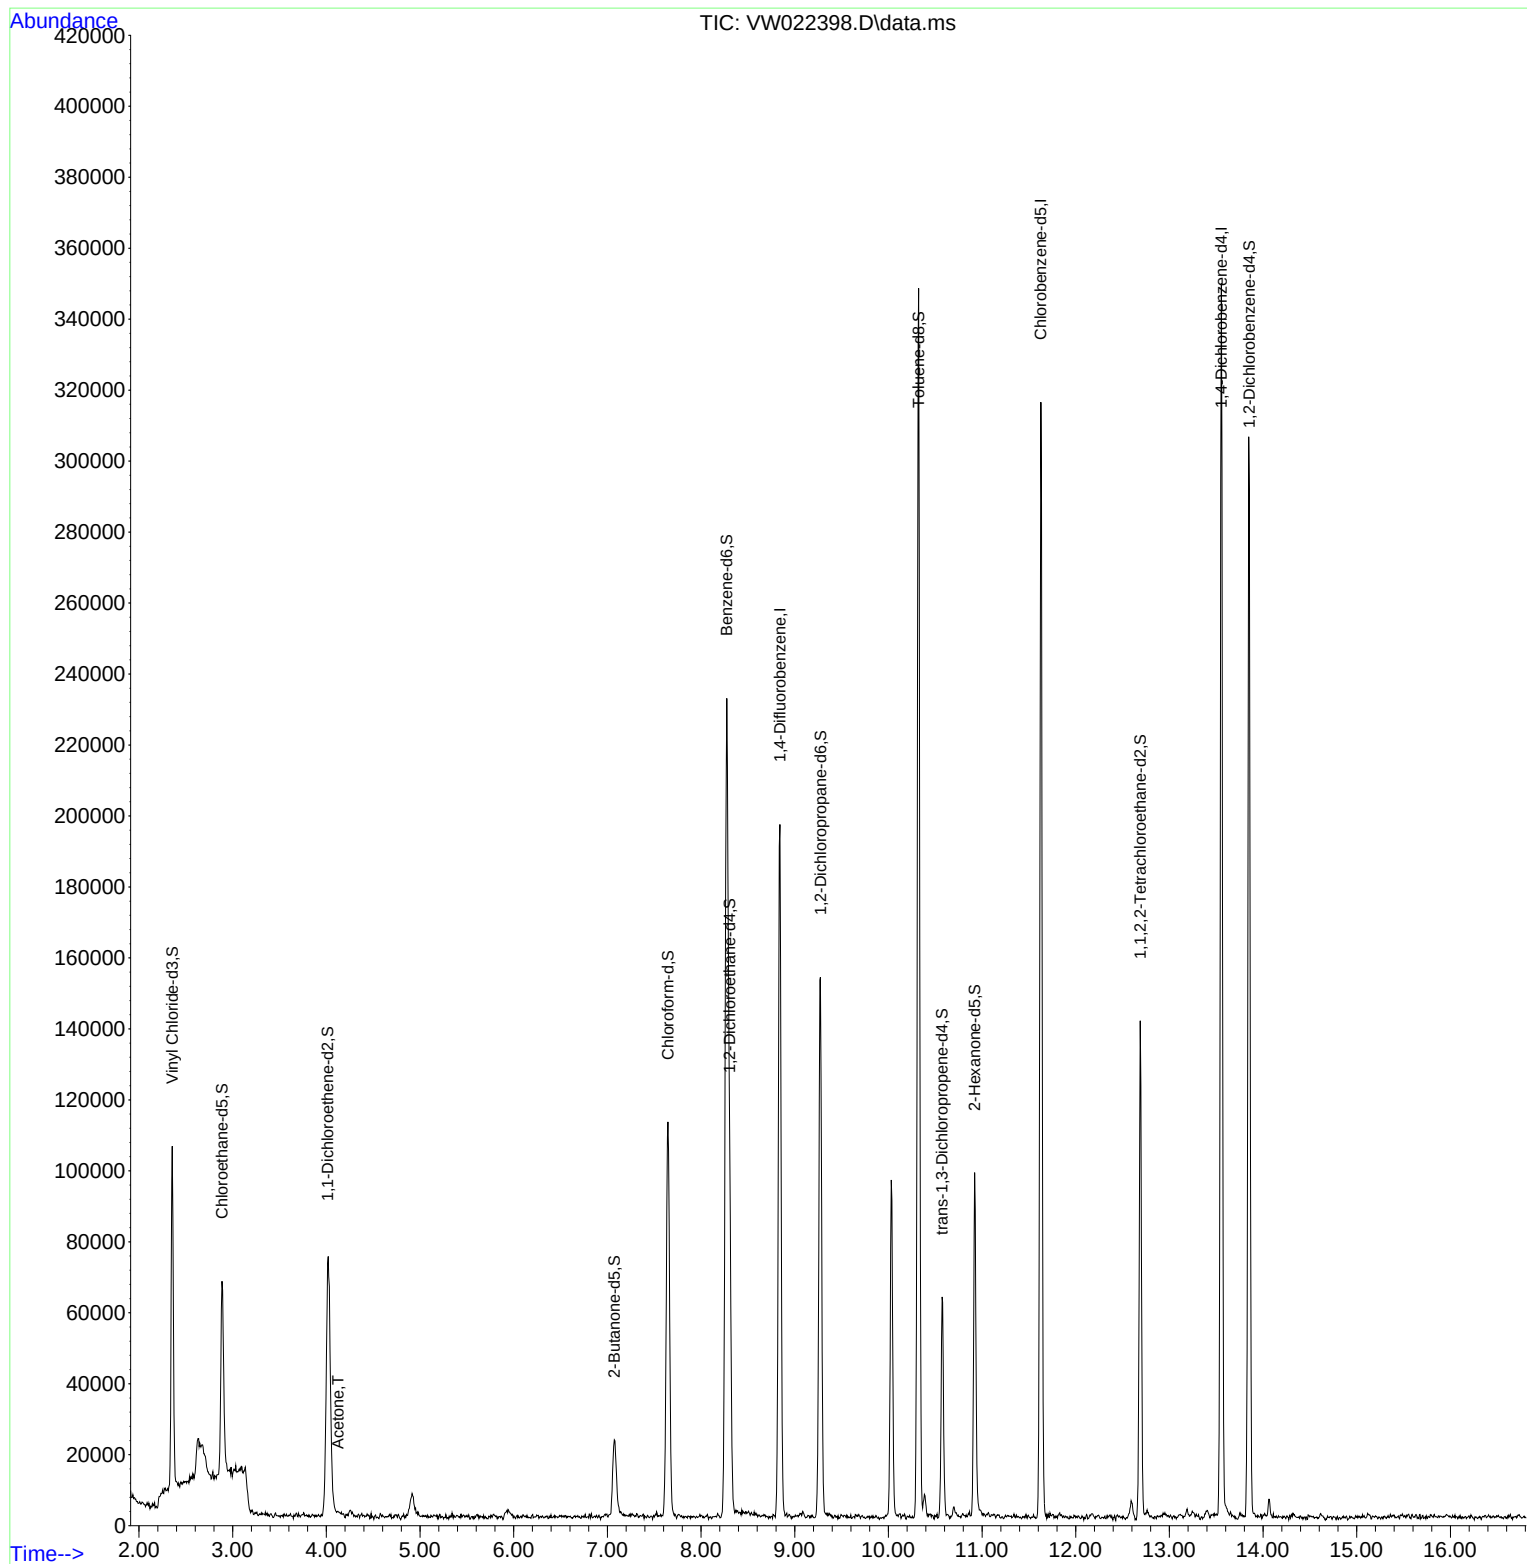

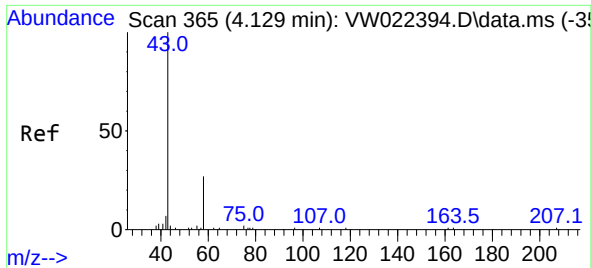

#13
Acetone
Concen: 6.821 ug/L m
RT: 4.123 min Scan# 30
Delta R.T. -0.006 min
Lab File: VW022398.D
Acq: 05 Apr 2022 16:39

Instrument :
MSVOA_W
ClientSampleId :
EW6K7

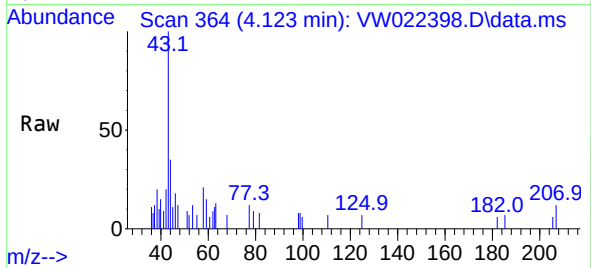

Tgt Ion: 43 Resp: 2964
Ion Ratio Lower Upper
43 100
58 9.1 0.0 69.2

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 04/06/2022
Supervised By :Mahesh Dadoda 04/07/2022

