

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
 Data File : VW022403.D
 Acq On : 05 Apr 2022 18:39
 Operator : SY/VA
 Sample : N2262-06
 Misc : 6.72g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6L0

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 04/06/2022
 Supervised By : Mahesh Dadoda 04/07/2022

Quant Time: Apr 06 02:15:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 06 02:13:06 2022
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene		8.842	114	148746	25.000	ug/L	0.00
28) Chlorobenzene-d5		11.628	117	141954	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.554	152	63899	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.355	65	86640	35.540	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	142.160%	
7) Chloroethane-d5		2.885	69	58616	40.277	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	161.120%#	
11) 1,1-Dichloroethene-d2		4.019	63	59859	16.549	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.200%	
21) 2-Butanone-d5		7.080	46	36992	62.101	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	124.200%	
24) Chloroform-d		7.647	84	104197	25.123	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	100.480%	
26) 1,2-Dichloroethane-d4		8.305	65	67228	27.413	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	109.640%	
32) Benzene-d6		8.275	84	215306	27.620	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	110.480%	
36) 1,2-Dichloropropane-d6		9.275	67	63607	27.179	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	108.720%	
41) Toluene-d8		10.323	98	211049	28.458	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	113.840%	
43) trans-1,3-Dichloroprop...		10.579	79	28054	23.838	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	95.360%	
47) 2-Hexanone-d5		10.921	63	30626	63.885	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	127.780%	
56) 1,1,2,2-Tetrachloroeth...		12.689	84	58279	29.519	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	118.080%	
66) 1,2-Dichlorobenzene-d4		13.853	152	60095	29.133	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	116.520%	
Target Compounds							Qvalue
13) Acetone		4.117	43	3694m	9.056	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
Data File : VW022403.D
Acq On : 05 Apr 2022 18:39
Operator : SY/VA
Sample : N2262-06
Misc : 6.72g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EW6L0

Quant Time: Apr 06 02:15:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 06 02:13:06 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : Semsettin Yesilyurt 04/06/2022
Supervised By : Mahesh Dadoda 04/07/2022

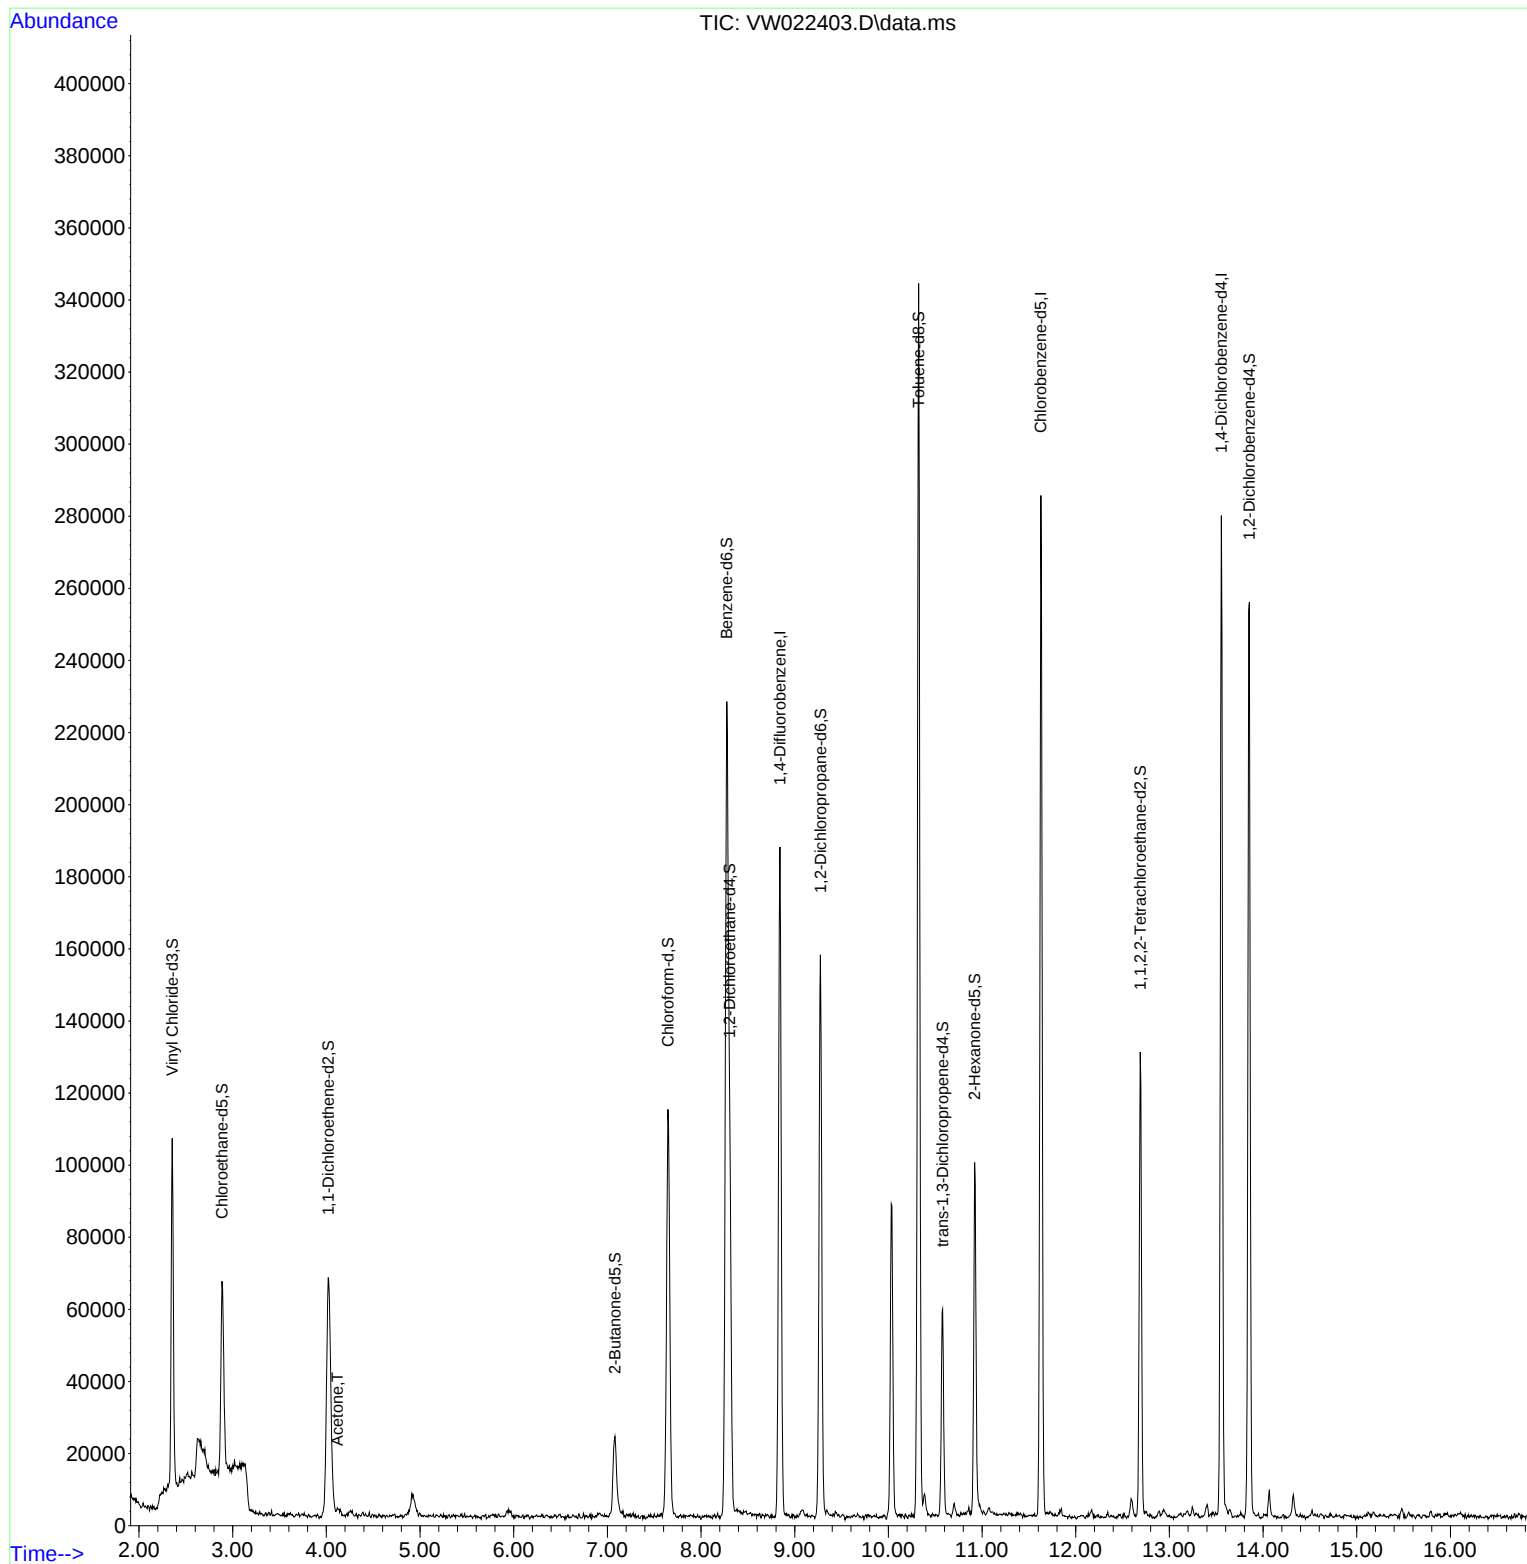

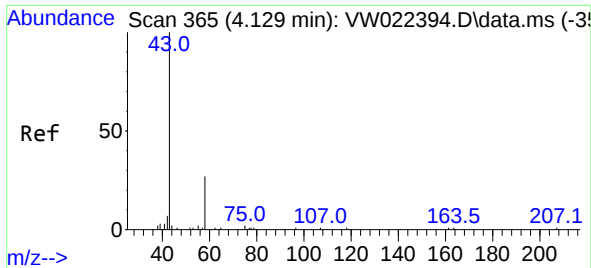

#13
Acetone
Concen: 9.056 ug/L m
RT: 4.117 min Scan# 30
Delta R.T. -0.012 min
Lab File: VW022403.D
Acq: 05 Apr 2022 18:39

Instrument :
MSVOA_W
ClientSampleId :
EW6L0

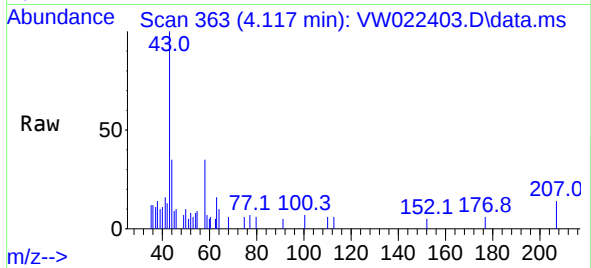

Tgt Ion: 43 Resp: 3694
Ion Ratio Lower Upper
43 100
58 9.3 0.0 69.2

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 04/06/2022
Supervised By :Mahesh Dadoda 04/07/2022

