

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
 Data File : VW022404.D
 Acq On : 05 Apr 2022 19:04
 Operator : SY/VA
 Sample : N2262-07
 Misc : 6.91g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6L1

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/06/2022
 Supervised By :Mahesh Dadoda 04/07/2022

Quant Time: Apr 06 02:15:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 06 02:13:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	169678	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	168949	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	73703	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	95495	34.340	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	137.360%
7) Chloroethane-d5	2.885	69	69200	41.683	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	166.720%#
11) 1,1-Dichloroethene-d2	4.013	63	68627	16.633	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.520%
21) 2-Butanone-d5	7.080	46	33895	49.882	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.760%
24) Chloroform-d	7.647	84	114186	24.135	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.560%
26) 1,2-Dichloroethane-d4	8.305	65	72231	25.819	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	103.280%
32) Benzene-d6	8.275	84	244102	26.311	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	105.240%
36) 1,2-Dichloropropane-d6	9.274	67	70533	25.323	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.280%
41) Toluene-d8	10.323	98	245004	27.758	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	111.040%
43) trans-1,3-Dichloroprop...	10.579	79	30445	21.737	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.960%
47) 2-Hexanone-d5	10.926	63	29829	52.281	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.560%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	58730	24.994	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	99.960%
66) 1,2-Dichlorobenzene-d4	13.853	152	72507	30.474	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	121.880%#
Target Compounds					Qvalue	
13) Acetone	4.123	43	3206m	6.890	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
Data File : VW022404.D
Acq On : 05 Apr 2022 19:04
Operator : SY/VA
Sample : N2262-07
Misc : 6.91g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EW6L1

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 04/06/2022
Supervised By :Mahesh Dadoda 04/07/2022


Quant Time: Apr 06 02:15:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 06 02:13:06 2022
Response via : Initial Calibration

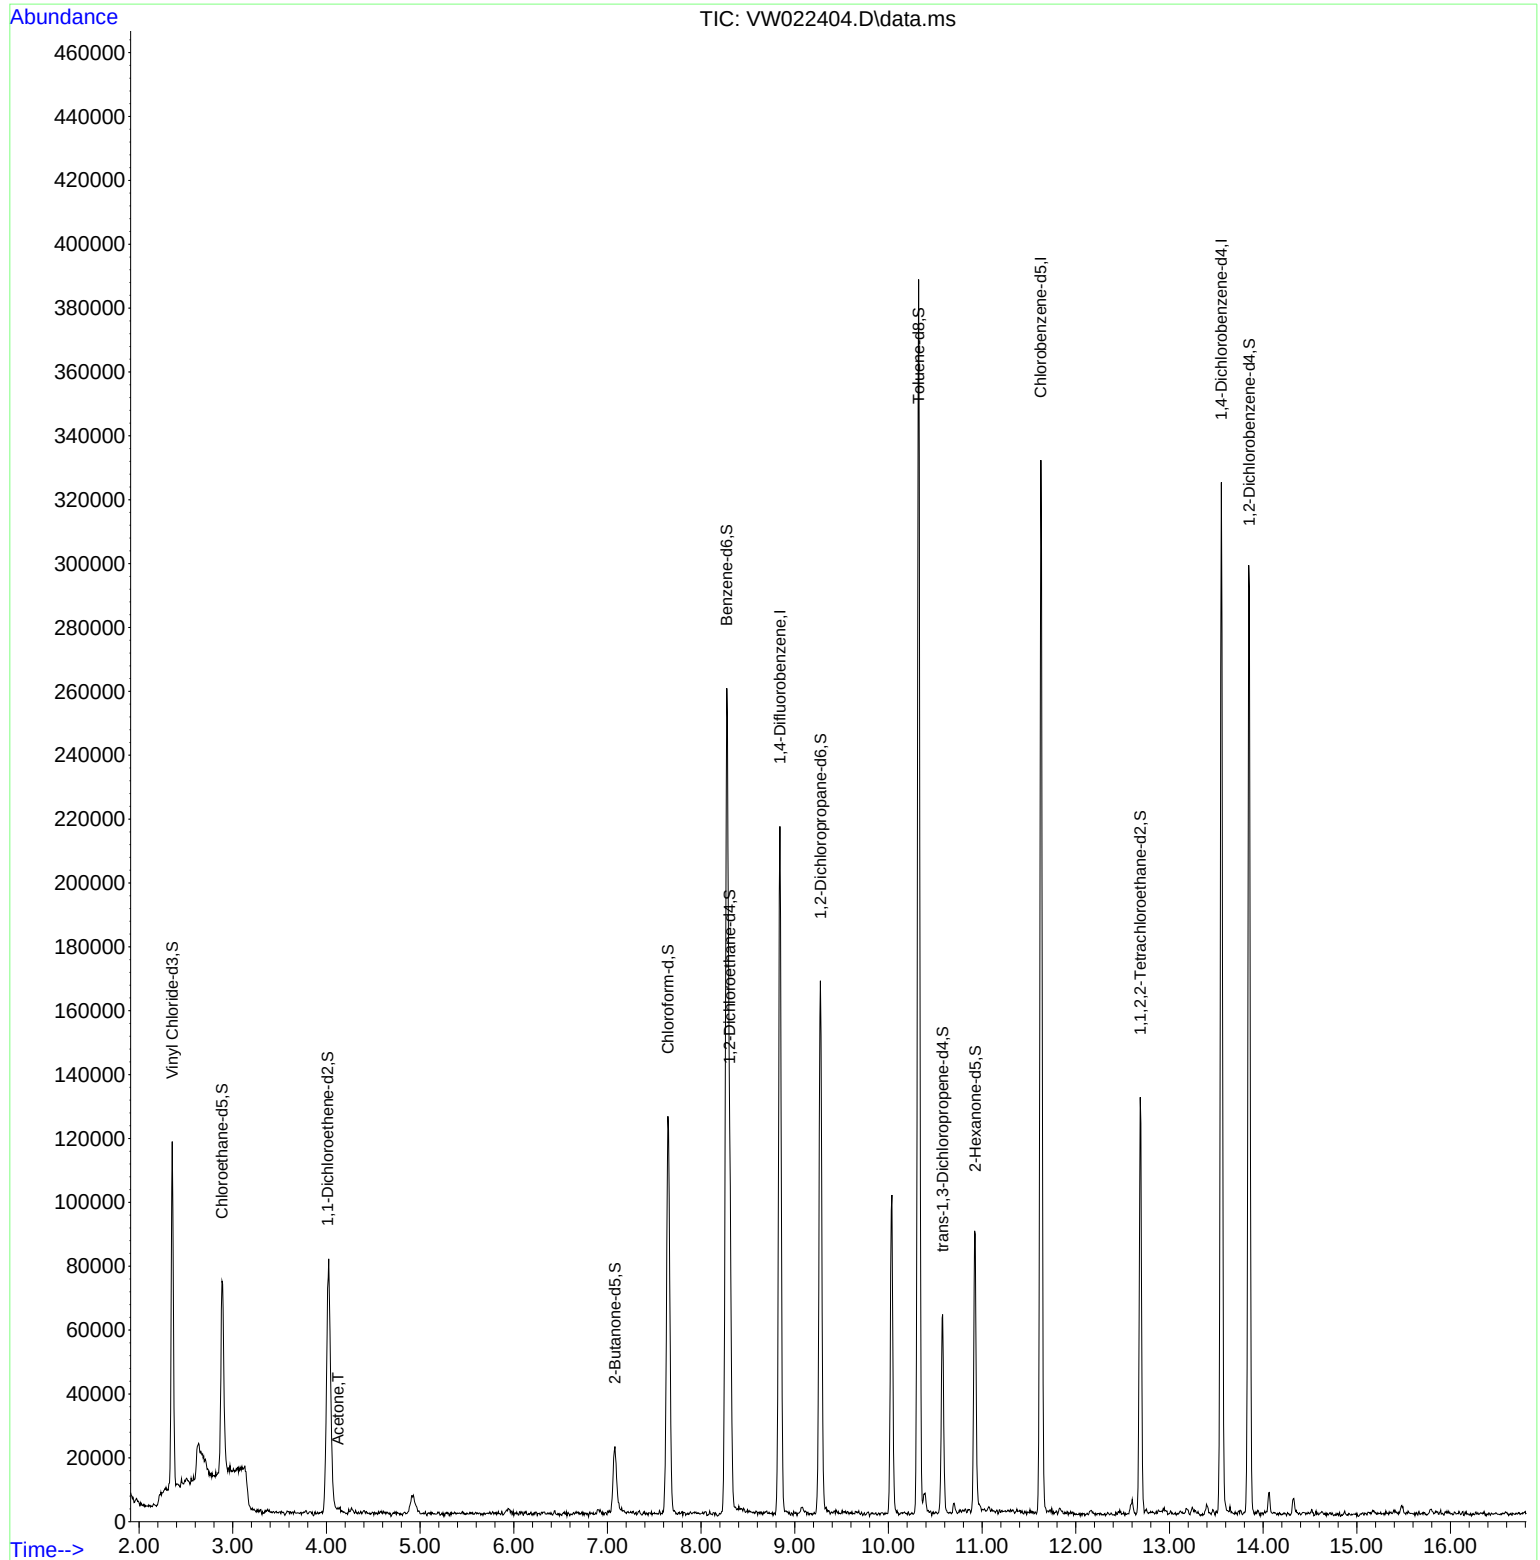

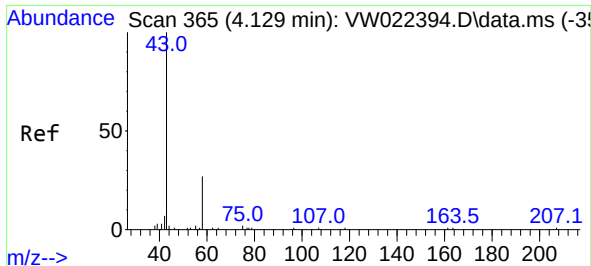

#13
Acetone
Concen: 6.890 ug/L m
RT: 4.123 min Scan# 30
Delta R.T. -0.006 min
Lab File: VW022404.D
Acq: 05 Apr 2022 19:04

Instrument :
MSVOA_W
ClientSampleId :
EW6L1

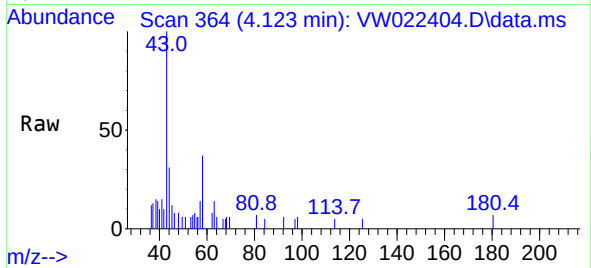

Tgt Ion: 43 Resp: 3200
Ion Ratio Lower Upper
43 100
58 28.3 0.0 69.2

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 04/06/2022
Supervised By :Mahesh Dadoda 04/07/2022

