

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
 Data File : VW022405.D
 Acq On : 05 Apr 2022 19:28
 Operator : SY/VA
 Sample : N2262-08
 Misc : 6.70g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6L2

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/06/2022
 Supervised By :Mahesh Dadoda 04/07/2022

Quant Time: Apr 06 02:16:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 06 02:13:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	186386	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	175857	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	78395	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	107247	35.109	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	140.440%
7) Chloroethane-d5	2.885	69	77642	42.576	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	170.320%#
11) 1,1-Dichloroethene-d2	4.019	63	76555	16.891	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.560%
21) 2-Butanone-d5	7.074	46	34109	45.697	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.400%
24) Chloroform-d	7.647	84	127008	24.439	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.760%
26) 1,2-Dichloroethane-d4	8.305	65	77344m	25.169	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	100.680%
32) Benzene-d6	8.275	84	268868	27.842	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	111.360%
36) 1,2-Dichloropropane-d6	9.274	67	76707	26.458	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	105.840%
41) Toluene-d8	10.323	98	267677	29.135	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	116.520%
43) trans-1,3-Dichloroprop...	10.579	79	33109	22.710	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	90.840%
47) 2-Hexanone-d5	10.920	63	29204	49.174	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.340%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	57256	23.410	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	93.640%
66) 1,2-Dichlorobenzene-d4	13.853	152	70336	27.793	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	111.160%
Target Compounds					Qvalue	
13) Acetone	4.123	43	3322m	6.499	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
Data File : VW022405.D
Acq On : 05 Apr 2022 19:28
Operator : SY/VA
Sample : N2262-08
Misc : 6.70g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EW6L2

Quant Time: Apr 06 02:16:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 06 02:13:06 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 04/06/2022
Supervised By :Mahesh Dadoda 04/07/2022

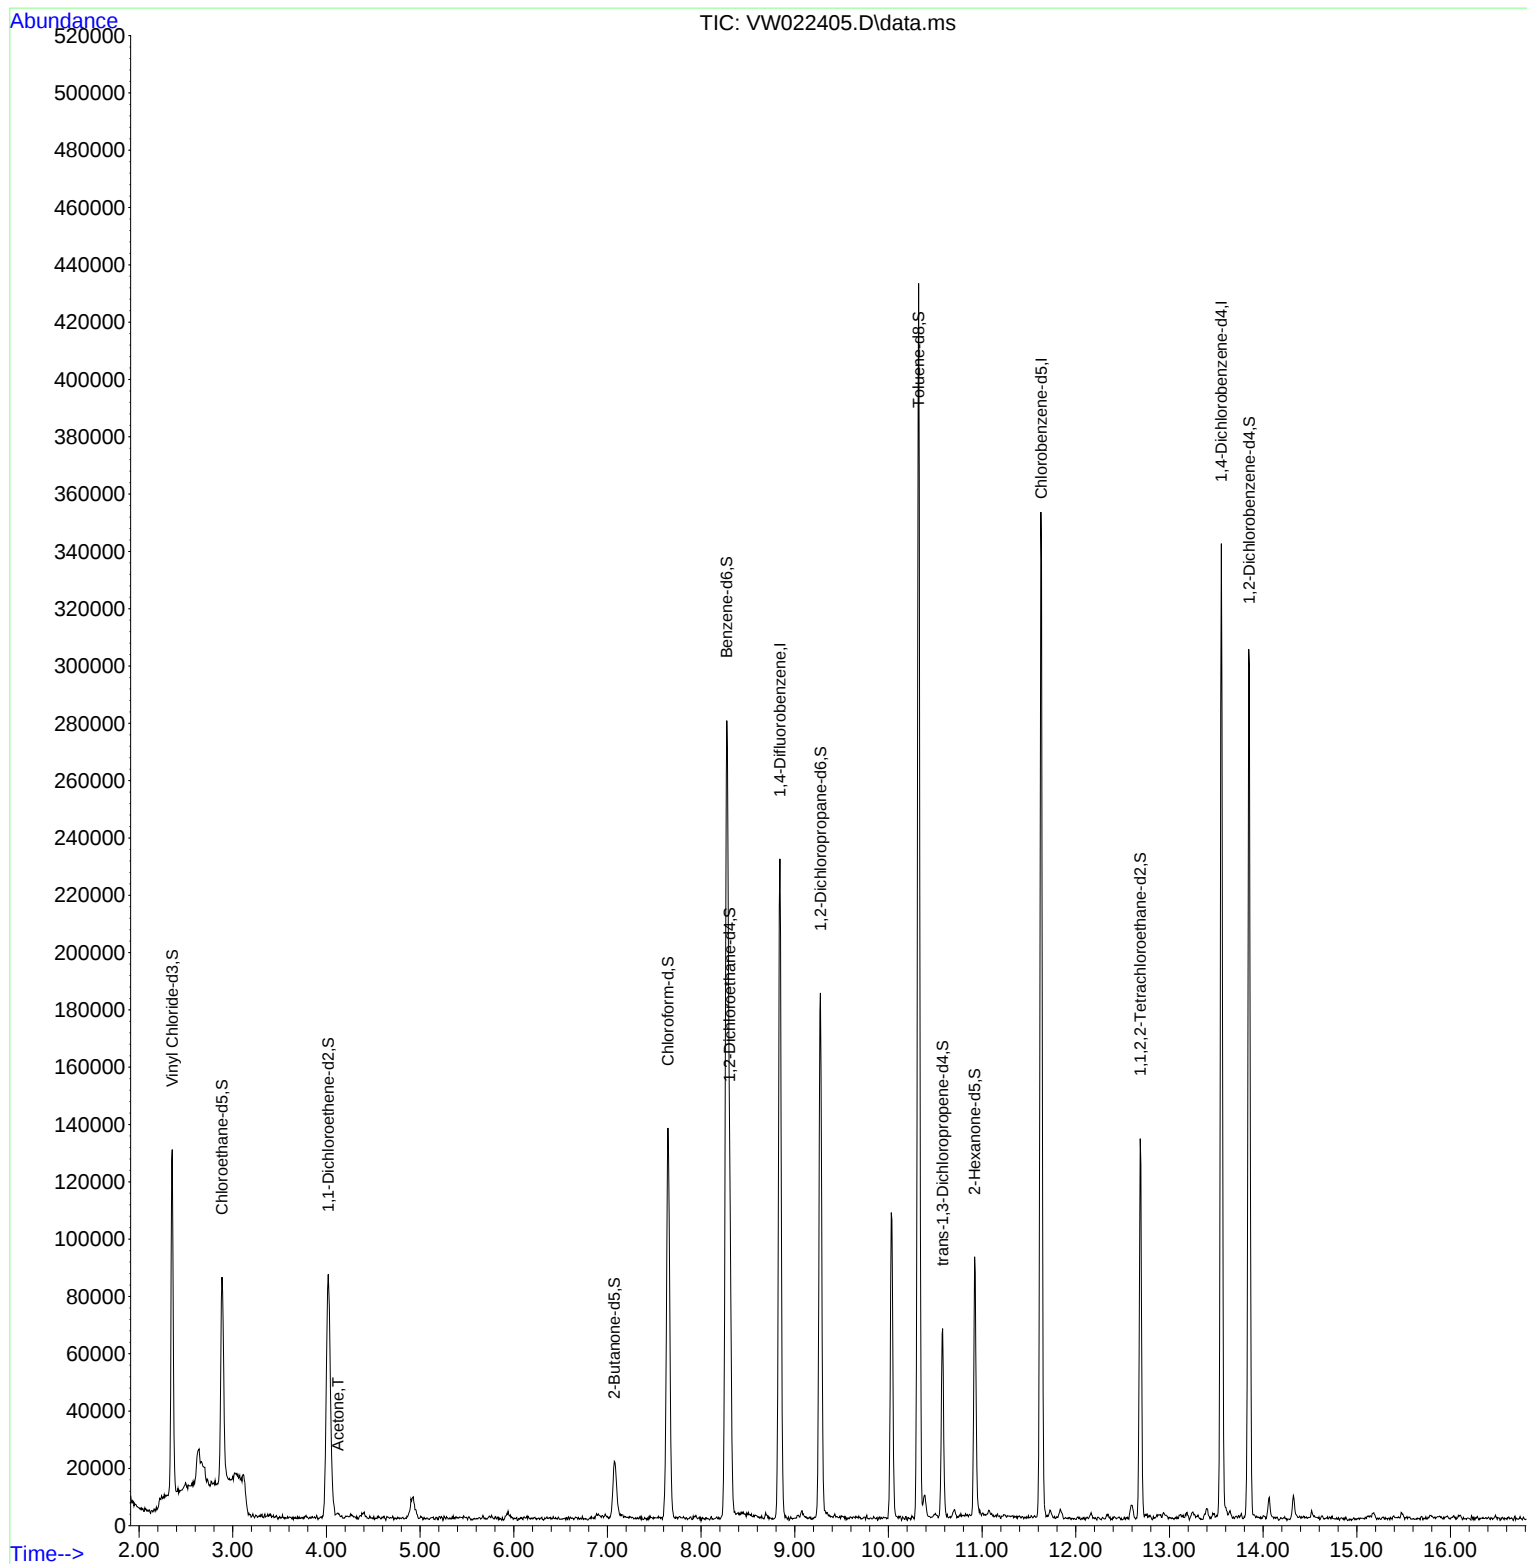

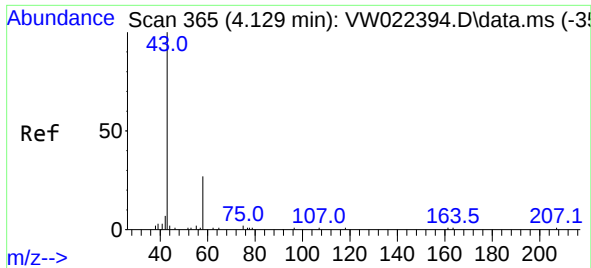

#13
 Acetone
 Concen: 6.499 ug/L m
 RT: 4.123 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VW022405.D
 Acq: 05 Apr 2022 19:28

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6L2

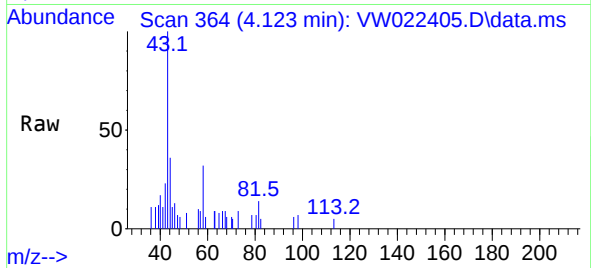

Tgt Ion: 43 Resp: 332
 Ion Ratio Lower Upper
 43 100
 58 26.2 0.0 69.2

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/06/2022
 Supervised By :Mahesh Dadoda 04/07/2022

