

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
 Data File : VW022406.D
 Acq On : 05 Apr 2022 19:52
 Operator : SY/VA
 Sample : N2262-09
 Misc : 7.19g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6L3

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 04/06/2022
 Supervised By : Mahesh Dadoda 04/07/2022

Quant Time: Apr 06 02:16:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 06 02:13:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	157787	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	140919	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	55897	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	95934	37.098	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	148.400%
7) Chloroethane-d5	2.885	69	69496	45.016	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	180.080%#
11) 1,1-Dichloroethene-d2	4.019	63	65837	17.159	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.640%
21) 2-Butanone-d5	7.074	46	30382	48.082	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.160%
24) Chloroform-d	7.647	84	108086	24.568	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.280%
26) 1,2-Dichloroethane-d4	8.305	65	65627	25.227	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	100.920%
32) Benzene-d6	8.275	84	226140	29.223	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	116.880%
36) 1,2-Dichloropropane-d6	9.274	67	66440	28.598	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	114.400%
41) Toluene-d8	10.323	98	215309	29.245	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	117.000%
43) trans-1,3-Dichloroprop...	10.579	79	25975	22.234	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	88.920%
47) 2-Hexanone-d5	10.920	63	24449	51.375	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	102.740%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	50353	25.692	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	102.760%
66) 1,2-Dichlorobenzene-d4	13.853	152	50597	28.040	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	112.160%
Target Compounds					Qvalue	
13) Acetone	4.123	43	2182m	5.043	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040522\
Data File : VW022406.D
Acq On : 05 Apr 2022 19:52
Operator : SY/VA
Sample : N2262-09
Misc : 7.19g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EW6L3

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 04/06/2022
Supervised By : Mahesh Dadoda 04/07/2022


Quant Time: Apr 06 02:16:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040122SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 06 02:13:06 2022
Response via : Initial Calibration

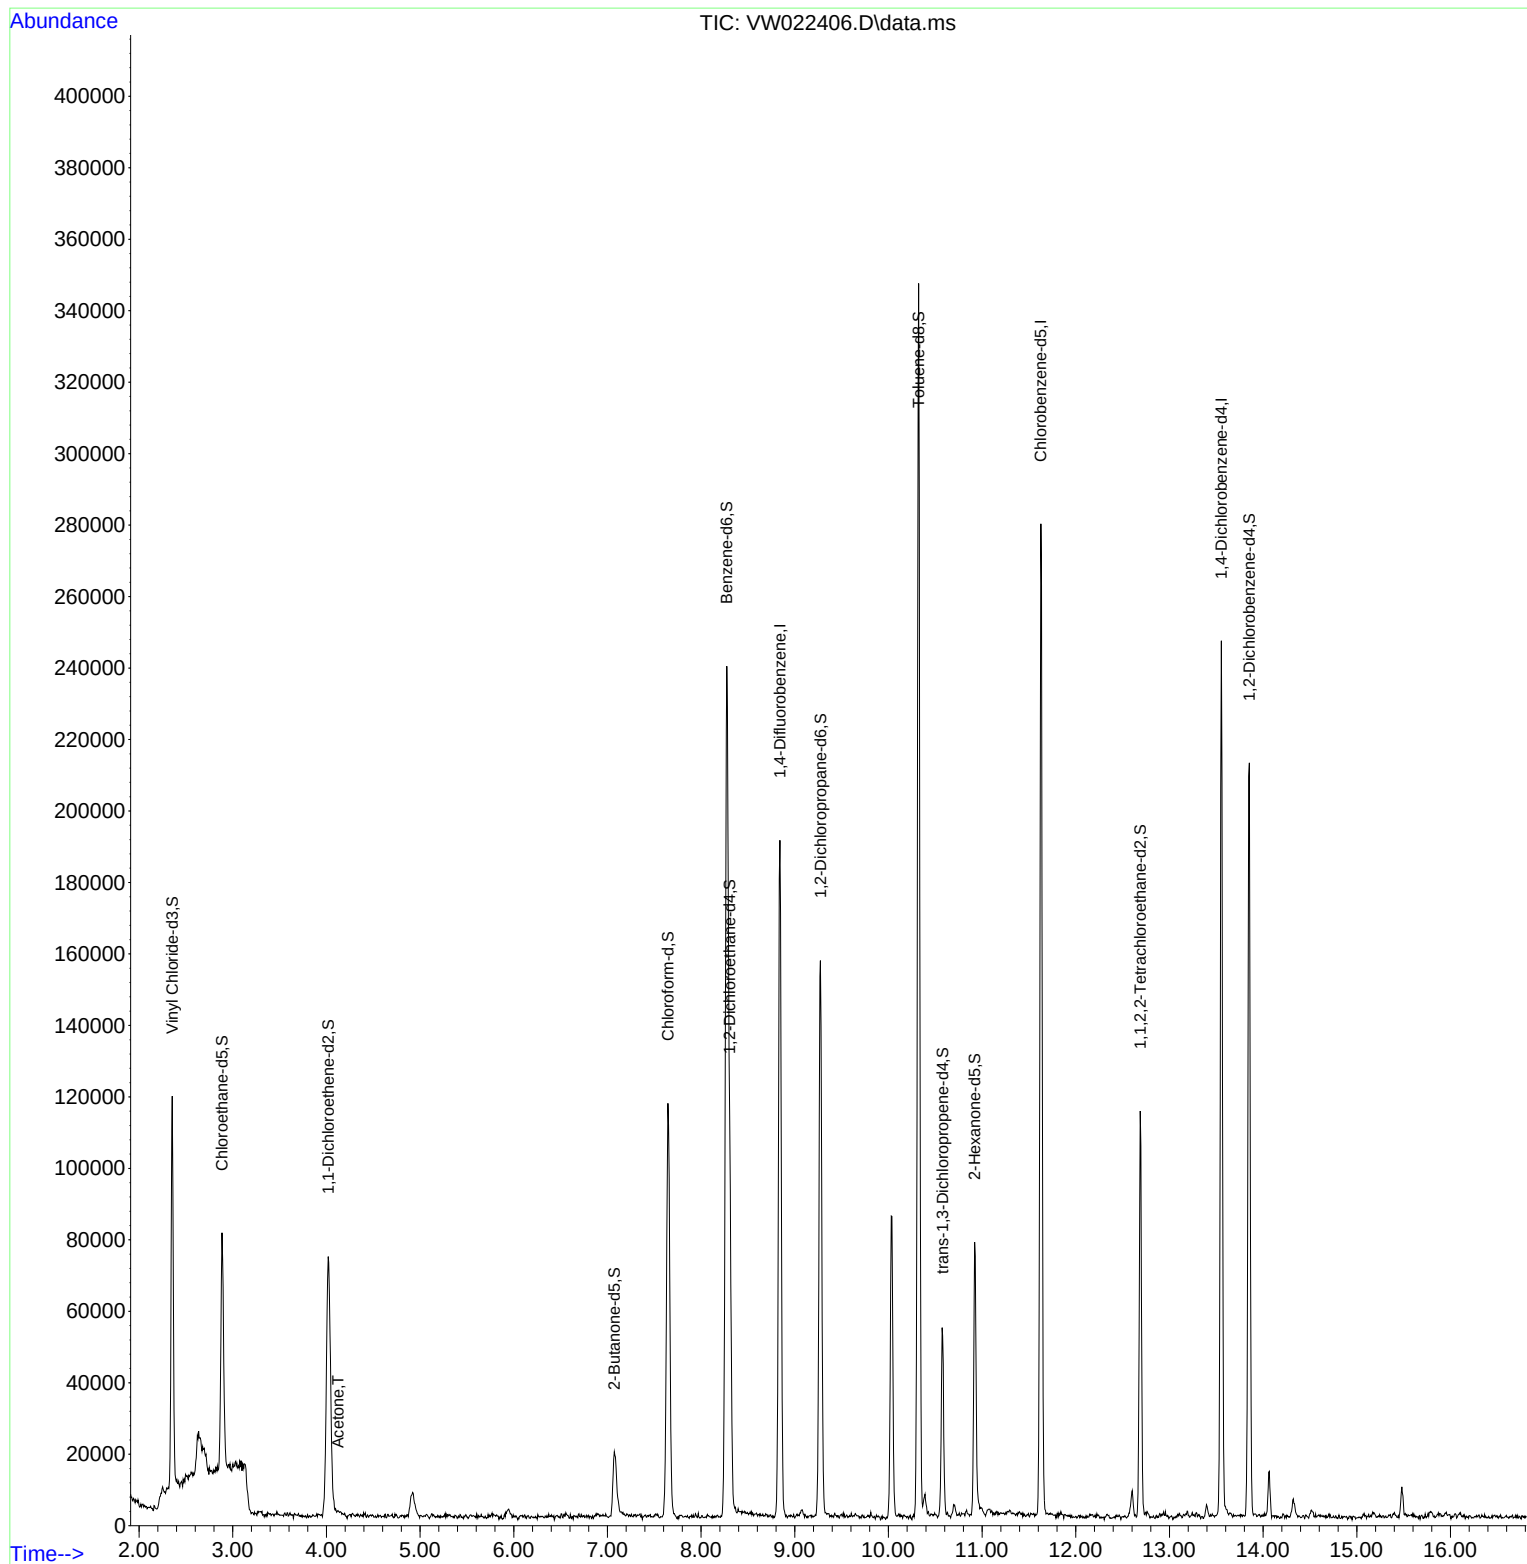

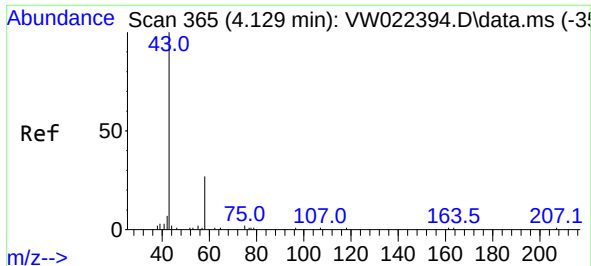

#13
Acetone
Concen: 5.043 ug/L m
RT: 4.123 min Scan# 30
Delta R.T. -0.006 min
Lab File: VW022406.D
Acq: 05 Apr 2022 19:52

Instrument :
MSVOA_W
ClientSampleId :
EW6L3

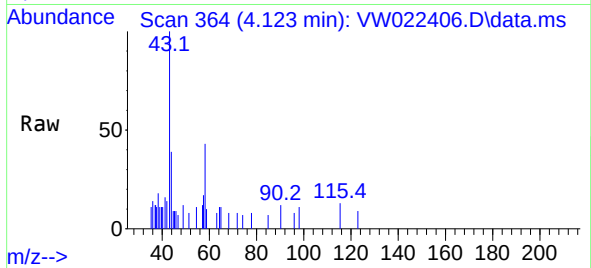

Tgt Ion: 43 Resp: 218
Ion Ratio Lower Upper
43 100
58 22.4 0.0 69.2

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 04/06/2022
Supervised By :Mahesh Dadoda 04/07/2022

