




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040619\
Data File : VW009754.D
Acq On : 06 Apr 2019 03:52
Operator : SY/VA
Sample : K2188-06
Misc : 3.22G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF662

Manual Integrations
APPROVED

MMDadoda
4/11/2019 11:42:52 AM

Quant Time: Apr 06 05:40:10 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 06 05:36:42 2019
Response via : Initial Calibration

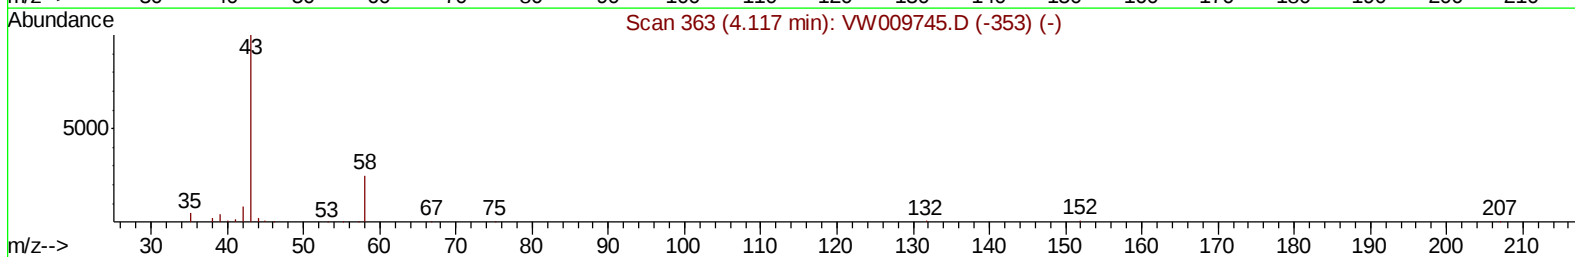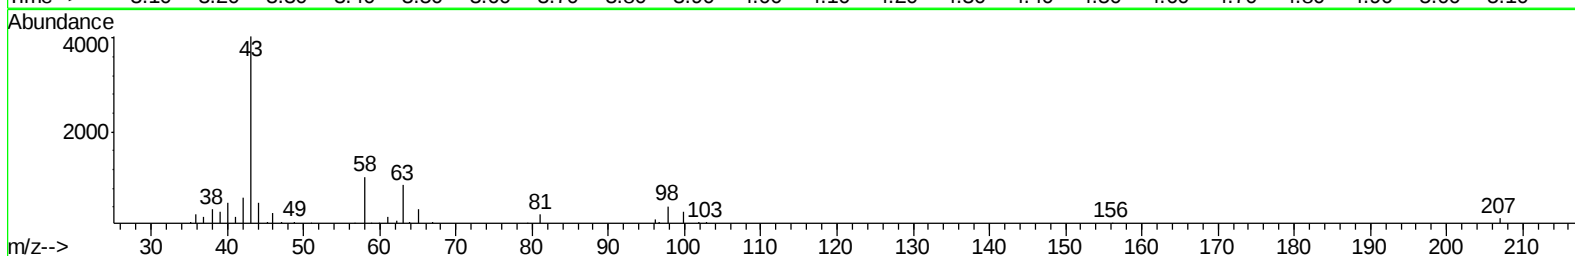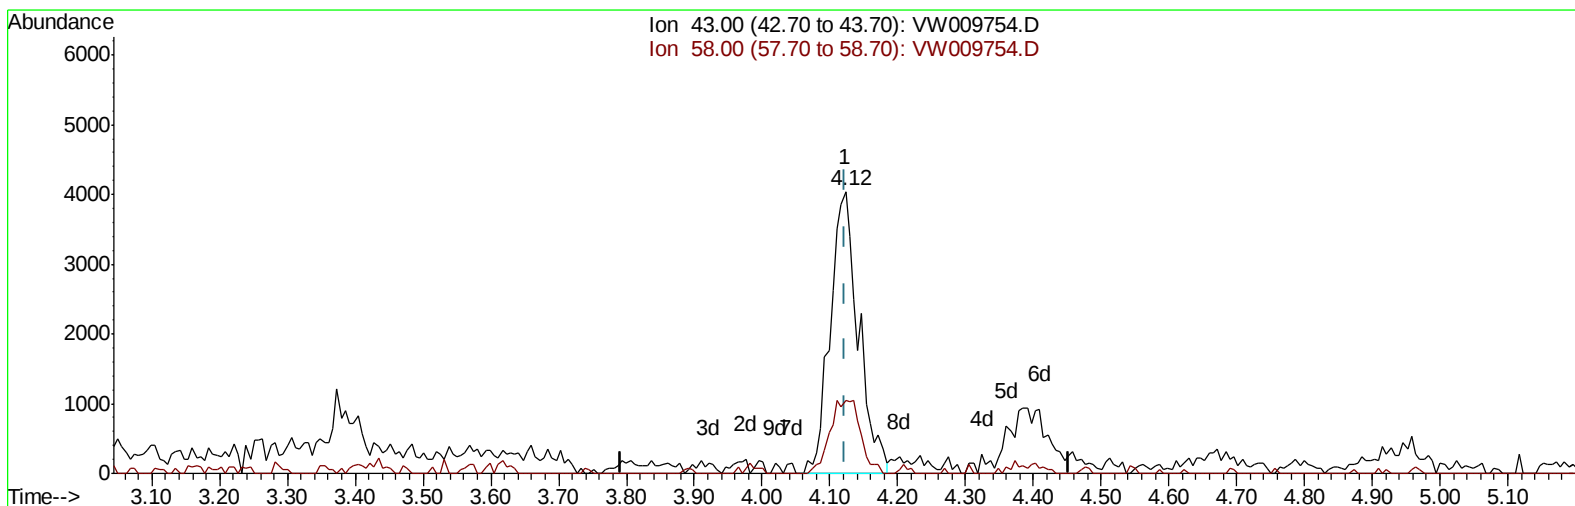

TIC: VW009754.D

(13) Acetone (T)

4.123min (+0.000) 6.36ug/L m

response 11661

Ion	Exp%	Act%
43.00	100	100
58.00	26.50	12.52
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040619\
 Data File : VW009754.D
 Acq On : 06 Apr 2019 03:52
 Operator : SY/VA
 Sample : K2188-06
 Misc : 3.22G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF662

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 11:42:52 AM

Quant Time: Apr 06 07:02:40 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M

Quant Title : VOC Analysis

QLast Update : Sat Apr 06 05:36:42 2019

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	402674	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	288536	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	73156	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	152765	28.99	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	115.96%
7) Chloroethane-d5	2.90	69	140722	29.15	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	116.60%
10) 1,1-Dichloroethene-d2	4.01	63	246274	21.73	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	86.92%
20) 2-Butanone-d5	7.08	46	79868	46.68	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.36%
24) Chloroform-d	7.65	84	303978	27.67	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	110.68%
26) 1,2-Dichloroethane-d4	8.31	65	179419	26.60	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	106.40%
29) Benzene-d6	8.27	84	584946	38.62	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	154.48%#
33) 1,2-Dichloropropane-d6	9.27	67	171207	36.60	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	146.40%#
37) Toluene-d8	10.32	98	458080	32.71	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	130.84%#
38) trans-1,3-Dichloropropene-	10.57	79	25163	11.28	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	45.12%
39) 2-Hexanone-d5	10.93	63	49343	55.96	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	111.92%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	82411	18.95	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	75.80%
61) 1,2-Dichlorobenzene-d4	13.86	152	63678	24.81	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.24%

Target Compounds

					Qvalue	
13) Acetone	4.12	43	11661m	6.361	ug/L	
14) Carbon disulfide	4.37	76	41994	2.526	ug/L	97
16) Methylene chloride	4.92	84	54604	7.689	ug/L	89
44) Toluene	10.38	91	20289	1.103	ug/L	91
47) Tetrachloroethene	10.86	164	1423	0.398	ug/L #	75
53) Ethylbenzene	11.73	91	35613	1.700	ug/L	94
54) m,p-Xylene	11.83	106	13130	1.695	ug/L	99
55) o-xylene	12.16	106	8413	1.140	ug/L	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040619\
Data File : VW009754.D
Acq On : 06 Apr 2019 03:52
Operator : SY/VA
Sample : K2188-06
Misc : 3.22G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF662

Manual Integrations
APPROVED

MMDadoda
4/11/2019 11:42:52 AM

Quant Time: Apr 06 07:02:40 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 06 05:36:42 2019
Response via : Initial Calibration

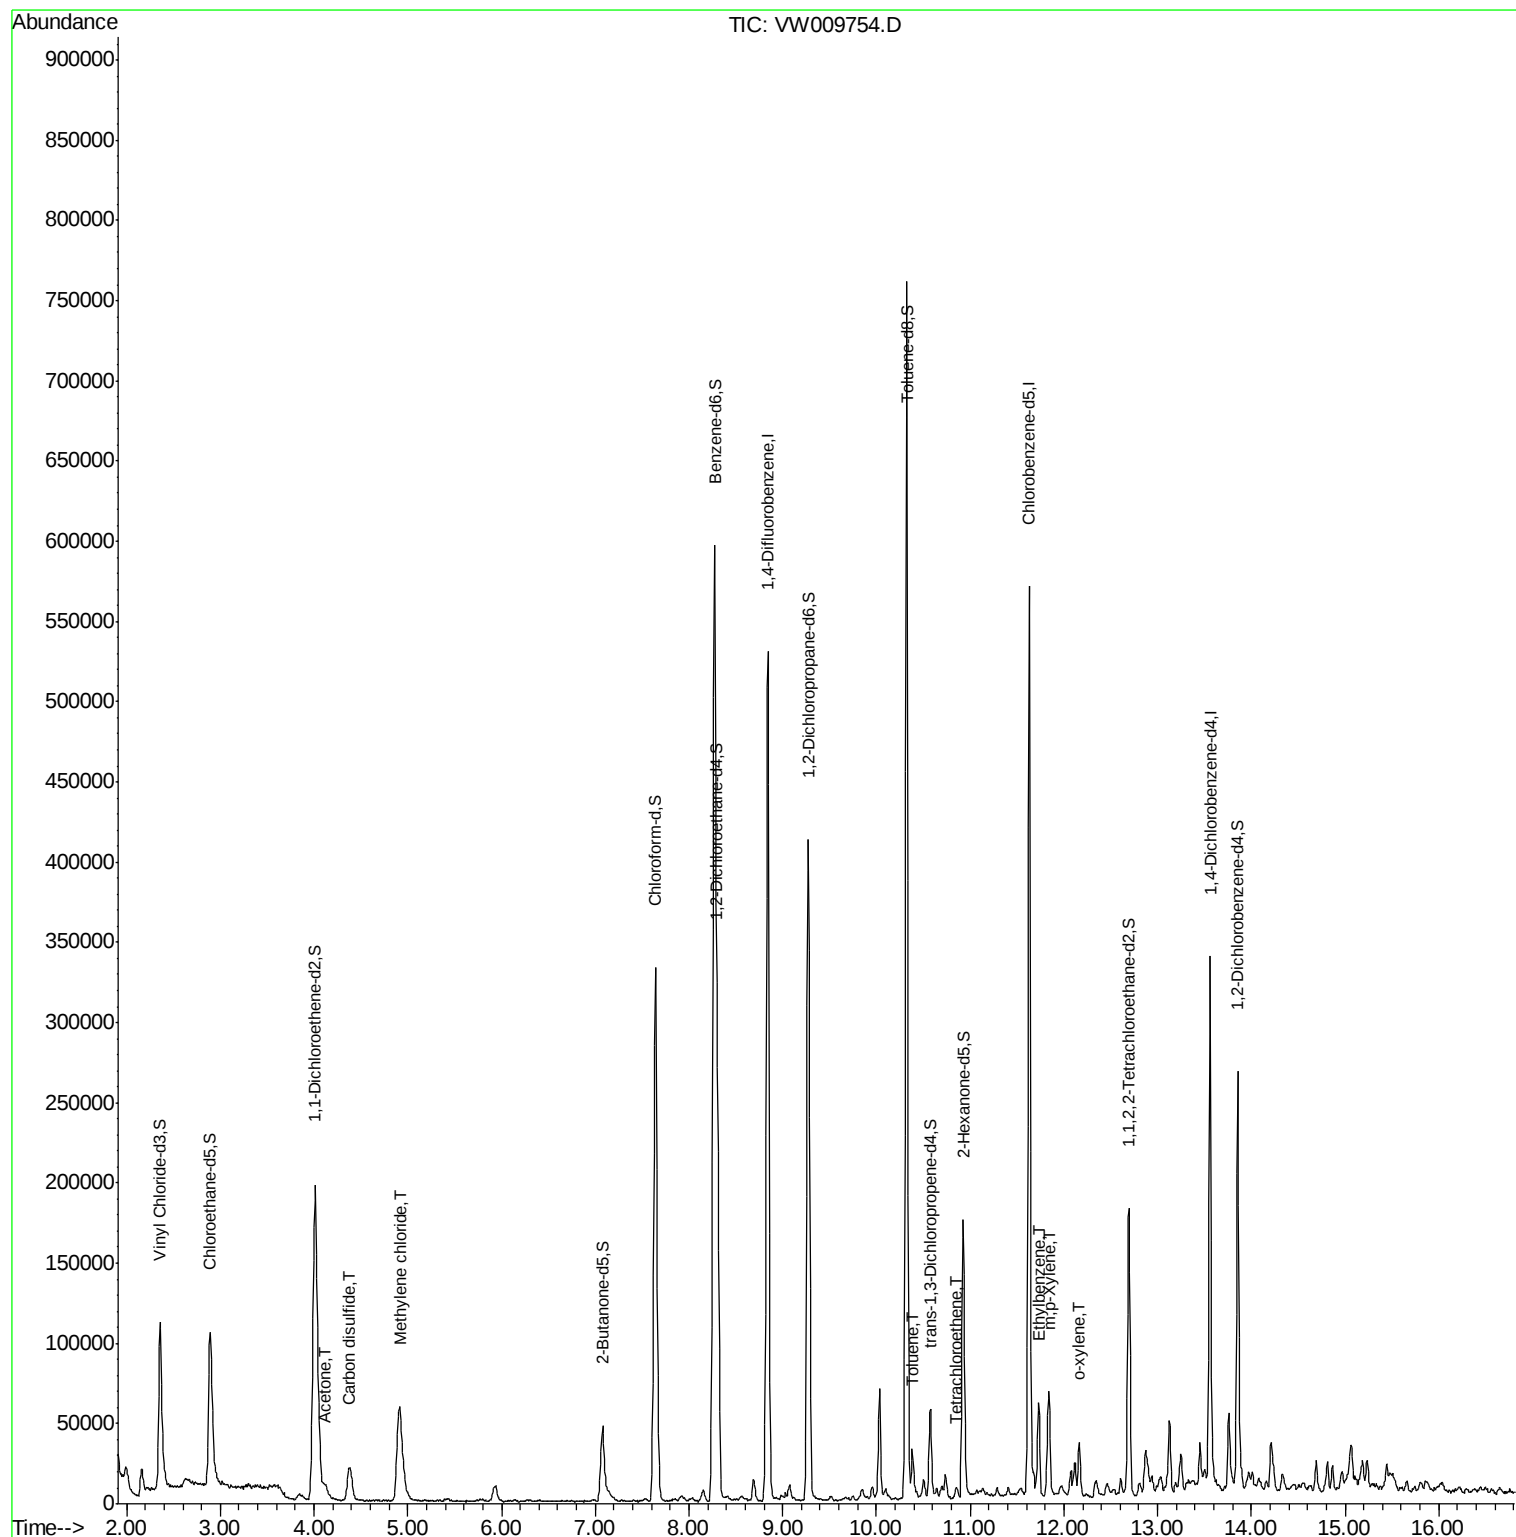




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040619\
Data File : VW009754.D
Acq On : 06 Apr 2019 03:52
Operator : SY/VA
Sample : K2188-06
Misc : 3.22G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF662

Manual Integrations
APPROVED

MMDadoda
4/11/2019 11:42:52 AM

Quant Time: Apr 06 05:40:10 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 06 05:36:42 2019
Response via : Initial Calibration

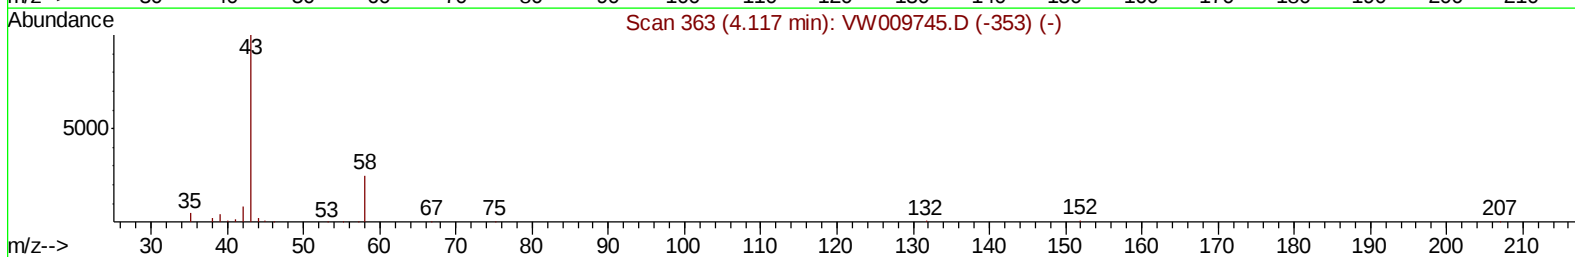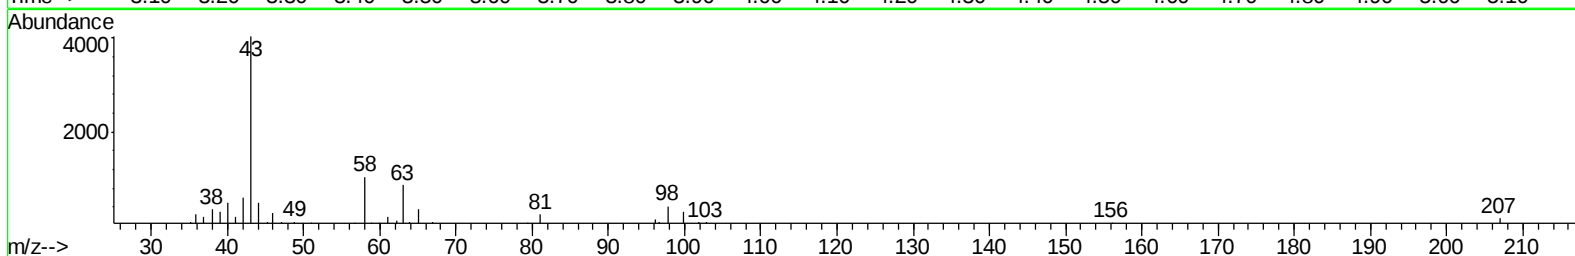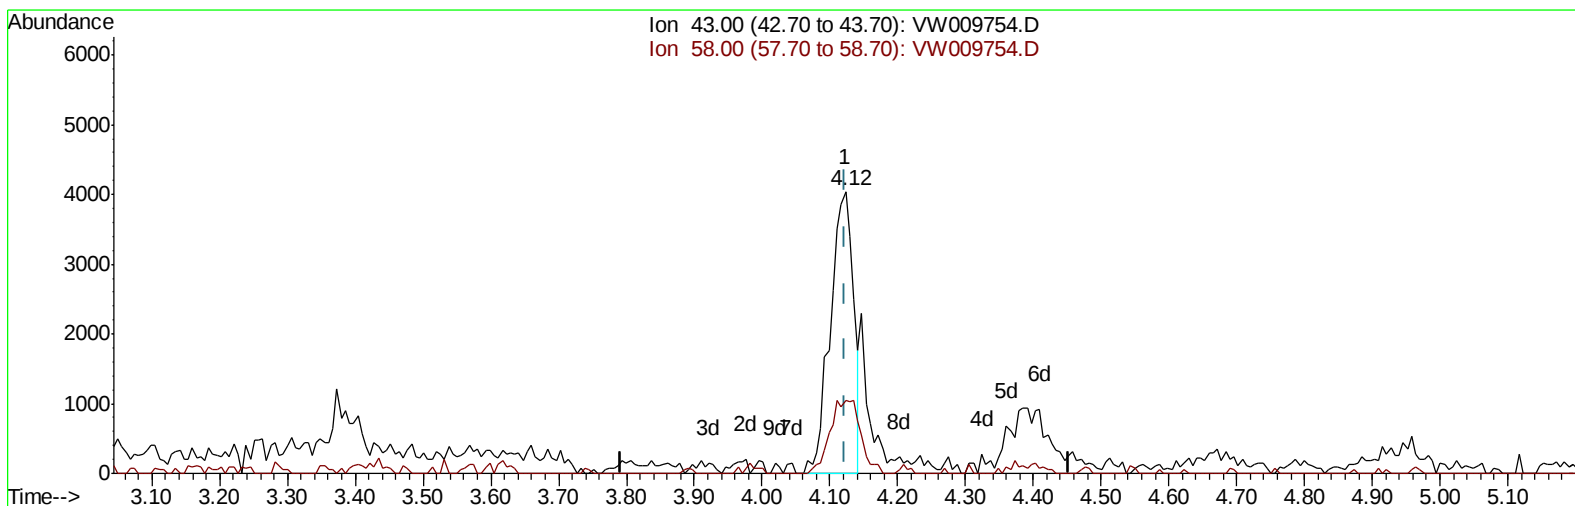

TIC: VW009754.D

(13) Acetone (T)

4.123min (+0.000) 5.27ug/L

response 9654

Ion	Exp%	Act%
43.00	100	100
58.00	26.50	15.12
0.00	0.00	0.00
0.00	0.00	0.00