




Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW040619\
Data File : VW009758.D
Acq On : 06 Apr 2019 05:41
Operator : SY/VA
Sample : K2188-09
Misc : 5.22G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF653

Quant Time: Apr 06 07:10:16 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 06 05:36:42 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
4/11/2019 11:42:55 AM

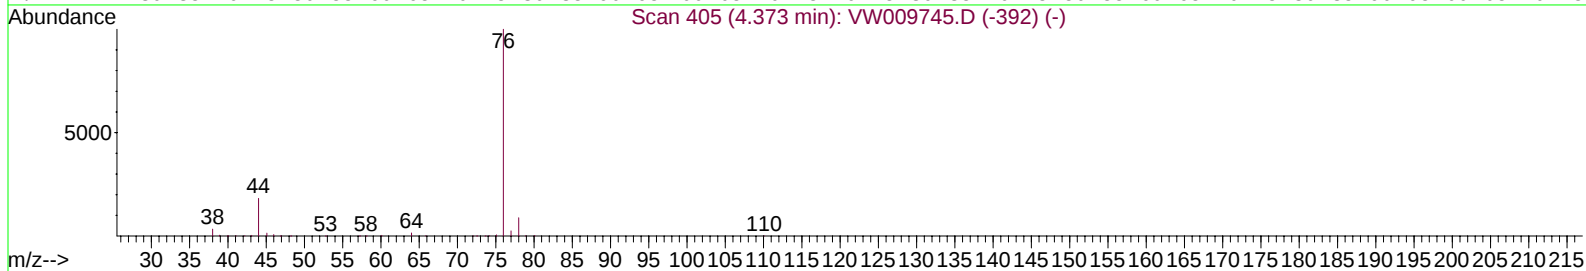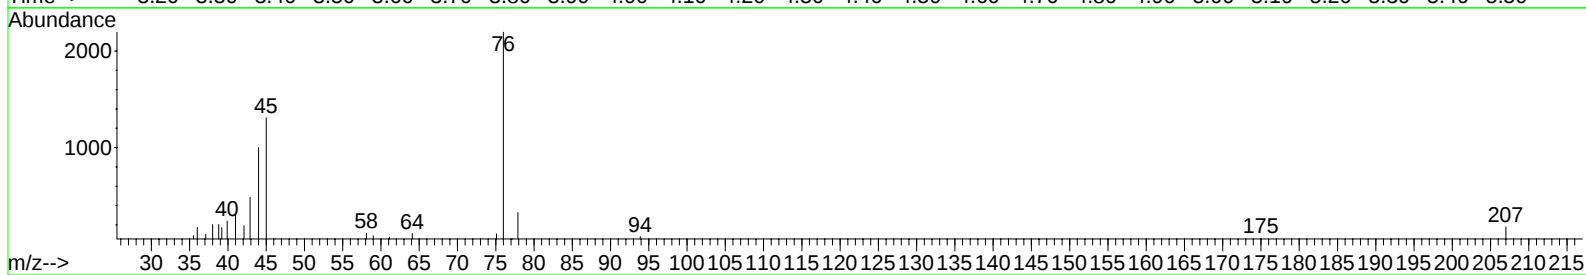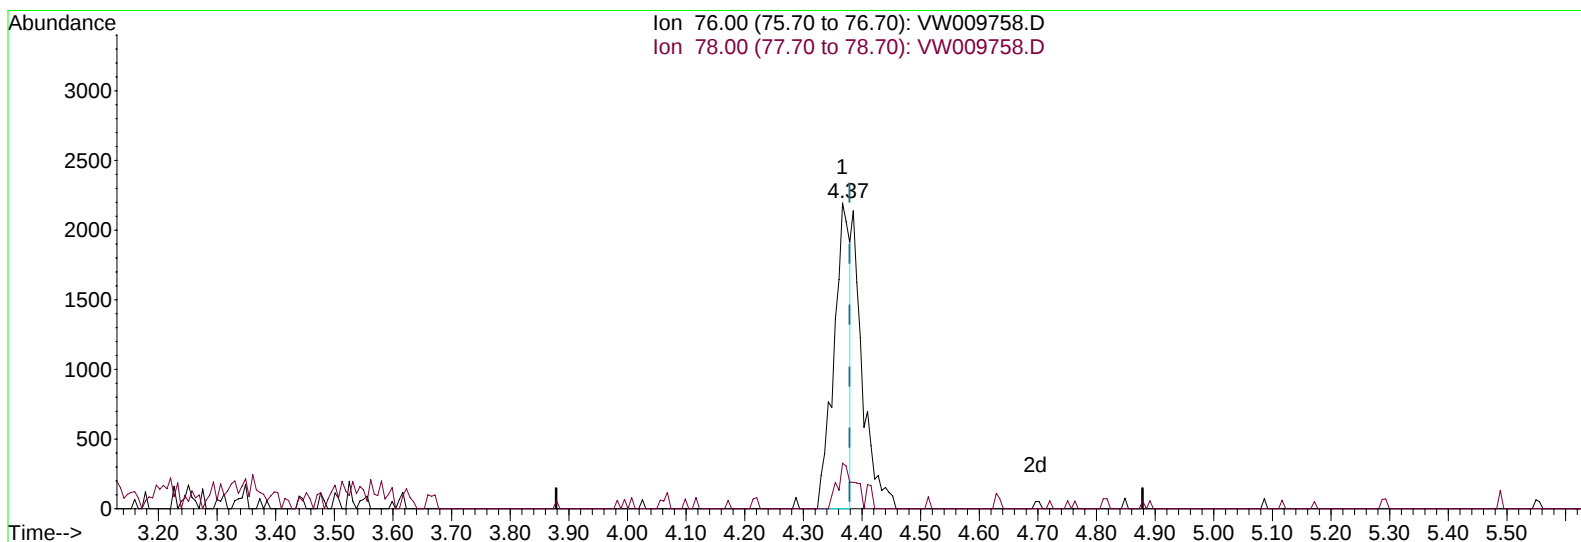

TIC: VW009758.D

(14) Carbon disulfide (T)

4.367min (-0.012) 0.26ug/L

response 4134

Ion	Exp%	Act%
76.00	100	100
78.00	9.10	14.90#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW040619\
 Data File : VW009758.D
 Acq On : 06 Apr 2019 05:41
 Operator : SY/VA
 Sample : K2188-09
 Misc : 5.22G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF653

Quant Time: Apr 06 07:10:16 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 06 05:36:42 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 11:42:55 AM

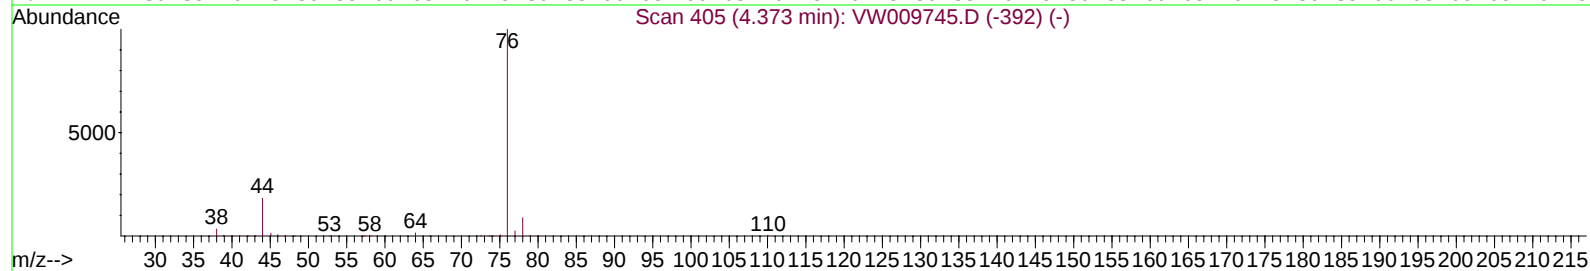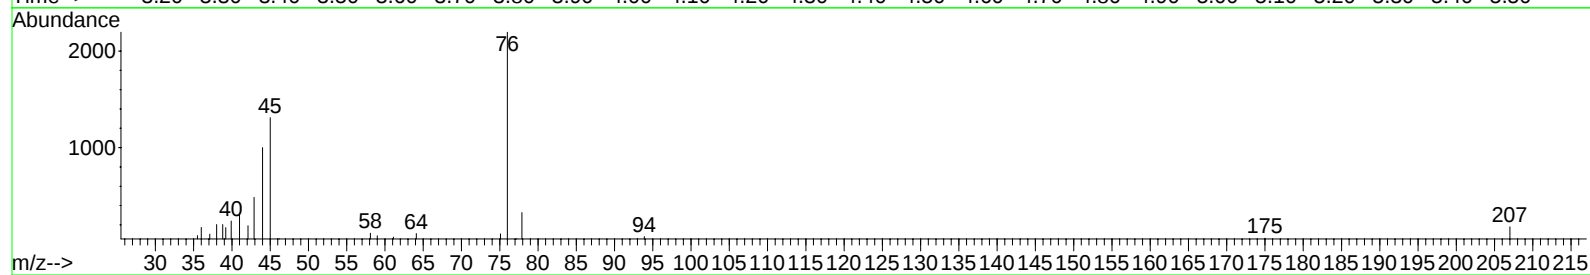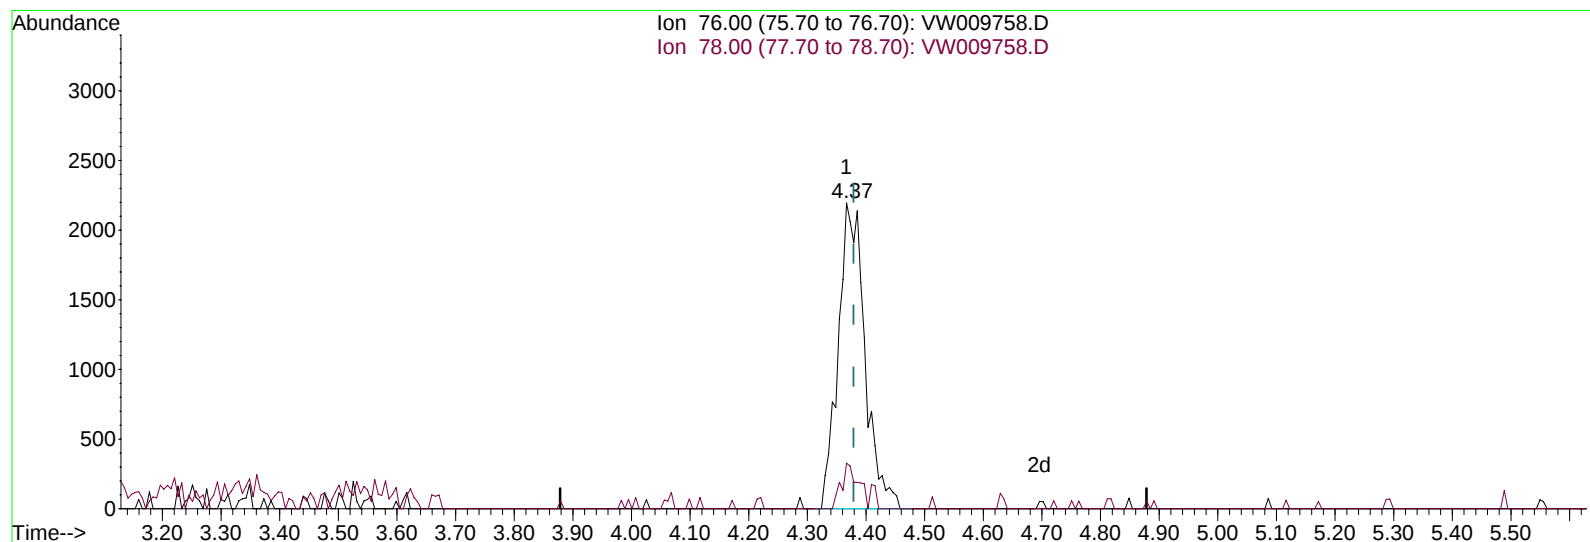

TIC: VW009758.D

(14) Carbon disulfide (T)

4.367min (-0.012) 0.44ug/L m

response 6942

Ion	Exp%	Act%
76.00	100	100
78.00	9.10	14.90#
0.00	0.00	0.00
0.00	0.00	0.00