




Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW040619\
Data File : VW009769.D
Acq On : 06 Apr 2019 13:40
Operator : SY/VA
Sample : K2327-02
Misc : 5.25G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF2R8

Manual Integrations
APPROVED

MMDadoda
4/11/2019 11:43:03 AM

Quant Time: Apr 07 04:00:22 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Sun Apr 07 03:56:20 2019
Response via : Initial Calibration

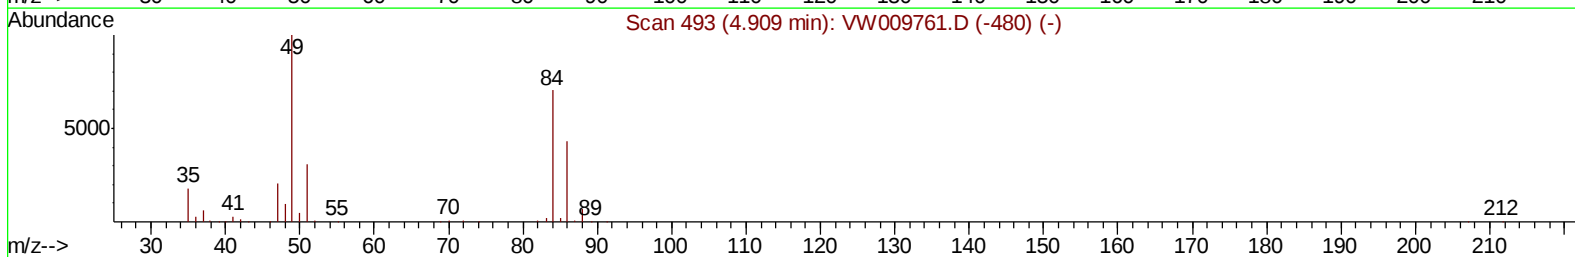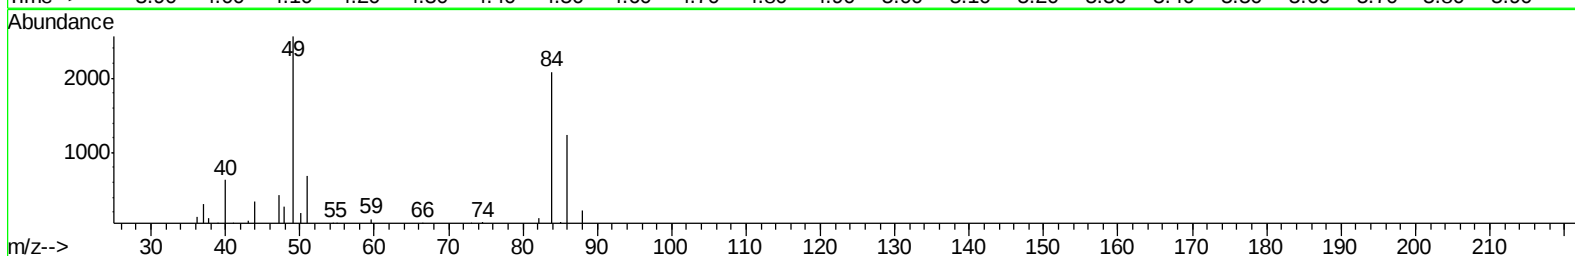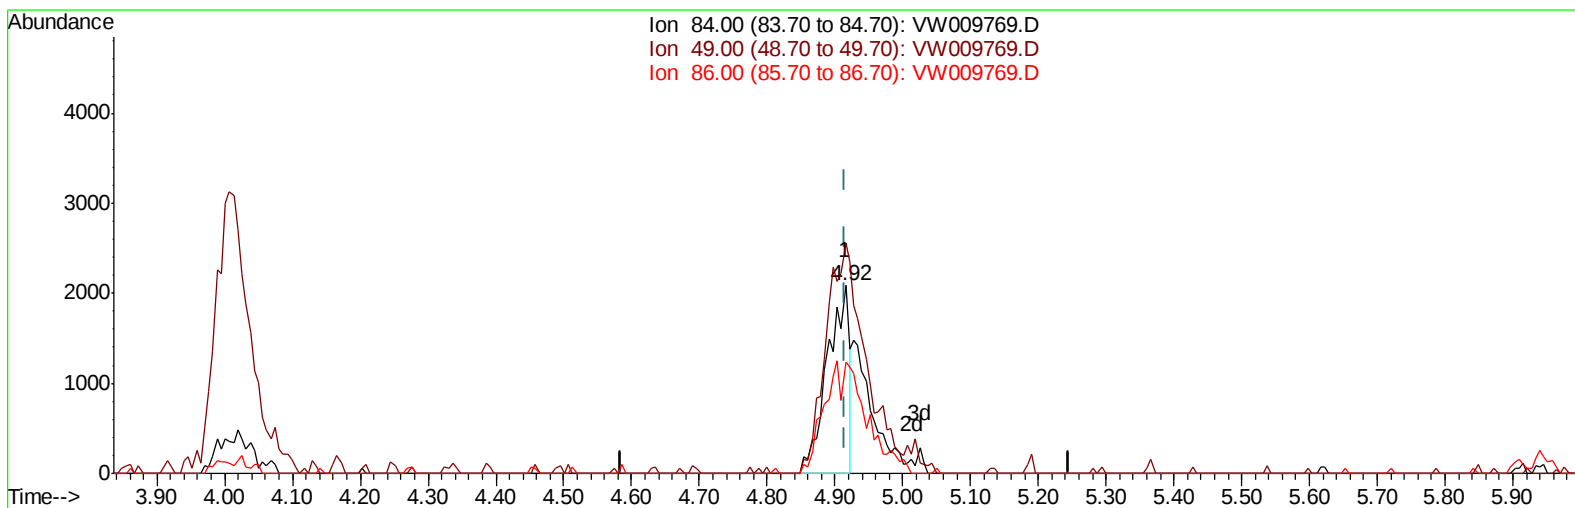

TIC: VW009769.D

(16) Methylene chloride (T)

4.915min (+0.000) 0.50ug/L

response 4633

Ion	Exp%	Act%
84.00	100	100
49.00	140.40	122.78
86.00	66.30	59.38
0.00	0.00	0.00




Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW040619\
Data File : VW009769.D
Acq On : 06 Apr 2019 13:40
Operator : SY/VA
Sample : K2327-02
Misc : 5.25G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF2R8

Manual Integrations
APPROVED

MMDadoda
4/11/2019 11:43:03 AM

Quant Time: Apr 07 04:00:22 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Sun Apr 07 03:56:20 2019
Response via : Initial Calibration

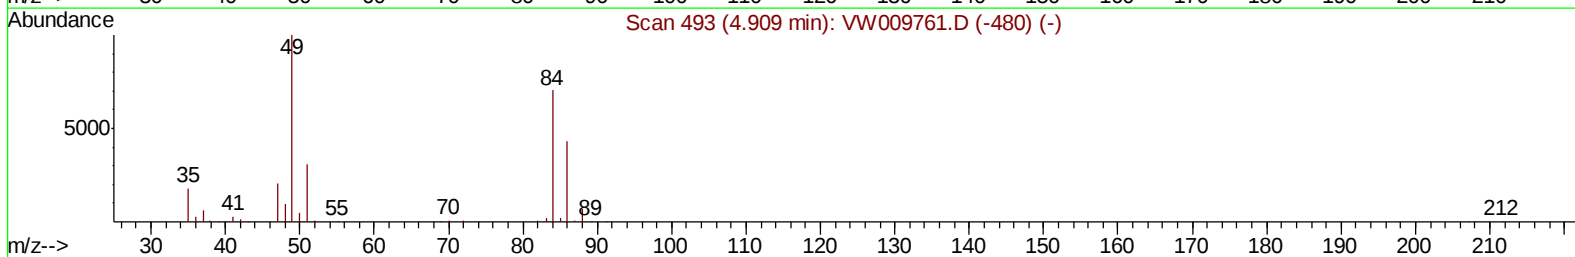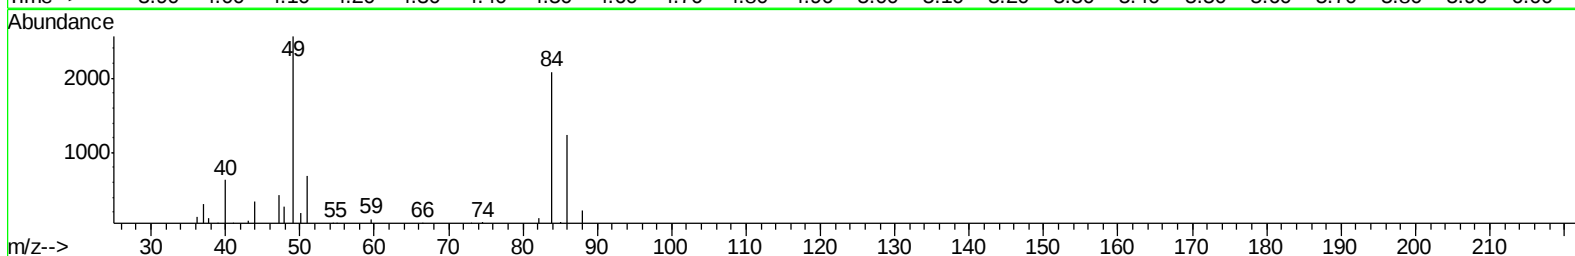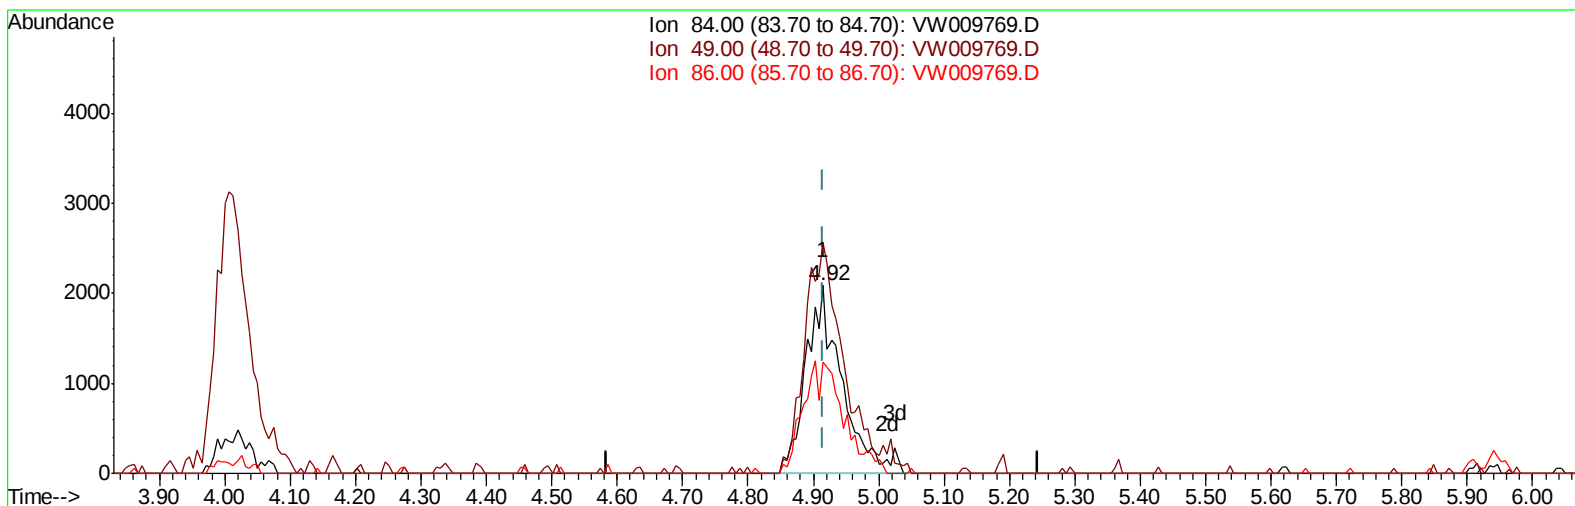

TIC: VW009769.D

(16) Methylene chloride (T)

4.915min (+0.000) 0.86ug/L m

response 7973

Ion	Exp%	Act%
84.00	100	100
49.00	140.40	122.78
86.00	66.30	59.38
0.00	0.00	0.00