




Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW040619\
Data File : VW009779.D
Acq On : 06 Apr 2019 18:13
Operator : SY/VA
Sample : K2168-15
Misc : 6.09G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF640

Manual Integrations
APPROVED

MMDadoda
4/11/2019 11:43:10 AM

Quant Time: Apr 07 04:01:38 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Sun Apr 07 03:56:20 2019
Response via : Initial Calibration

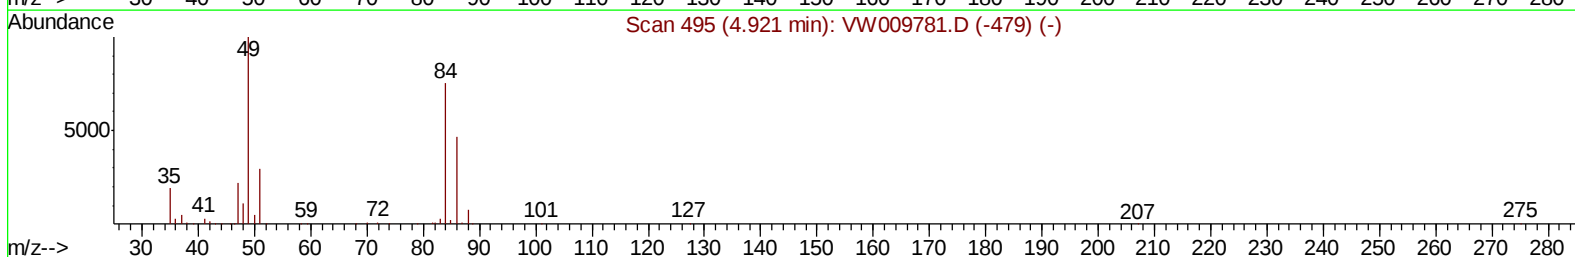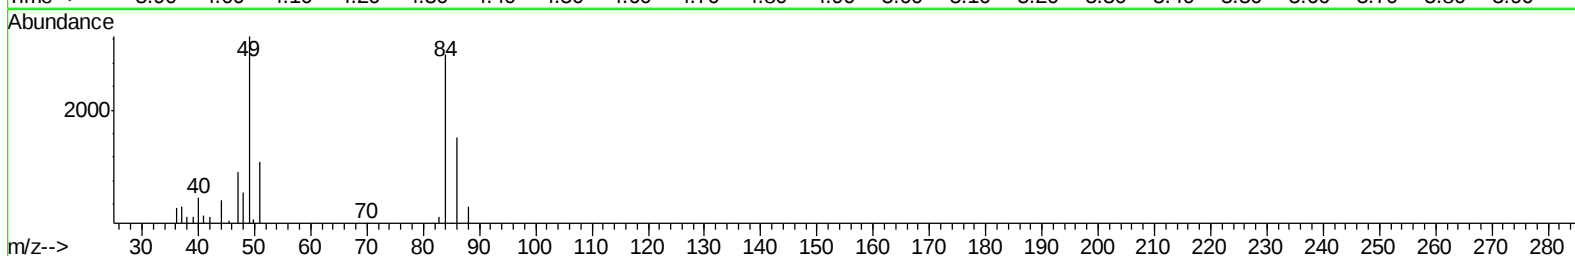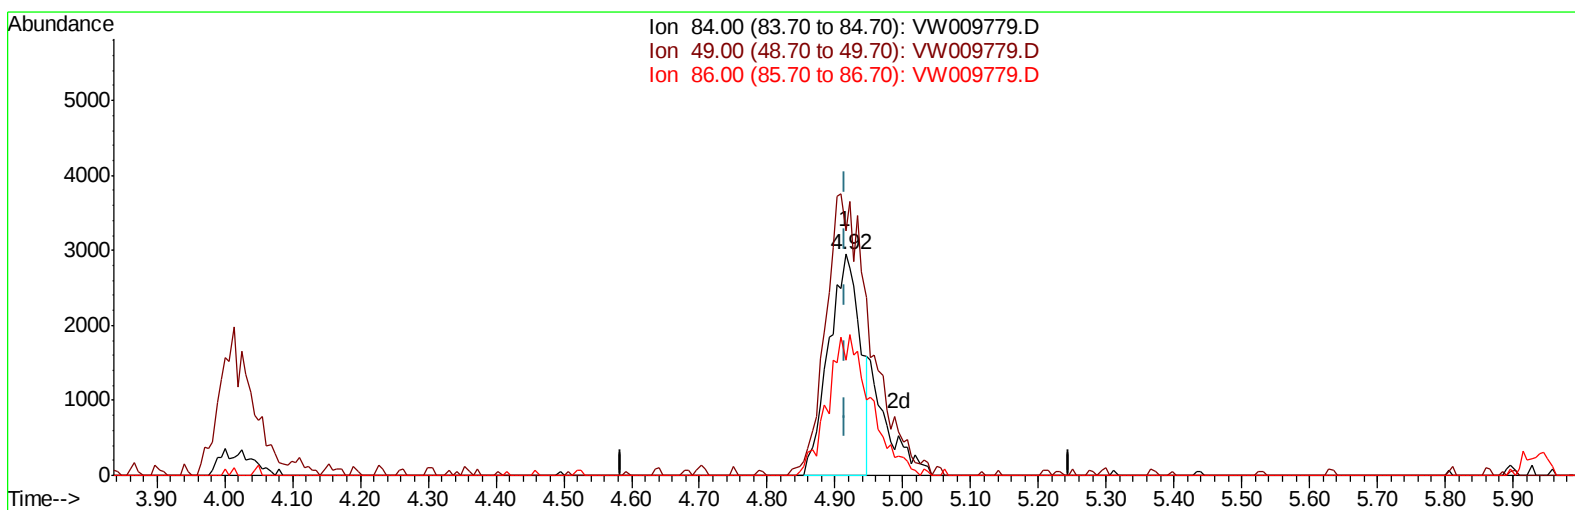

TIC: VW009779.D

(16) Methylene chloride (T)

4.915min (+0.000) 1.42ug/L

response 9455

Ion	Exp%	Act%
84.00	100	100
49.00	140.40	110.20
86.00	66.30	52.02
0.00	0.00	0.00




Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW040619\
Data File : VW009779.D
Acq On : 06 Apr 2019 18:13
Operator : SY/VA
Sample : K2168-15
Misc : 6.09G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF640

Manual Integrations
APPROVED

MMDadoda
4/11/2019 11:43:10 AM

Quant Time: Apr 07 04:01:38 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Sun Apr 07 03:56:20 2019
Response via : Initial Calibration

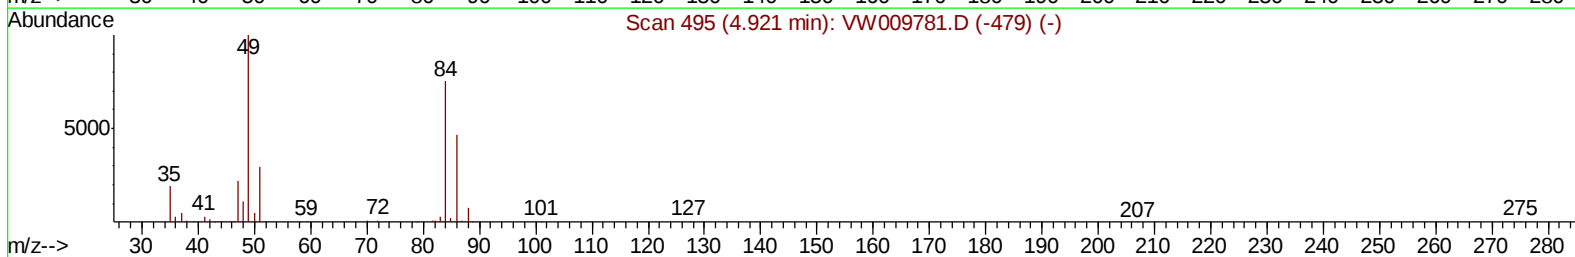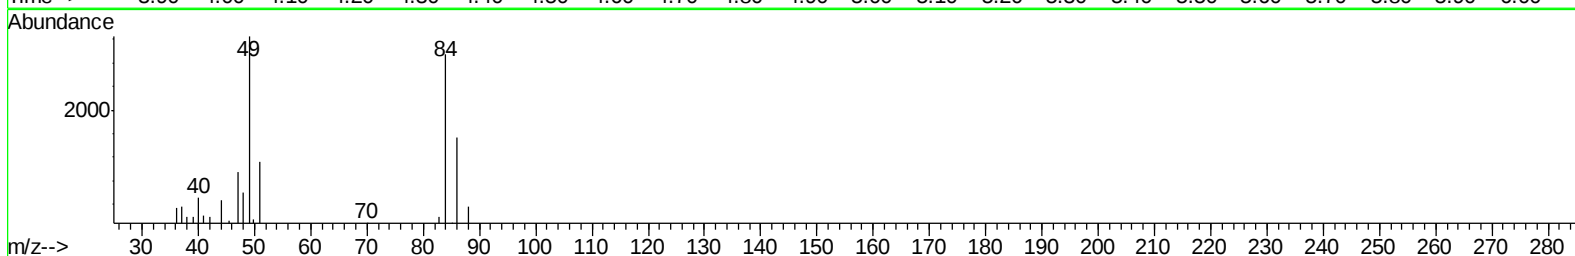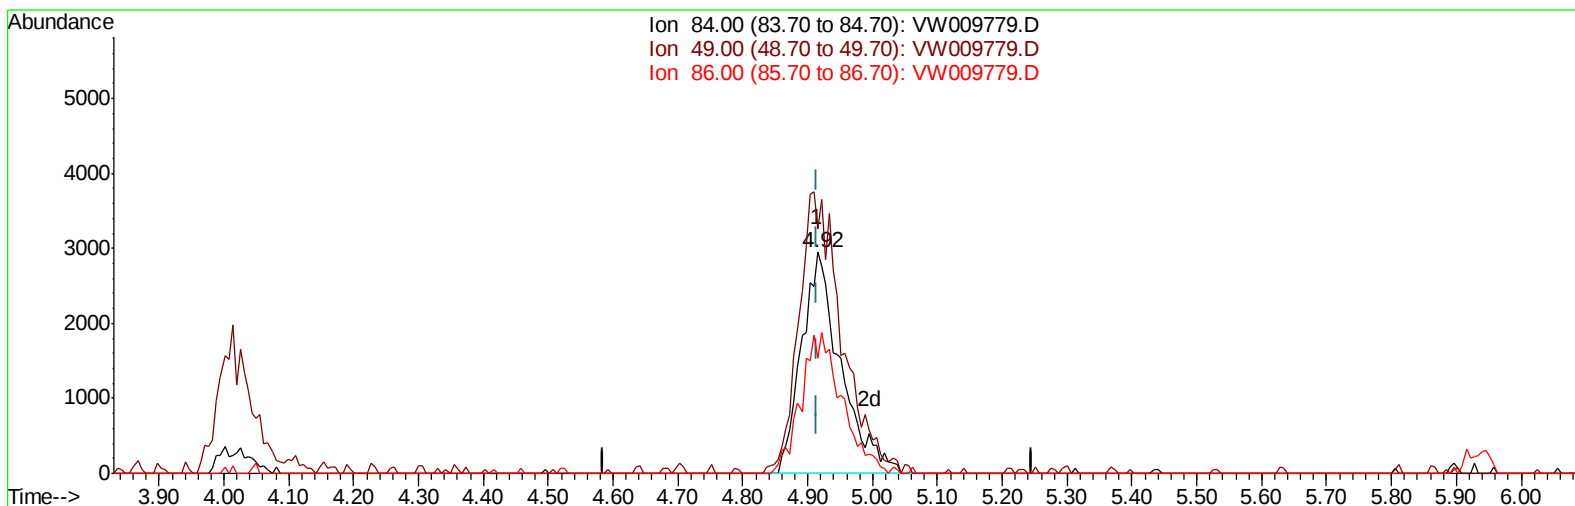

TIC: VW009779.D

(16) Methylene chloride (T)

4.915min (+0.000) 1.87ug/L m

response 12424

Ion	Exp%	Act%
84.00	100	100
49.00	140.40	110.20
86.00	66.30	52.02
0.00	0.00	0.00