




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040619\
Data File : VW009788.D
Acq On : 06 Apr 2019 23:52
Operator : SY/VA
Sample : K2217-09
Misc : 5.82G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF618

Manual Integrations
APPROVED

MMDadoda
4/11/2019 11:43:18 AM

Quant Time: Apr 07 05:39:56 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Sun Apr 07 05:36:41 2019
Response via : Initial Calibration

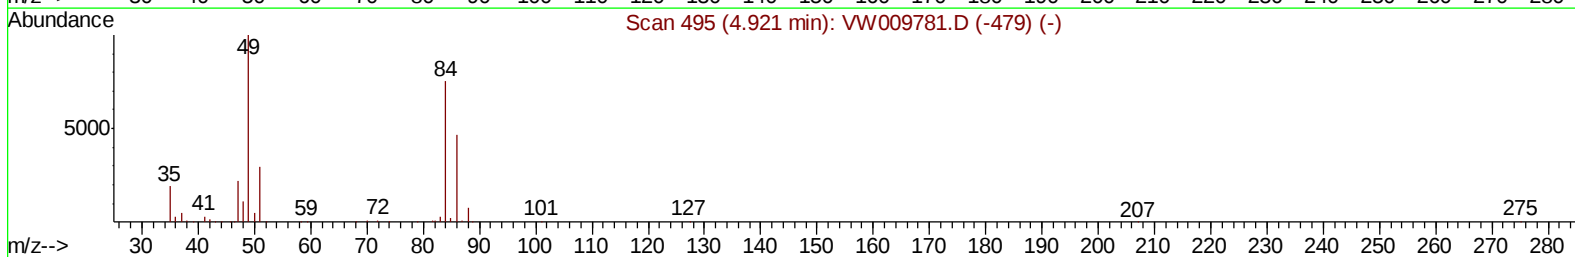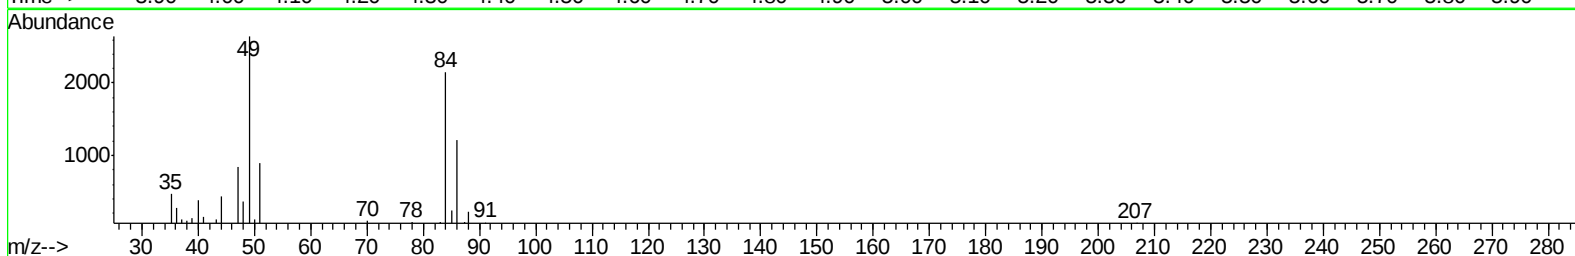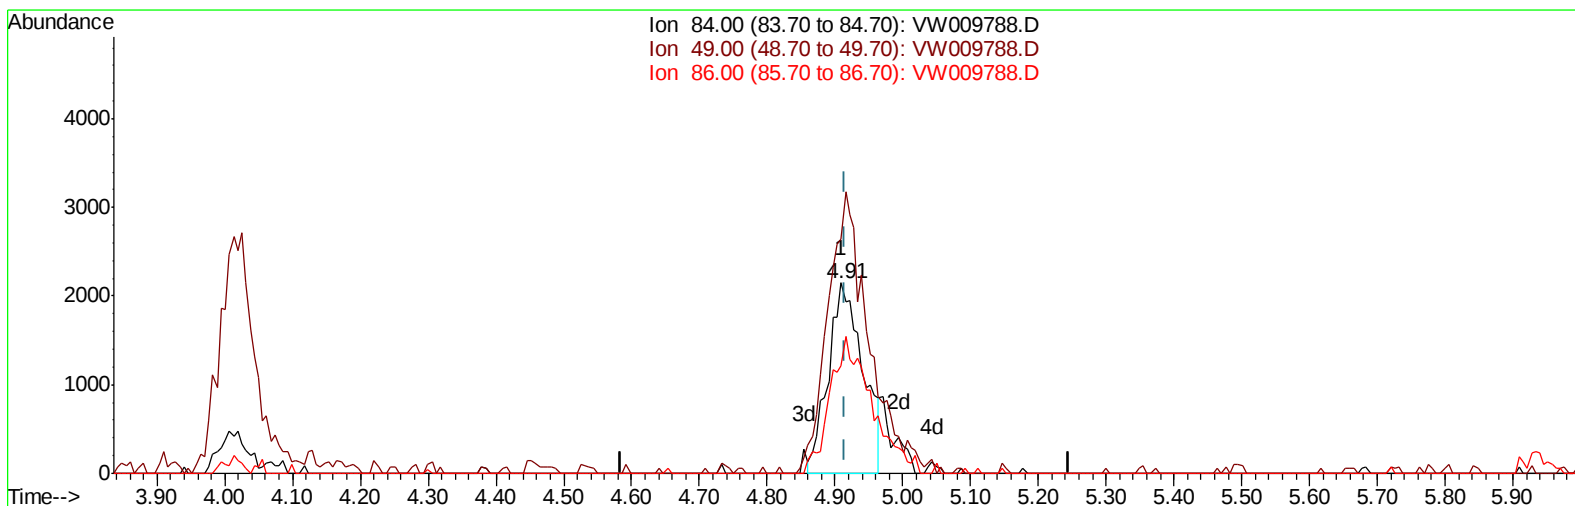

TIC: VW009788.D

(16) Methylene chloride (T)

4.909min (-0.006) 1.10ug/L

response 7670

Ion	Exp%	Act%
84.00	100	100
49.00	140.40	123.20
86.00	66.30	56.64
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040619\
Data File : VW009788.D
Acq On : 06 Apr 2019 23:52
Operator : SY/VA
Sample : K2217-09
Misc : 5.82G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF618

Manual Integrations
APPROVED

MMDadoda
4/11/2019 11:43:18 AM

Quant Time: Apr 07 05:39:56 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Sun Apr 07 05:36:41 2019
Response via : Initial Calibration

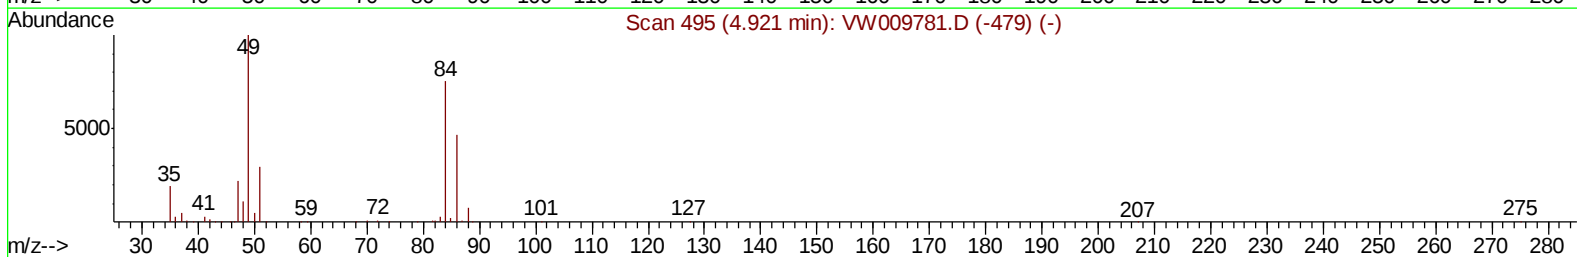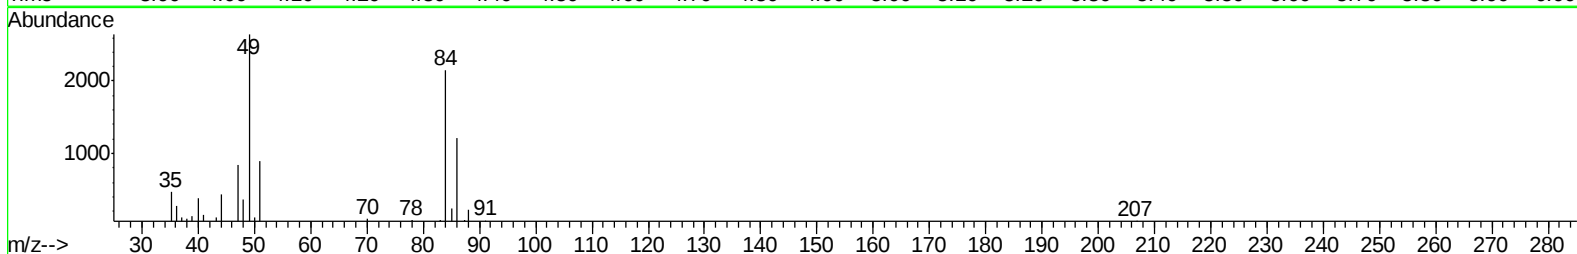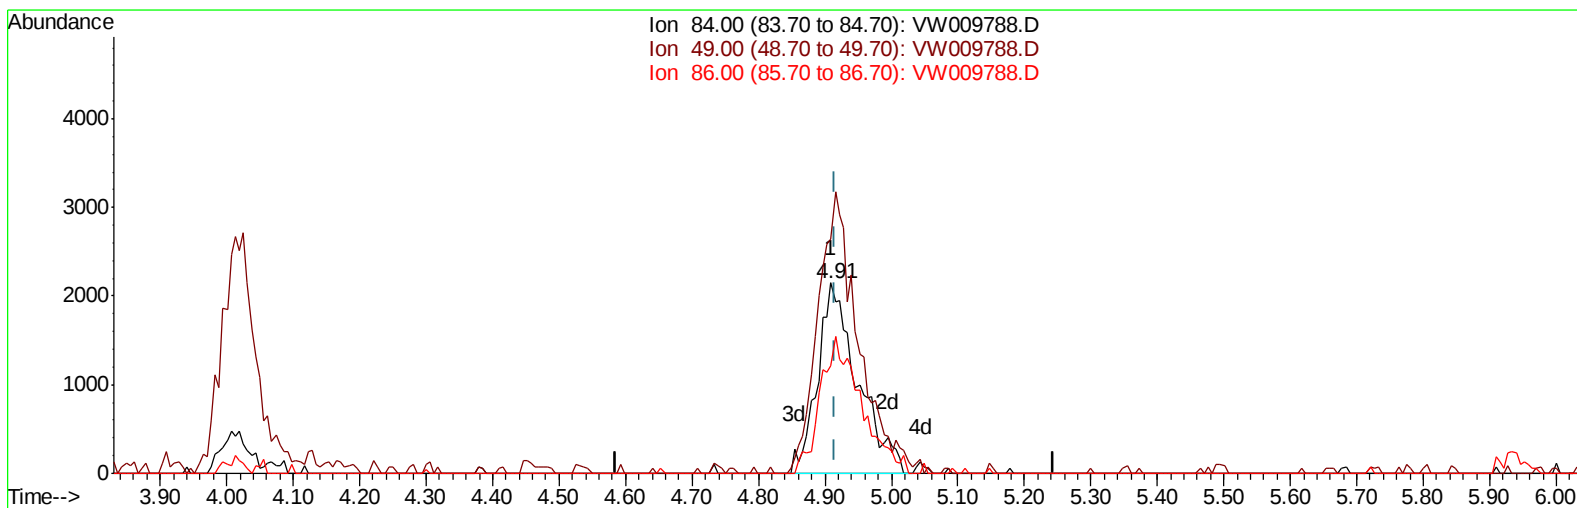

TIC: VW009788.D

(16) Methylene chloride (T)

4.909min (-0.006) 1.29ug/L m

response 8994

Ion	Exp%	Act%
84.00	100	100
49.00	140.40	123.20
86.00	66.30	56.64
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040619\
 Data File : VW009788.D
 Acq On : 06 Apr 2019 23:52
 Operator : SY/VA
 Sample : K2217-09
 Misc : 5.82G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF618

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 11:43:18 AM

Quant Time: Apr 07 23:48:56 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Sun Apr 07 05:36:41 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	394851	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	372001	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	145113	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	149271	28.89	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	115.56%
7) Chloroethane-d5	2.89	69	141726	29.94	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	119.76%
10) 1,1-Dichloroethene-d2	4.01	63	262369	23.61	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	94.44%
20) 2-Butanone-d5	7.07	46	115111	68.62	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	137.24%#
24) Chloroform-d	7.65	84	359316	33.35	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	133.40%
26) 1,2-Dichloroethane-d4	8.30	65	233788	35.34	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	141.36%#
29) Benzene-d6	8.27	84	670262	34.32	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	137.28%#
33) 1,2-Dichloropropane-d6	9.27	67	214331	35.53	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	142.12%#
37) Toluene-d8	10.32	98	599237	33.19	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	132.76%#
38) trans-1,3-Dichloropropene-	10.58	79	87292	30.34	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	121.36%
39) 2-Hexanone-d5	10.93	63	74343	65.39	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	130.78%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	182358	32.52	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	130.08%#
61) 1,2-Dichlorobenzene-d4	13.85	152	184518	36.24	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	144.96%#

Target Compounds					Qvalue
13) Acetone	4.12	43	8402	4.674 ug/L	64
16) Methylene chloride	4.91	84	8994m	1.292 ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040619\
Data File : VW009788.D
Acq On : 06 Apr 2019 23:52
Operator : SY/VA
Sample : K2217-09
Misc : 5.82G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF618

Manual Integrations
APPROVED

MMDadoda
4/11/2019 11:43:18 AM

Quant Time: Apr 07 23:48:56 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Sun Apr 07 05:36:41 2019
Response via : Initial Calibration

