




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040619\
Data File : VW009801.D
Acq On : 07 Apr 2019 11:13
Operator : SY/VA
Sample : K2168-18
Misc : 4.89G/10ML/MSVOA_W/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF675

Manual Integrations
APPROVED

MMDadoda
4/11/2019 11:43:29 AM

Quant Time: Apr 08 00:54:39 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Mon Apr 08 00:51:56 2019
Response via : Initial Calibration

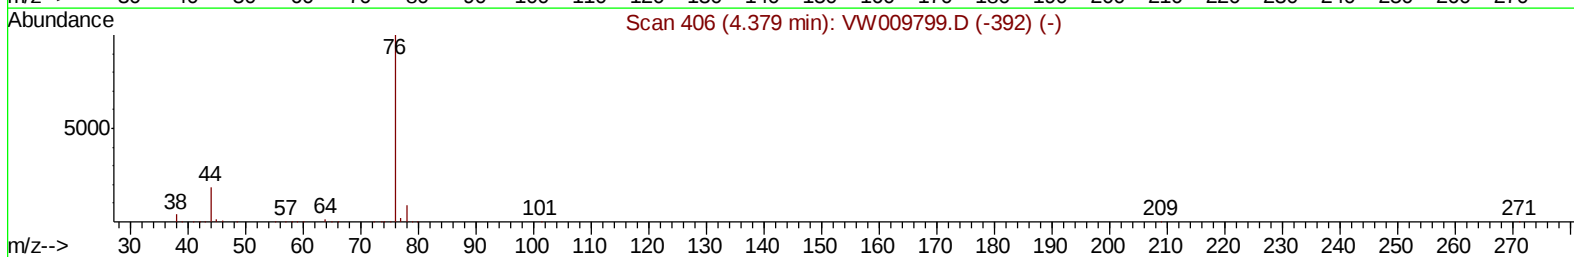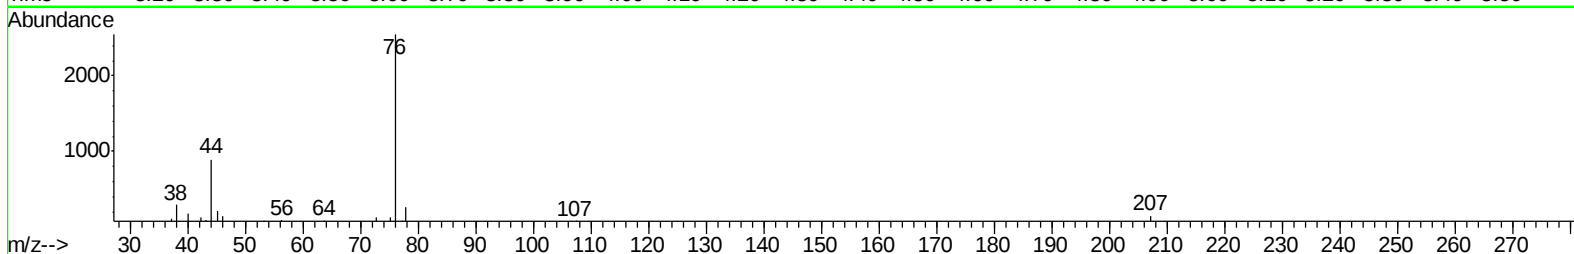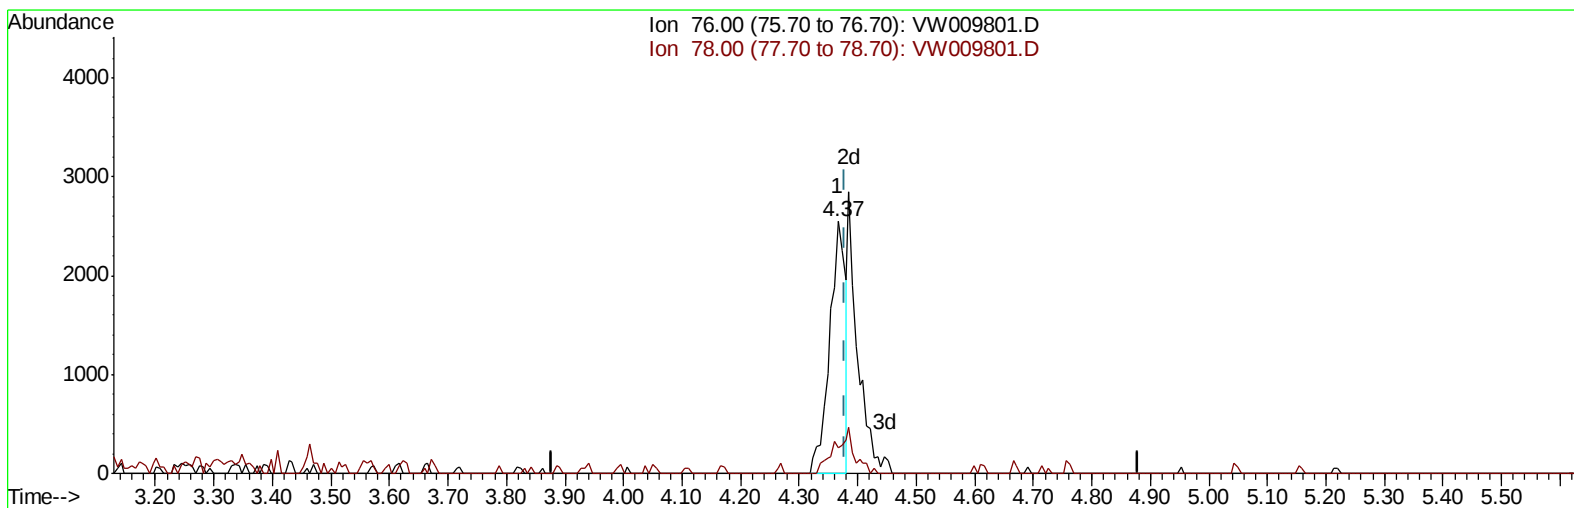

TIC: VW009801.D

(14) Carbon disulfide (T)

4.367min (-0.012) 0.39ug/L

response 4644

Ion	Exp%	Act%
76.00	100	100
78.00	9.10	10.05
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW040619\
Data File : VW009801.D
Acq On : 07 Apr 2019 11:13
Operator : SY/VA
Sample : K2168-18
Misc : 4.89G/10ML/MSVOA_W/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF675

Manual Integrations
APPROVED

MMDadoda
4/11/2019 11:43:29 AM

Quant Time: Apr 08 00:54:39 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Mon Apr 08 00:51:56 2019
Response via : Initial Calibration

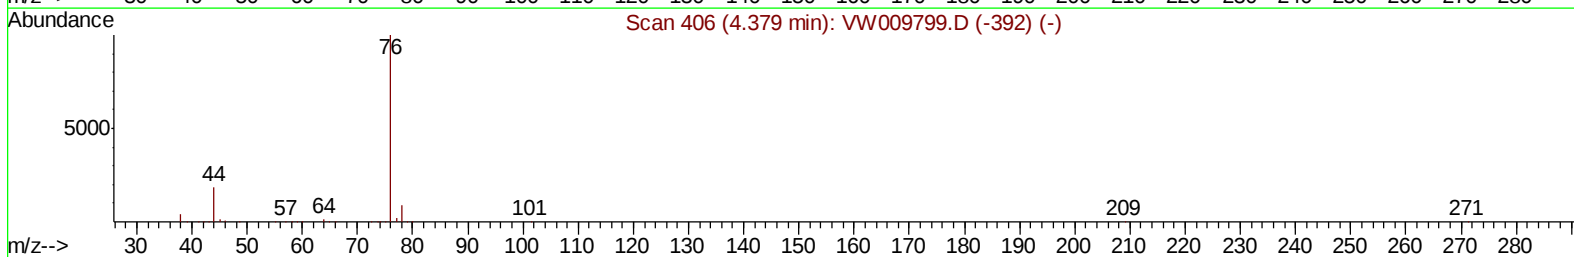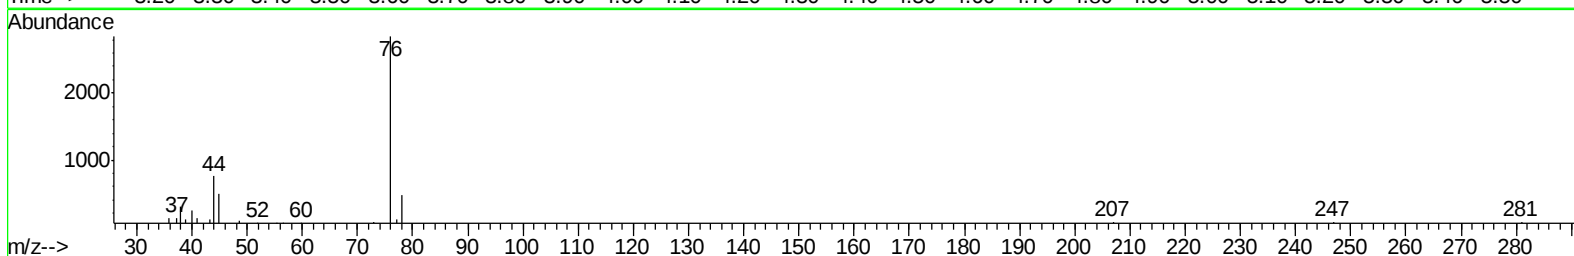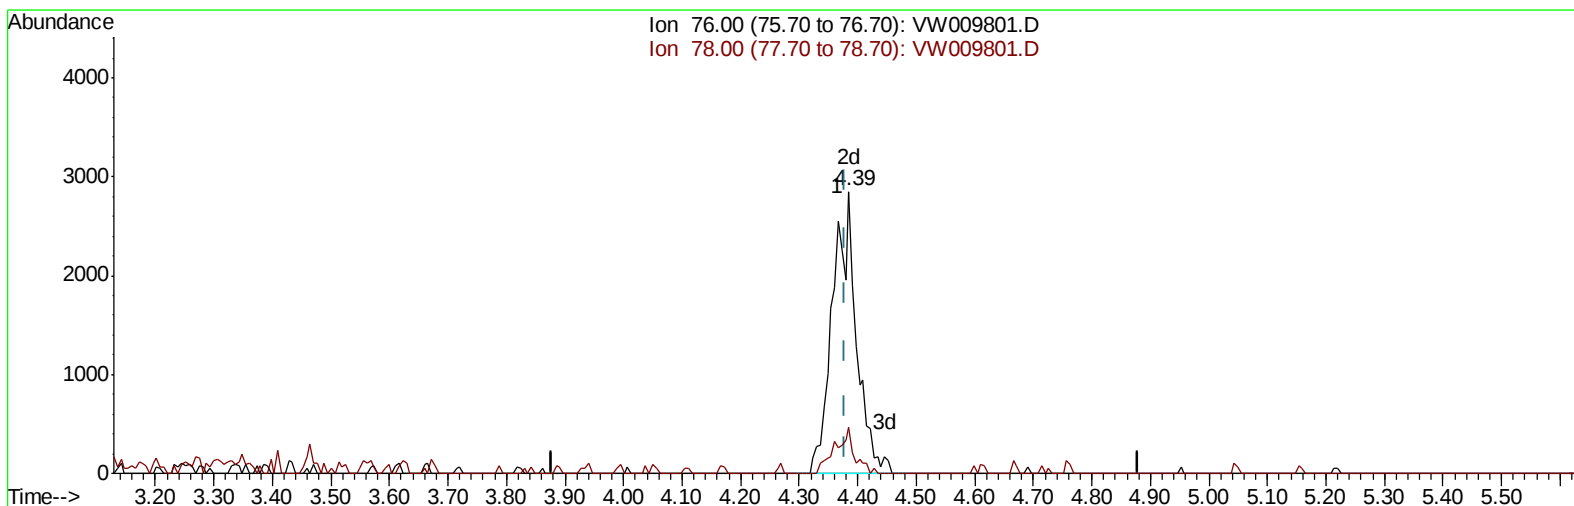

TIC: VW009801.D

(14) Carbon disulfide (T)

4.385min (+0.006) 0.68ug/L m

response 8114

Ion	Exp%	Act%
76.00	100	100
78.00	9.10	16.50#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040619\
Data File : VW009801.D
Acq On : 07 Apr 2019 11:13
Operator : SY/VA
Sample : K2168-18
Misc : 4.89G/10ML/MSVOA_W/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF675

Manual Integrations
APPROVED

MMDadoda
4/11/2019 11:43:29 AM

Quant Time: Apr 08 00:54:39 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Mon Apr 08 00:51:56 2019
Response via : Initial Calibration

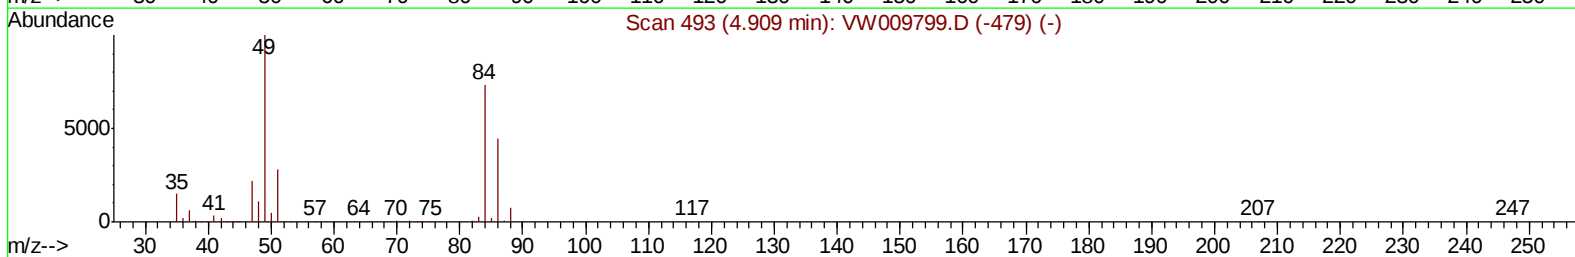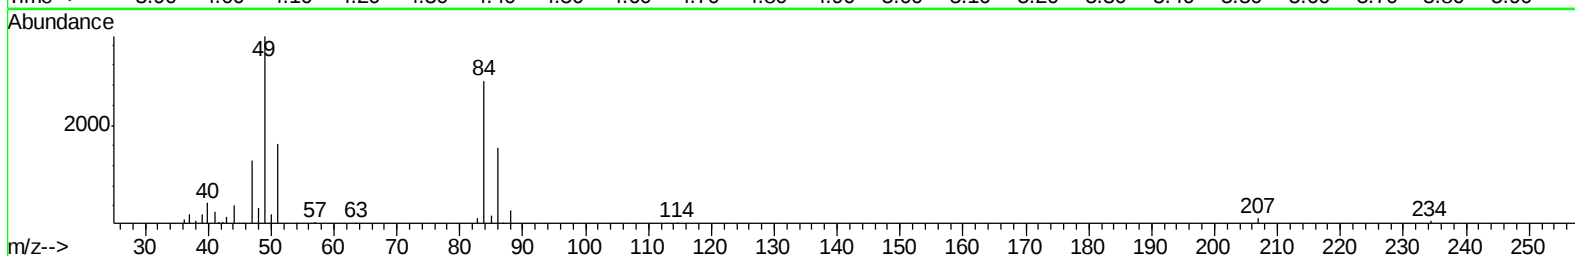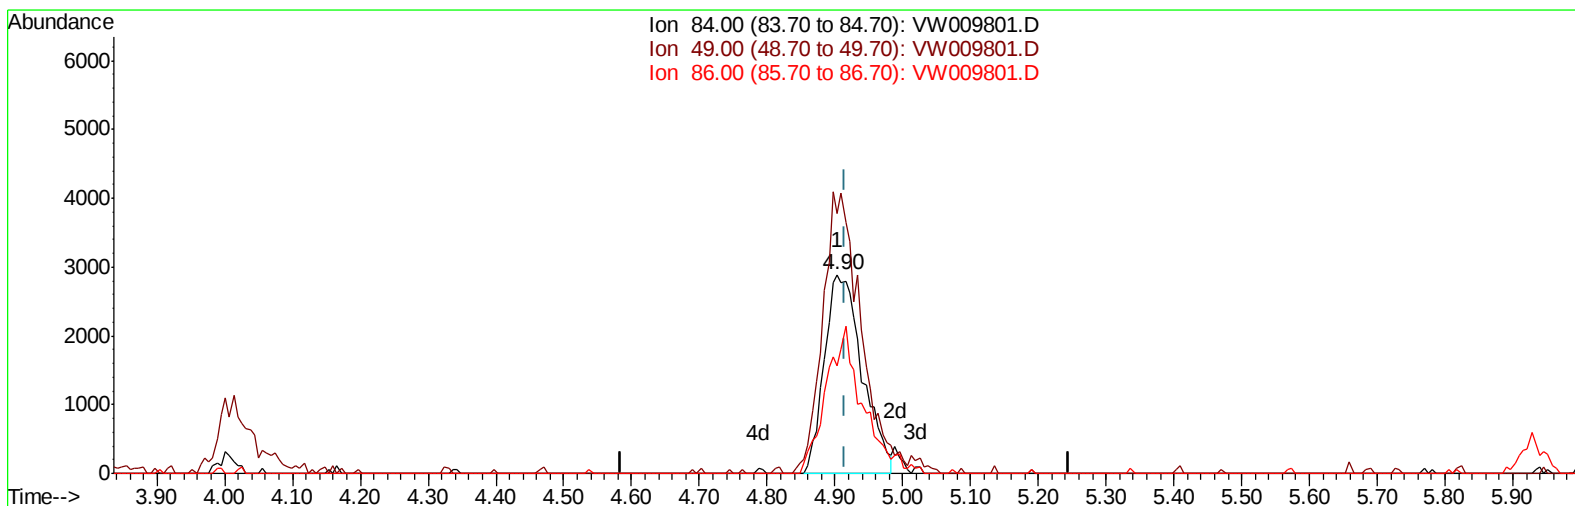

TIC: VW009801.D

(16) Methylene chloride (T)

4.903min (-0.012) 2.20ug/L

response 11197

Ion	Exp%	Act%
84.00	100	100
49.00	140.40	130.45
86.00	66.30	54.15
0.00	0.00	0.00




Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW040619\
Data File : VW009801.D
Acq On : 07 Apr 2019 11:13
Operator : SY/VA
Sample : K2168-18
Misc : 4.89G/10ML/MSVOA_W/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF675

Manual Integrations
APPROVED

MMDadoda
4/11/2019 11:43:29 AM

Quant Time: Apr 08 00:54:39 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Mon Apr 08 00:51:56 2019
Response via : Initial Calibration

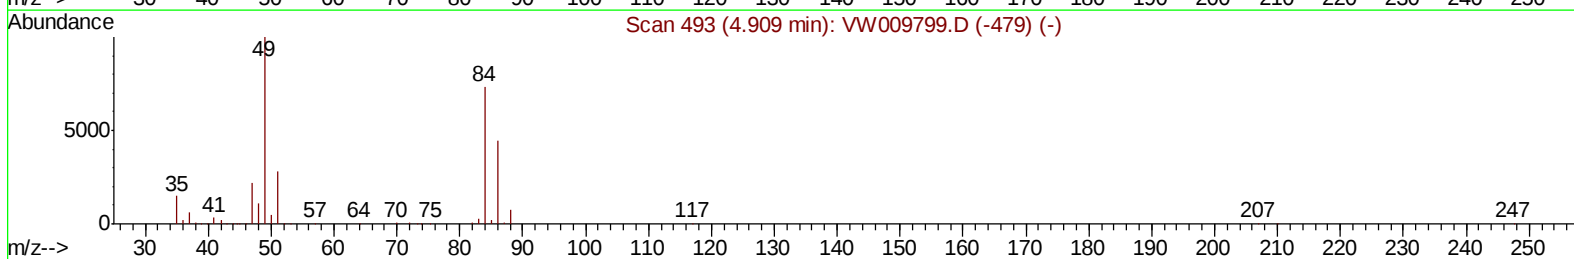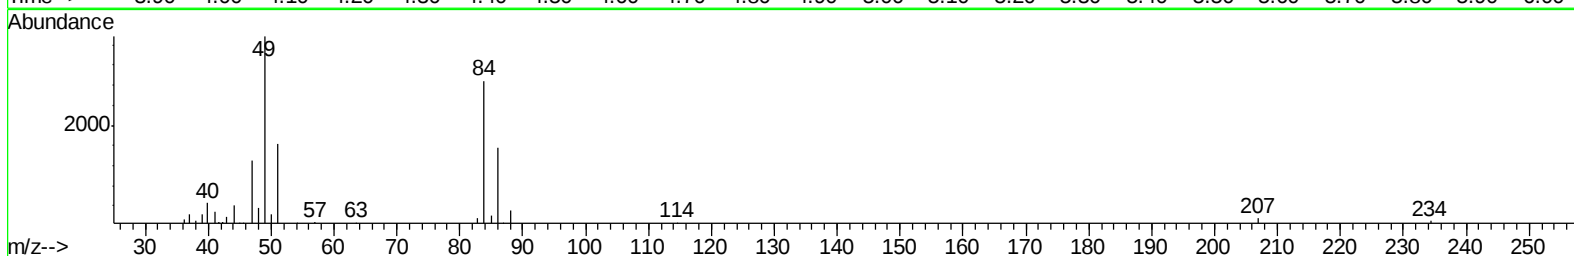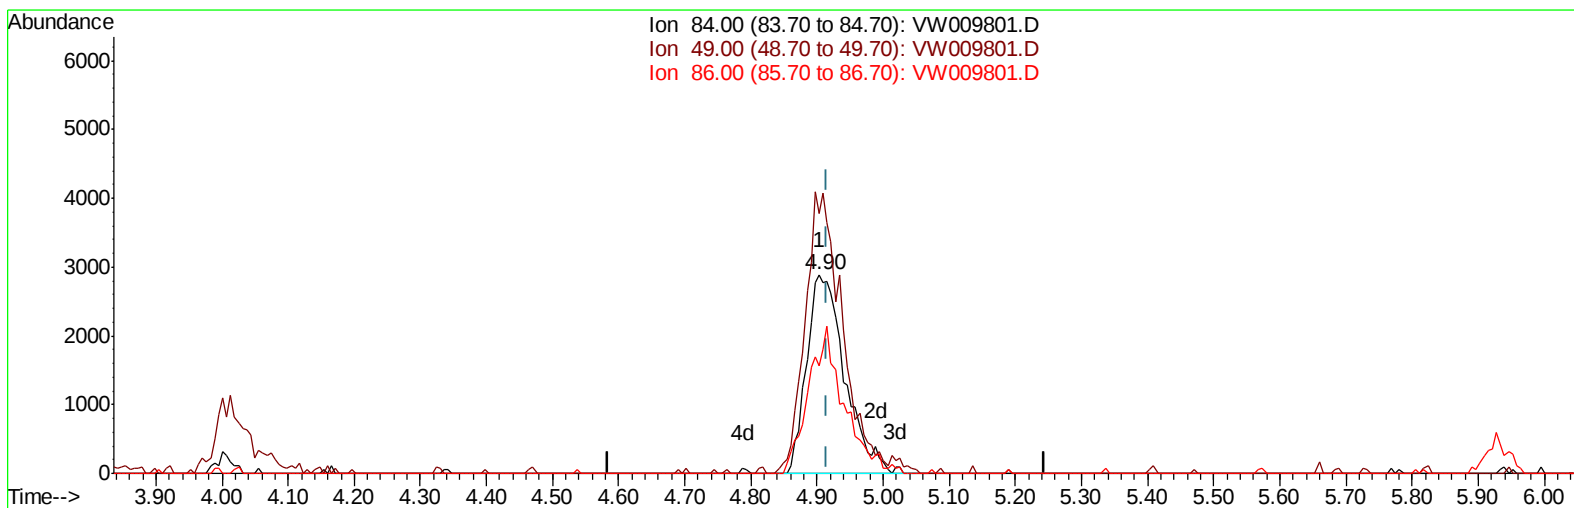

TIC: VW009801.D

(16) Methylene chloride (T)
4.903min (-0.012) 2.27ug/L m
response 11569

Ion	Exp%	Act%
84.00	100	100
49.00	140.40	130.45
86.00	66.30	54.15
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040619\
 Data File : VW009801.D
 Acq On : 07 Apr 2019 11:13
 Operator : SY/VA
 Sample : K2168-18
 Misc : 4.89G/10ML/MSVOA_W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF675

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 11:43:29 AM

Quant Time: Apr 08 01:03:43 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M

Quant Title : VOC Analysis

QLast Update : Mon Apr 08 00:51:56 2019

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	288508	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	303369	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	114150	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	40348	10.69	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	42.76%
7) Chloroethane-d5	2.89	69	59868	17.31	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.24%
10) 1,1-Dichloroethene-d2	4.01	63	90374	11.13	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	44.52%#
20) 2-Butanone-d5	7.07	46	72389	59.05	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	118.10%
24) Chloroform-d	7.64	84	224068	28.46	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	113.84%
26) 1,2-Dichloroethane-d4	8.30	65	155834	32.24	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	128.96%
29) Benzene-d6	8.27	84	372011	23.36	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.44%
33) 1,2-Dichloropropane-d6	9.27	67	140866	28.64	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	114.56%
37) Toluene-d8	10.32	98	314749	21.38	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.52%
38) trans-1,3-Dichloropropene-	10.57	79	51456	21.93	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.72%
39) 2-Hexanone-d5	10.93	63	44145	47.61	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	95.22%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	109934	24.04	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	96.16%
61) 1,2-Dichlorobenzene-d4	13.85	152	110579	27.61	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	110.44%

Target Compounds

					Qvalue
13) Acetone	4.12	43	18369	13.986 ug/L	99
14) Carbon disulfide	4.39	76	8114m	0.681 ug/L	
16) Methylene chloride	4.90	84	11569m	2.274 ug/L	
21) 2-Butanone	7.18	43	3373	2.019 ug/L	92
53) Ethylbenzene	11.73	91	7791	0.354 ug/L	96
54) m,p-Xylene	11.83	106	13463	1.653 ug/L	98
55) o-xylene	12.16	106	7530	0.971 ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW040619\
Data File : VW009801.D
Acq On : 07 Apr 2019 11:13
Operator : SY/VA
Sample : K2168-18
Misc : 4.89G/10ML/MSVOA_W/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF675

Manual Integrations
APPROVED

MMDadoda
4/11/2019 11:43:29 AM

Quant Time: Apr 08 01:03:43 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Mon Apr 08 00:51:56 2019
Response via : Initial Calibration

