
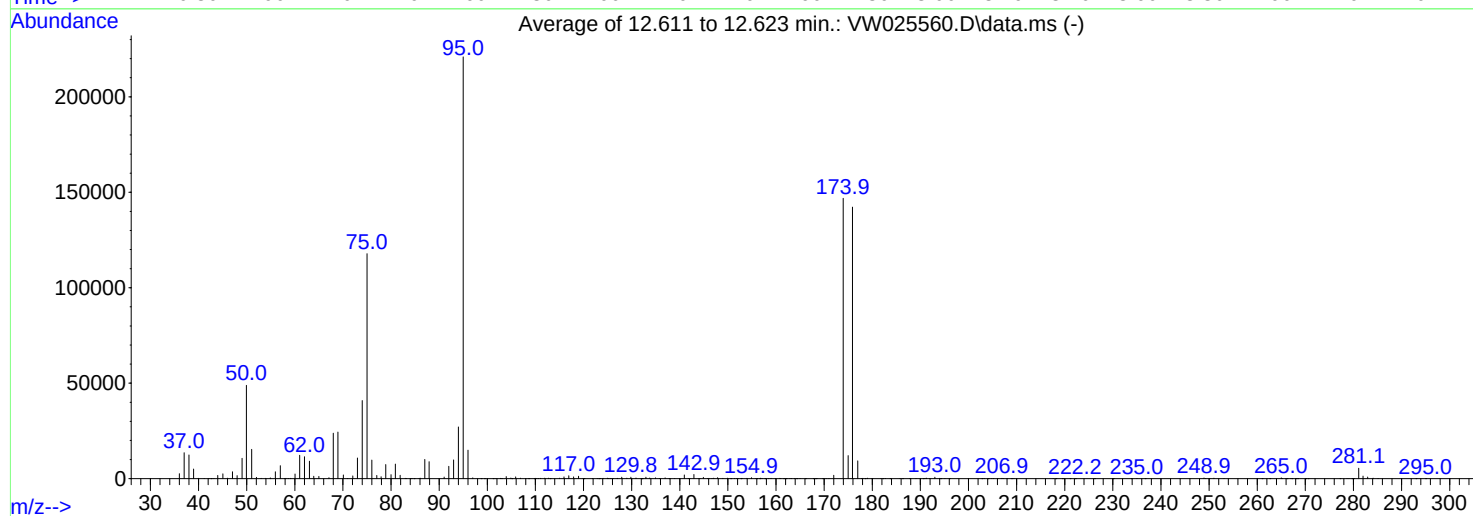


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040723\
 Data File : VW025560.D
 Acq On : 07 Apr 2023 07:29
 Operator : SY/MD
 Sample : BFB497
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB497

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022323WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Mar 23 01:48:30 2023

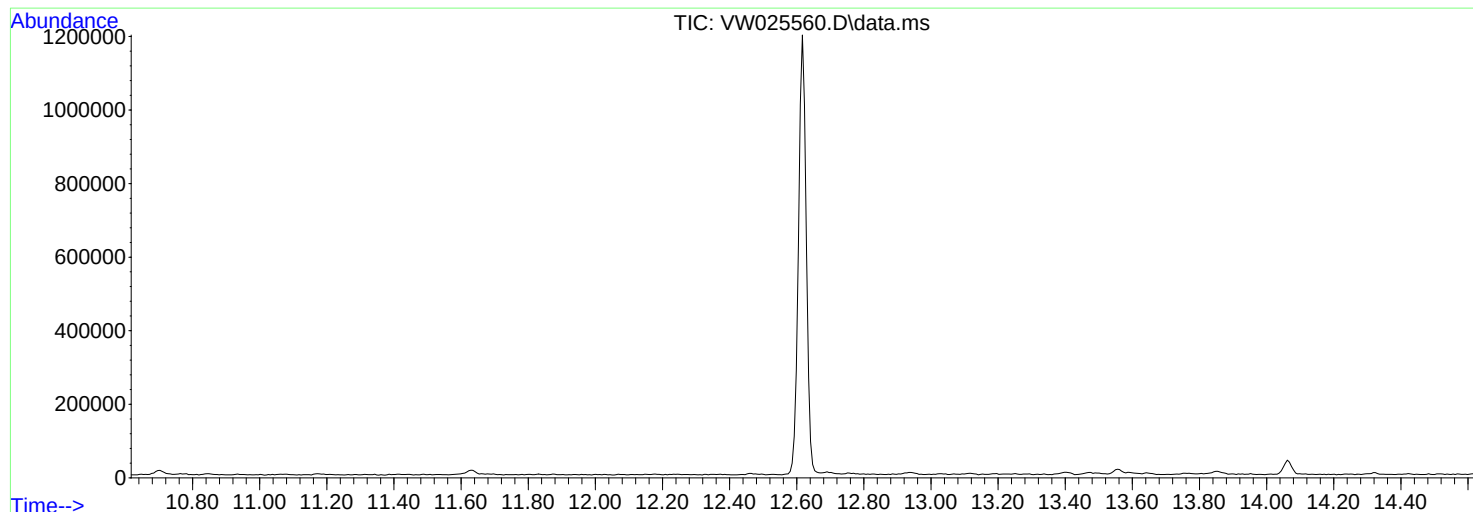

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	48867	PASS
75	95	30	80	53.3	117837	PASS
95	95	100	100	100.0	220949	PASS
96	95	5	9	6.8	14961	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	66.4	146808	PASS
175	174	5	9	8.3	12112	PASS
176	174	95	105	96.9	142200	PASS
177	176	5	10	6.5	9293	PASS