

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040822\
 Data File : VW022464.D
 Acq On : 08 Apr 2022 15:18
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK416

Quant Time: Apr 08 23:34:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 08 23:31:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	322102	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	322389	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	166911	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	149412	20.983	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.920%
7) Chloroethane-d5	2.892	69	98585	22.091	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.360%
11) 1,1-Dichloroethene-d2	4.019	63	142299	15.407	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	61.640%
21) 2-Butanone-d5	7.074	46	72203	58.079	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	116.160%
24) Chloroform-d	7.647	84	226822	22.529	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.120%
26) 1,2-Dichloroethane-d4	8.305	65	142941	24.849	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	99.400%
32) Benzene-d6	8.275	84	438260	22.250	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	89.000%
36) 1,2-Dichloropropane-d6	9.275	67	131778	23.119	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.480%
41) Toluene-d8	10.323	98	413349	21.427	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.720%
43) trans-1,3-Dichloroprop...	10.579	79	60315	22.421	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.680%
47) 2-Hexanone-d5	10.927	63	60421	56.974	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	113.940%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	122533	25.282	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	101.120%
66) 1,2-Dichlorobenzene-d4	13.847	152	140626	23.787	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.160%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	5954	0.716	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040822\
Data File : VW022464.D
Acq On : 08 Apr 2022 15:18
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK416

Quant Time: Apr 08 23:34:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 08 23:31:17 2022
Response via : Initial Calibration

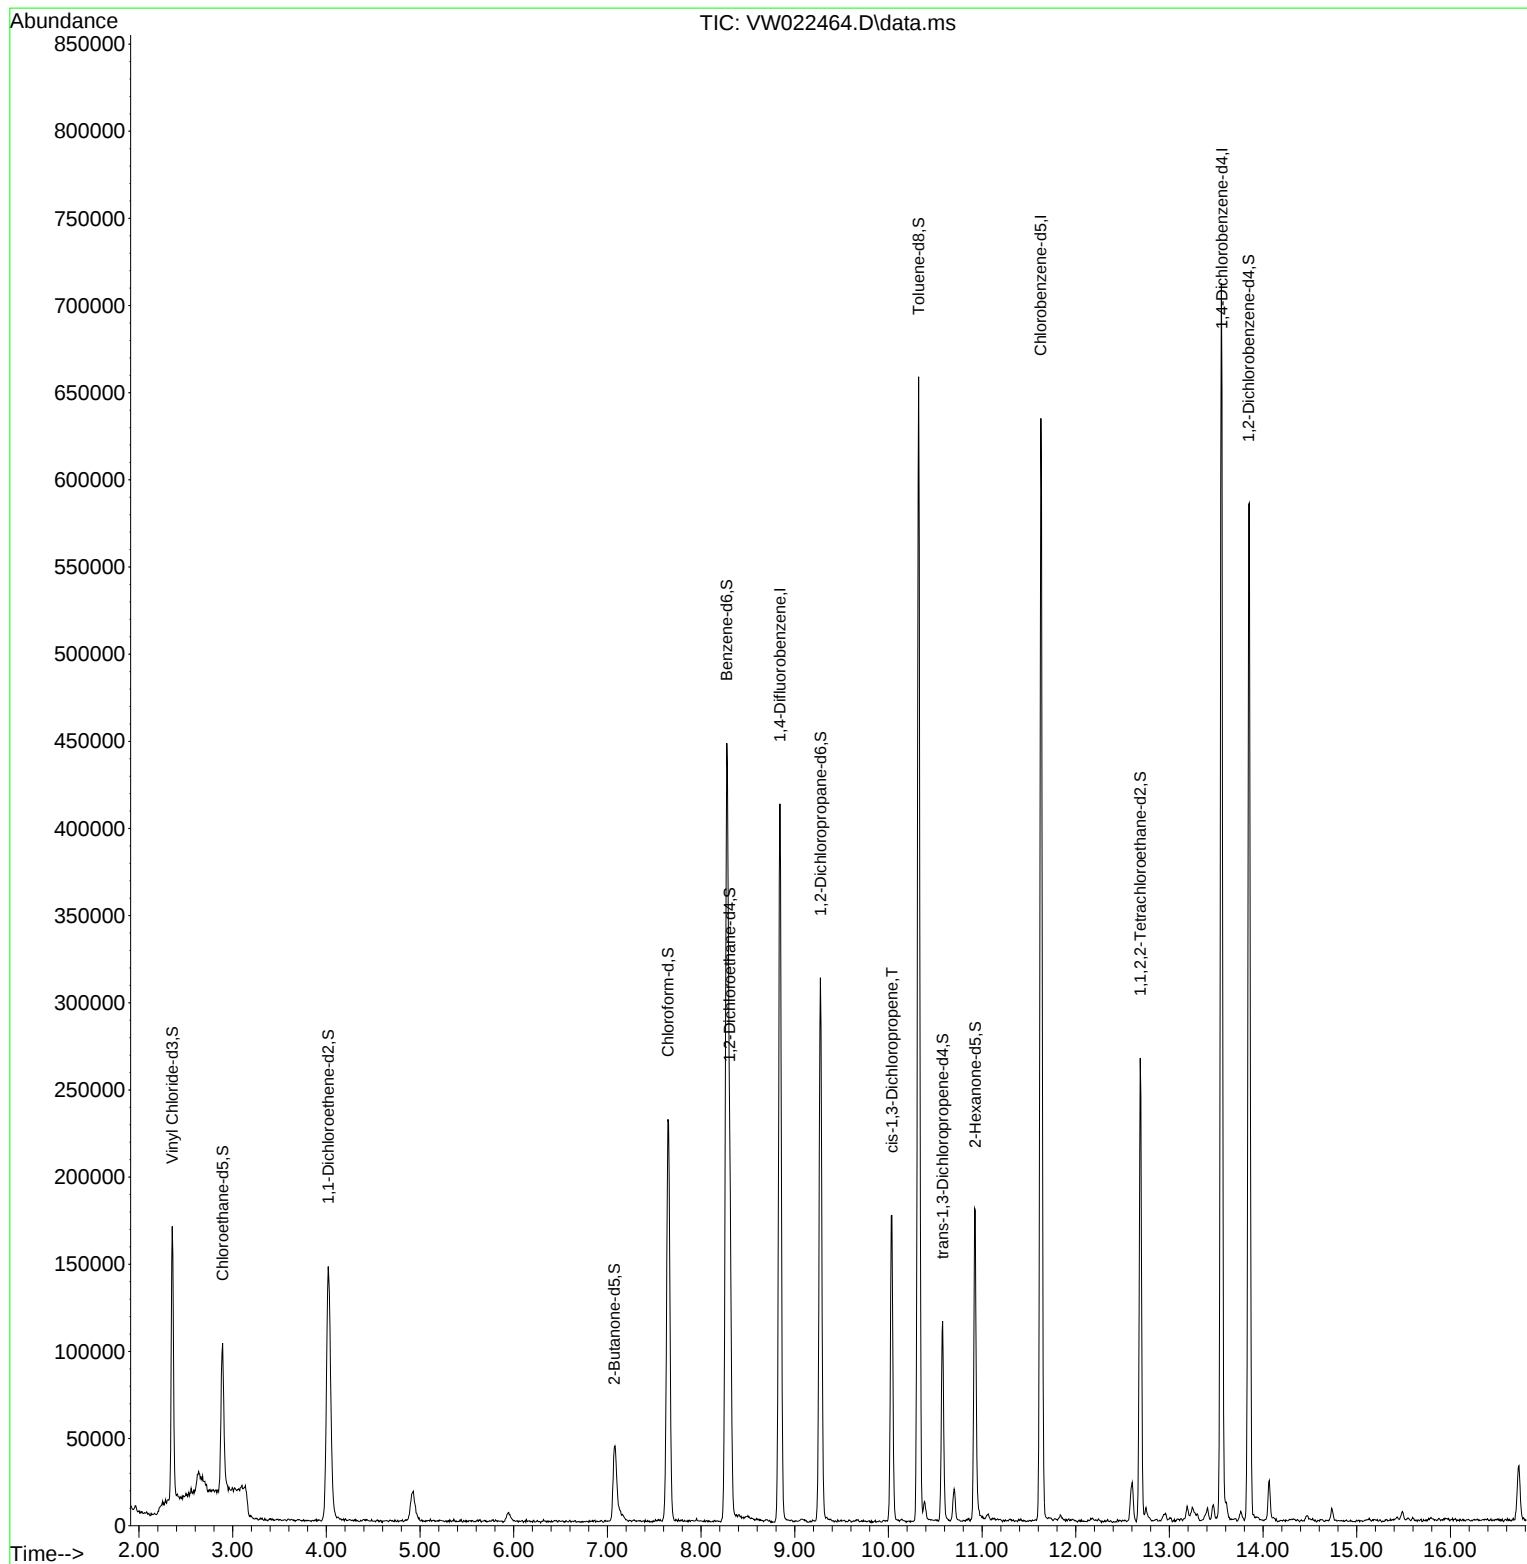

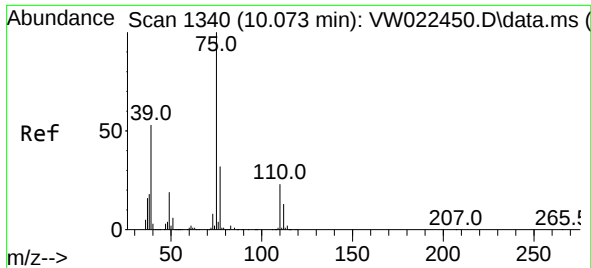

#39
 cis-1,3-Dichloropropene
 Concen: 0.716 ug/L
 RT: 10.037 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW022464.D
 Acq: 08 Apr 2022 15:18

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK416

Tgt Ion: 75 Resp: 5954
 Ion Ratio Lower Upper
 75 100
 77 39.1 22.6 42.0

