




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040822\
 Data File : VW022452.D
 Acq On : 08 Apr 2022 10:24
 Operator : SY/VA
 Sample : N2262-14RE
 Misc : 5.95g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6L4RE

Manual IntegrationsAPPROVED

Quant Time: Apr 08 23:32:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 08 23:31:17 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/09/2022
 Supervised By :Mahesh Dadoda 04/11/2022

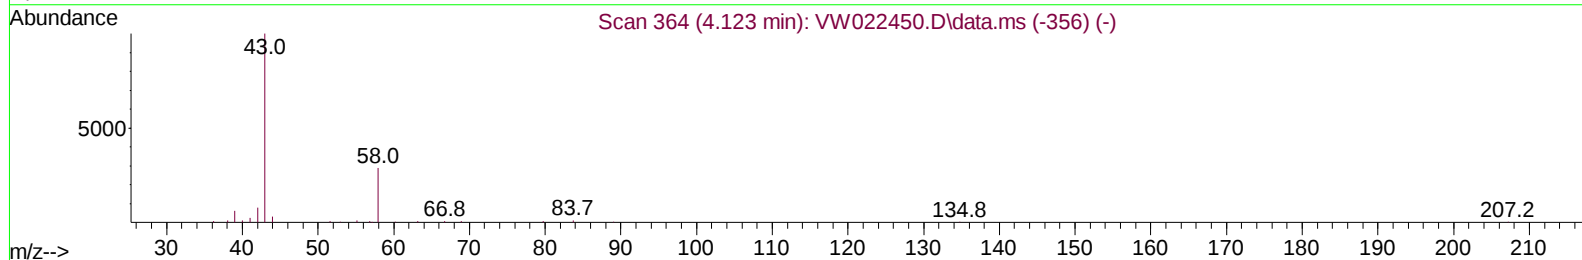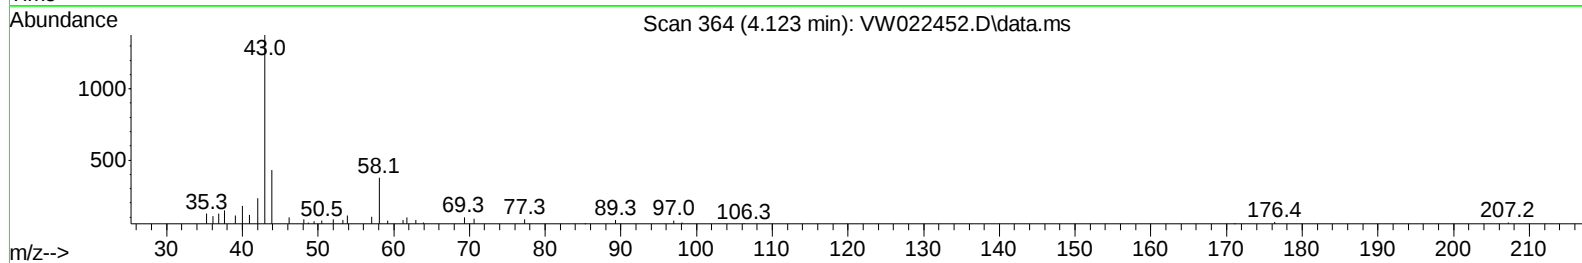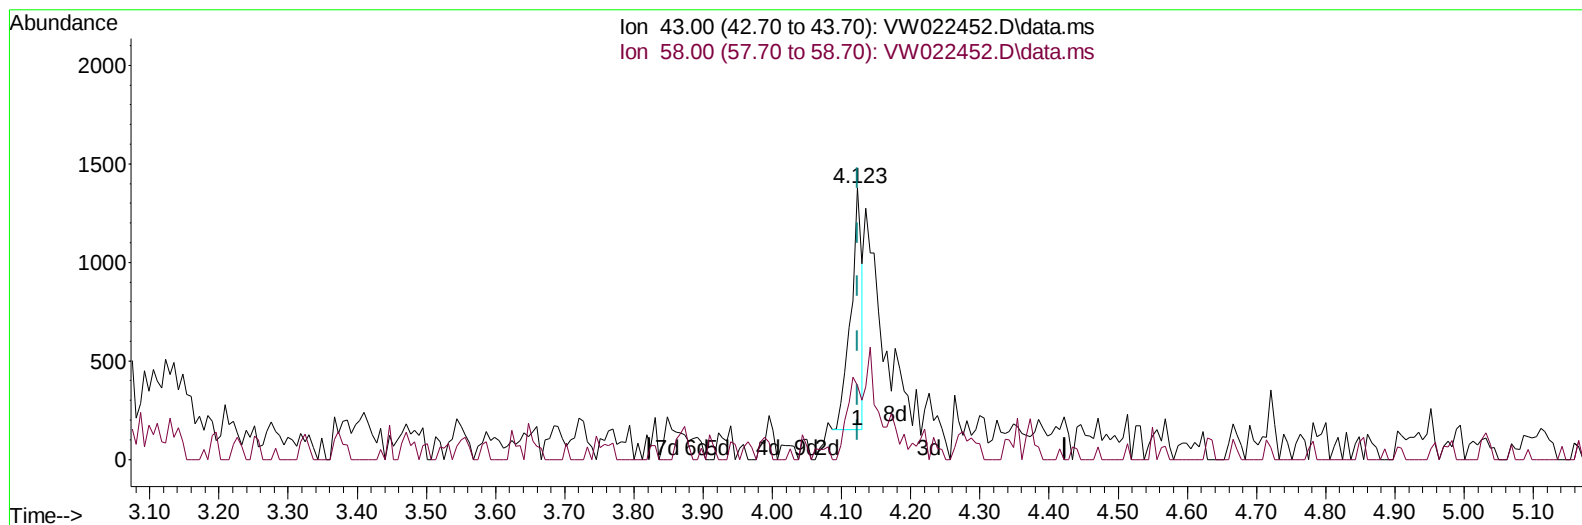

TIC: VW022452.D\data.ms

(13) Acetone (T)

4.123min (+ 0.000) 2.12 ug/L

response 1340

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	44.93
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040822\
 Data File : VW022452.D
 Acq On : 08 Apr 2022 10:24
 Operator : SY/VA
 Sample : N2262-14RE
 Misc : 5.95g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6L4RE

Manual IntegrationsAPPROVED

Quant Time: Apr 08 23:32:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 08 23:31:17 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/09/2022
 Supervised By :Mahesh Dadoda 04/11/2022

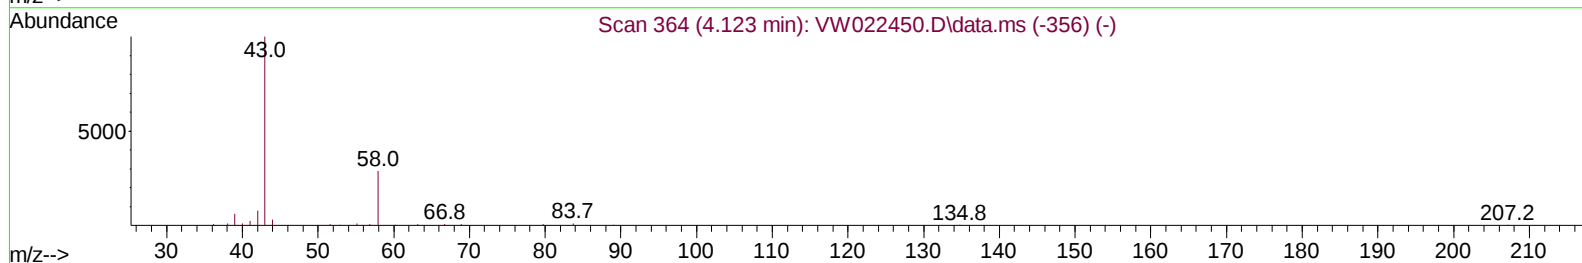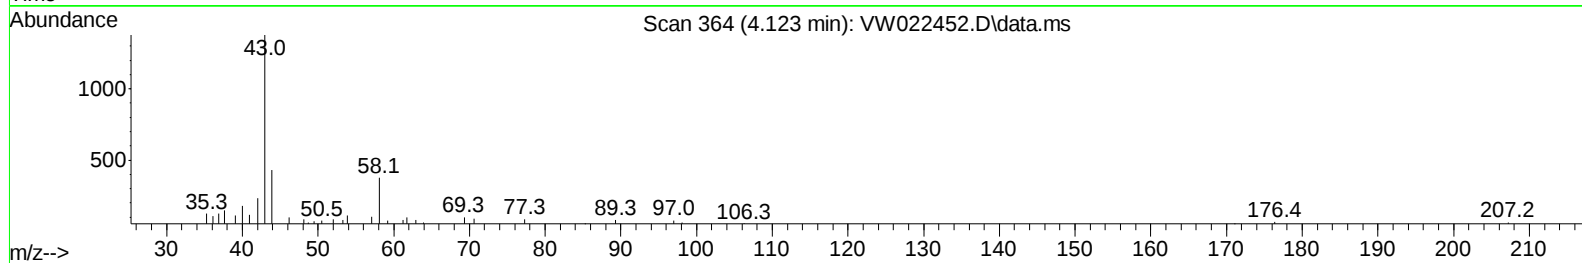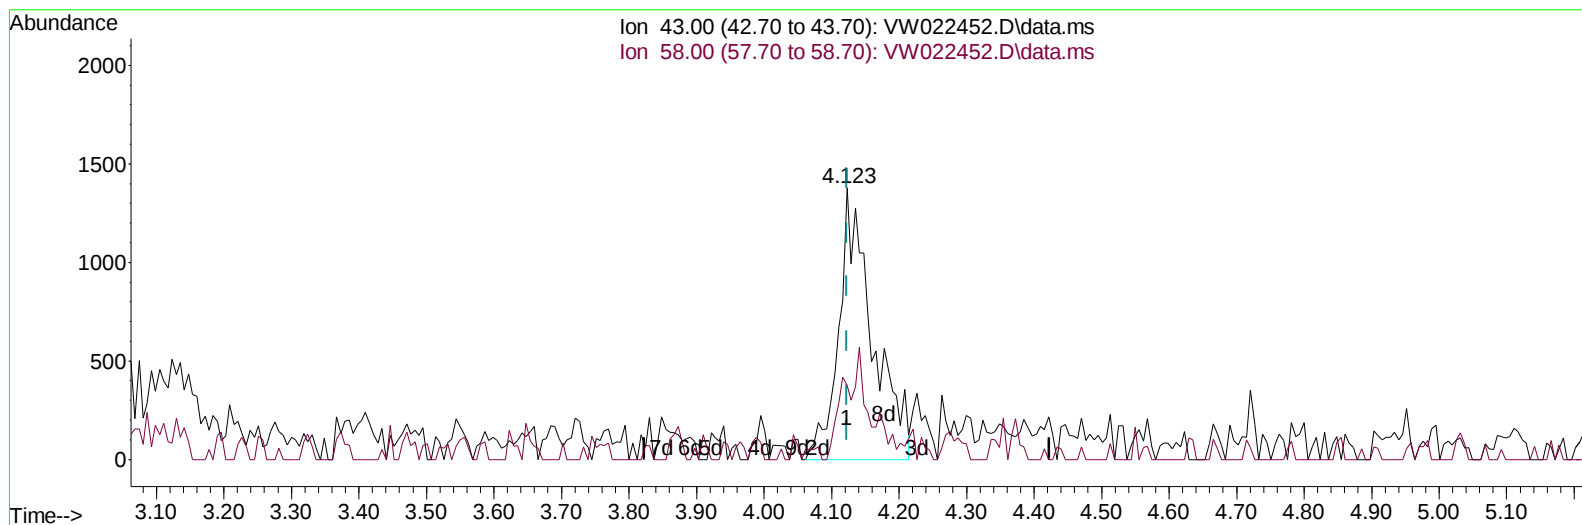

TIC: VW022452.D\data.ms

(13) Acetone (T)

4.123min (+ 0.000) 7.56 ug/L m

response 4773

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	12.61
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040822\
 Data File : VW022452.D
 Acq On : 08 Apr 2022 10:24
 Operator : SY/VA
 Sample : N2262-14RE
 Misc : 5.95g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6L4RE

Manual IntegrationsAPPROVED

Quant Time: Apr 08 23:32:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 08 23:31:17 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/09/2022
 Supervised By :Mahesh Dadoda 04/11/2022

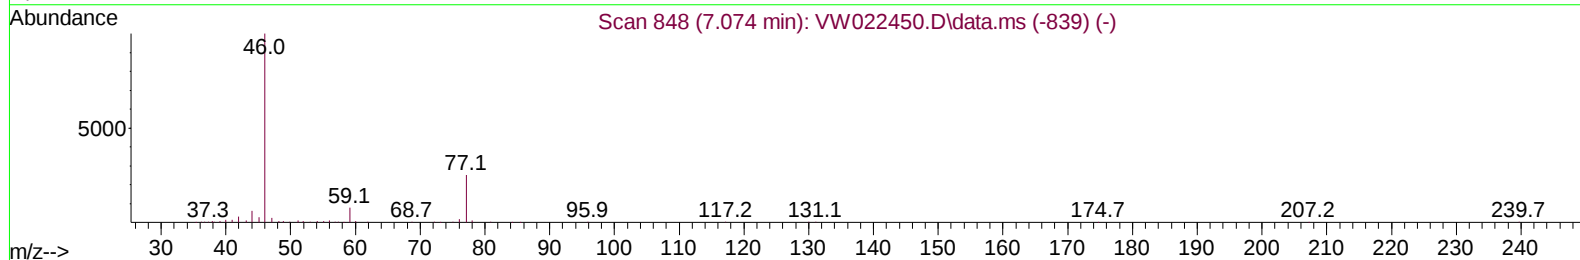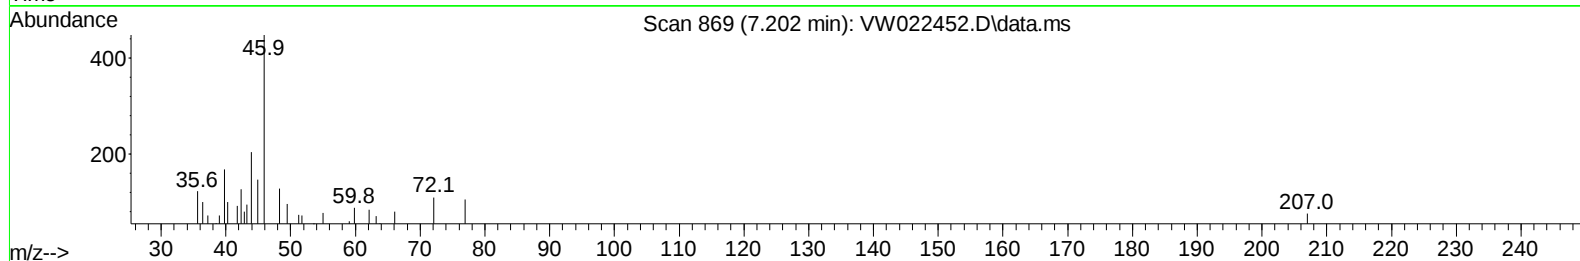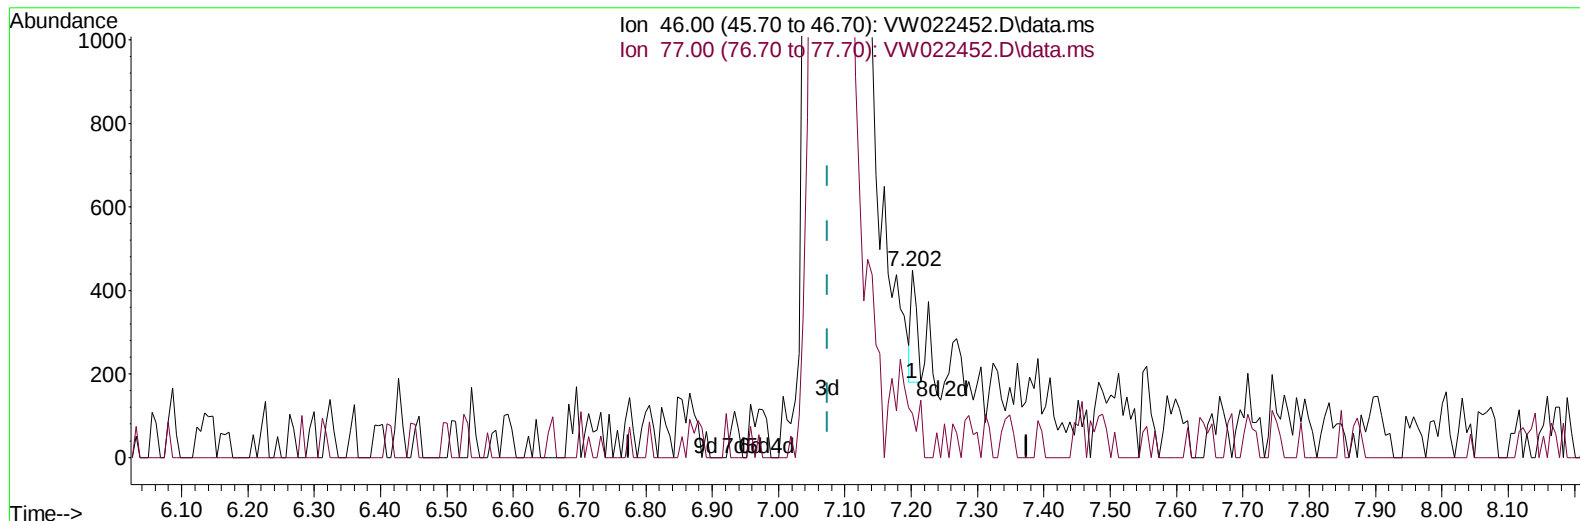

TIC: VW022452.D\data.ms

(21) 2-Butanone-d5 (S)

7.202min (+ 0.128) 0.18 ug/L

response 164

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	24.70	30.49
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040822\
 Data File : VW022452.D
 Acq On : 08 Apr 2022 10:24
 Operator : SY/VA
 Sample : N2262-14RE
 Misc : 5.95g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6L4RE

Manual IntegrationsAPPROVED

Quant Time: Apr 08 23:32:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 08 23:31:17 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/09/2022
 Supervised By :Mahesh Dadoda 04/11/2022

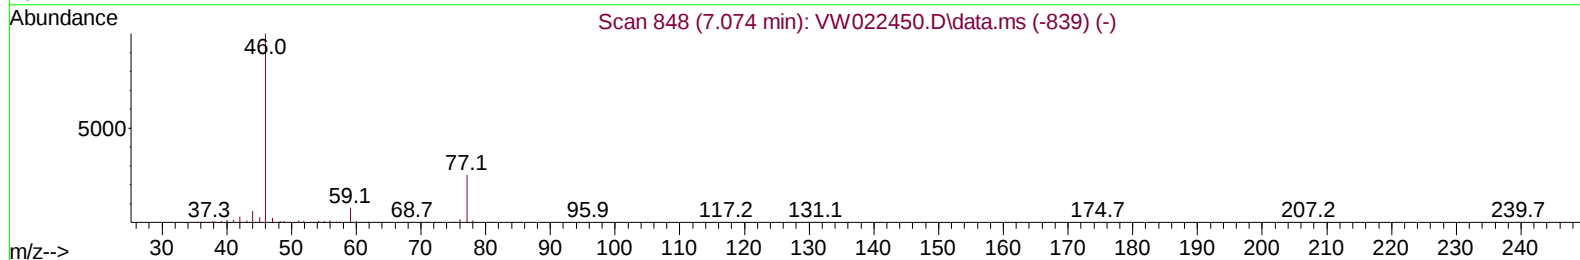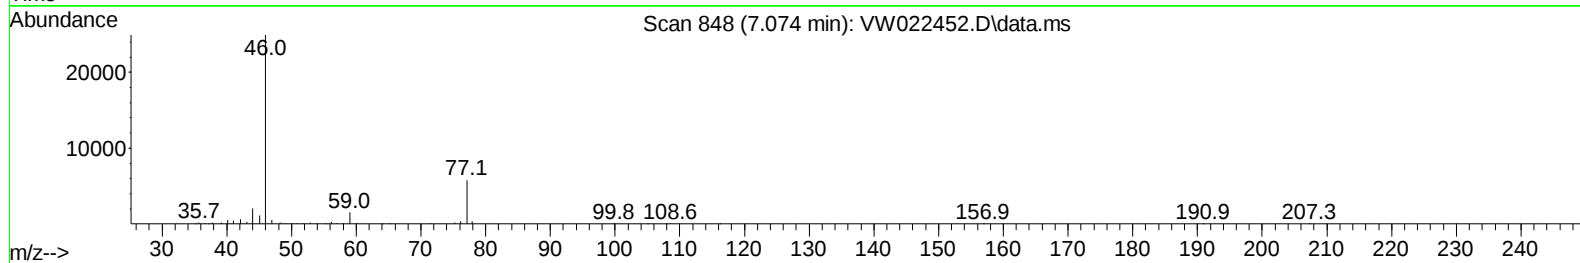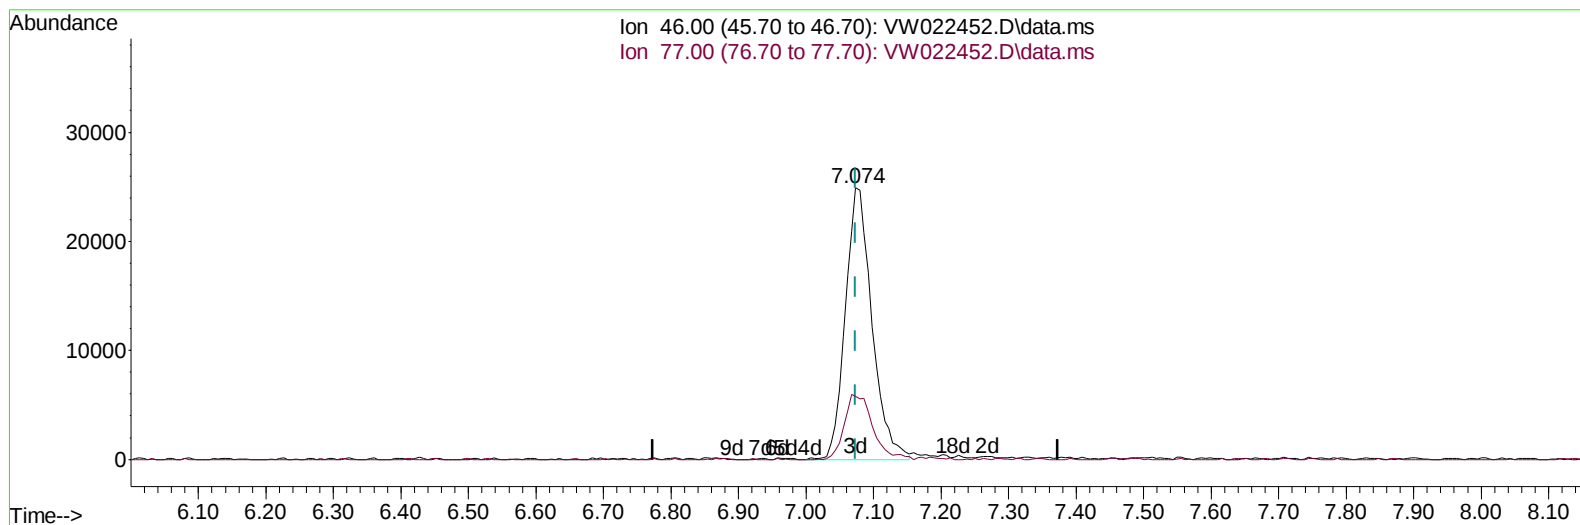

TIC: VW022452.D\data.ms

(21) 2-Butanone-d5 (S)

7.074min (+ 0.000) 73.42 ug/L m

response 68096

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	24.70	0.07#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040822\
Data File : VW022452.D
Acq On : 08 Apr 2022 10:24
Operator : SY/VA
Sample : N2262-14RE
Misc : 5.95g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW6L4RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
Supervised By :Mahesh Dadoda 04/11/2022

Quant Time: Apr 08 23:32:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 08 23:31:17 2022
Response via : Initial Calibration

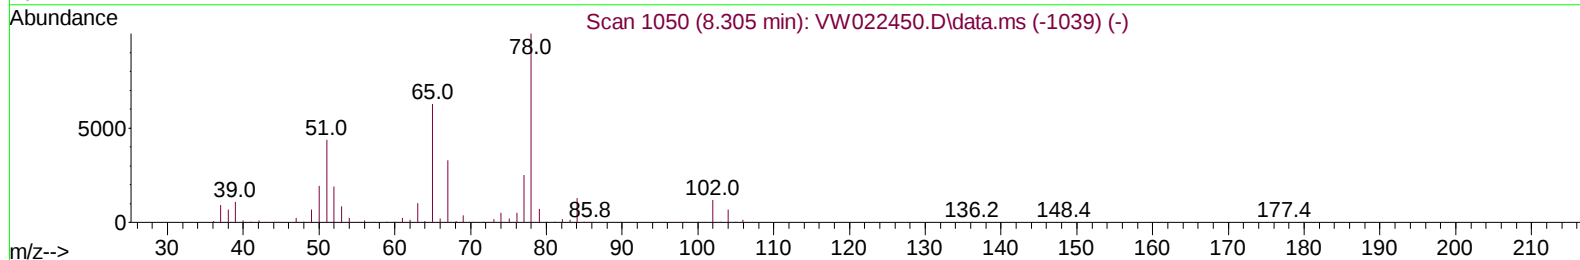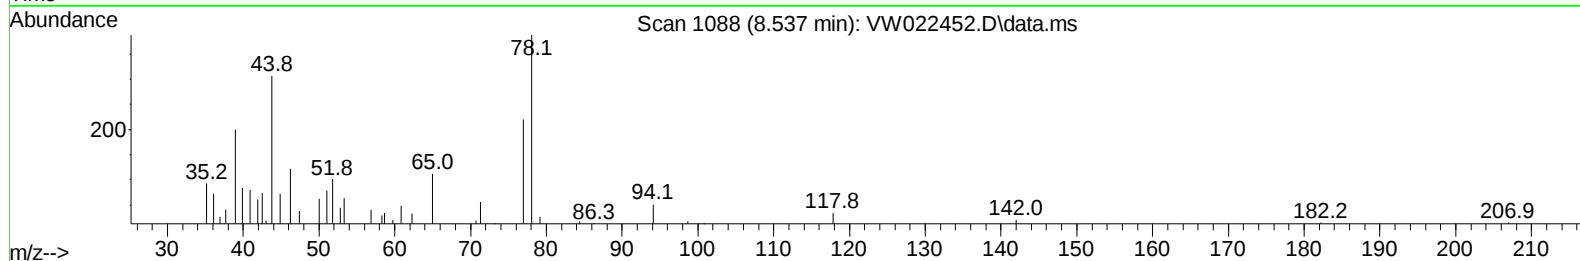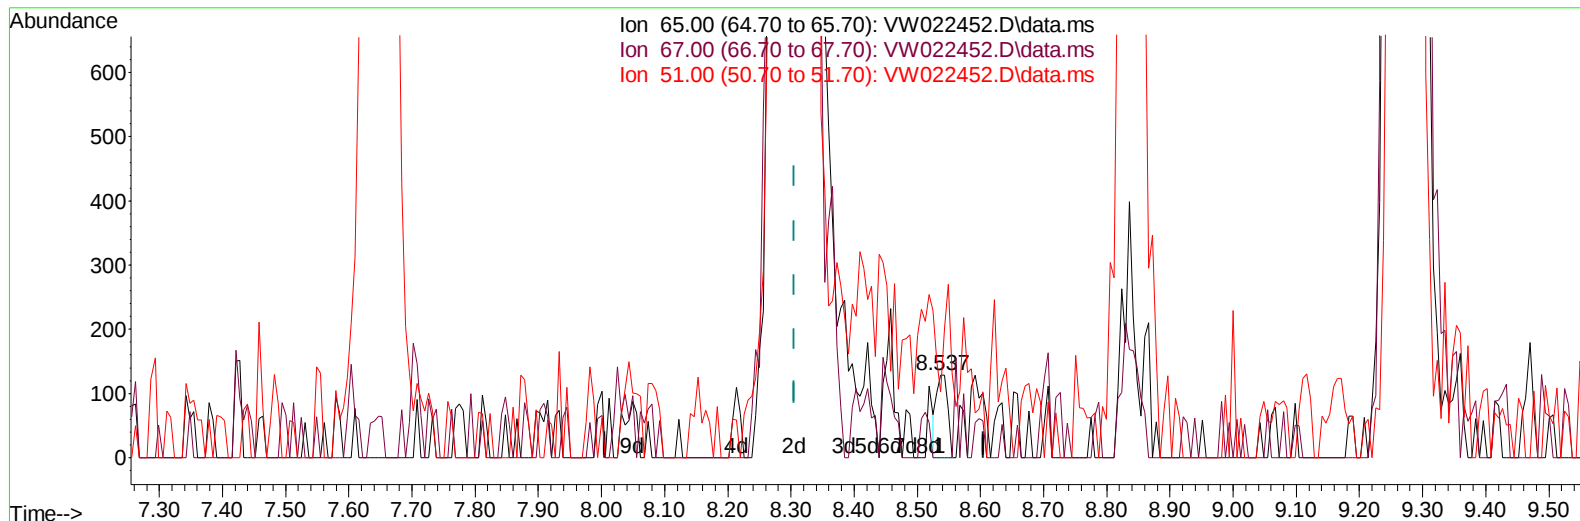

TIC: VW022452.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.537min (+ 0.232) 0.04 ug/L

response 159

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	35.85
51.00	99.30	83.02
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040822\
Data File : VW022452.D
Acq On : 08 Apr 2022 10:24
Operator : SY/VA
Sample : N2262-14RE
Misc : 5.95g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW6L4RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
Supervised By :Mahesh Dadoda 04/11/2022

Quant Time: Apr 08 23:32:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 08 23:31:17 2022
Response via : Initial Calibration

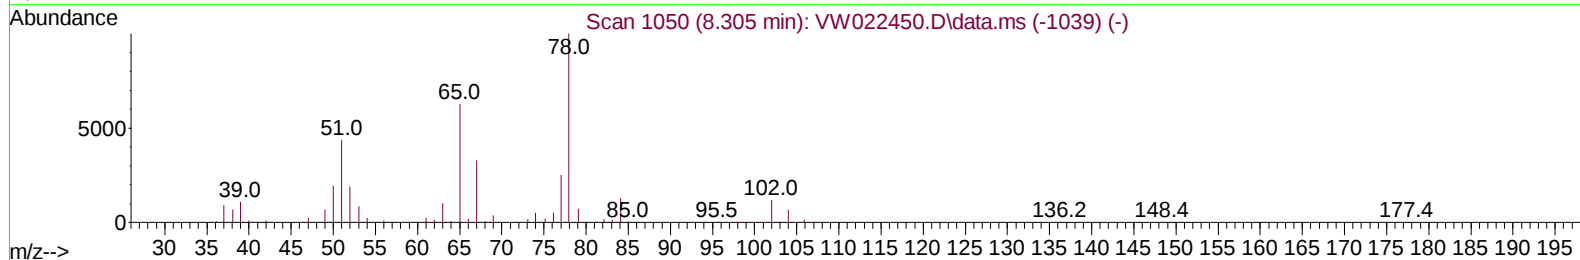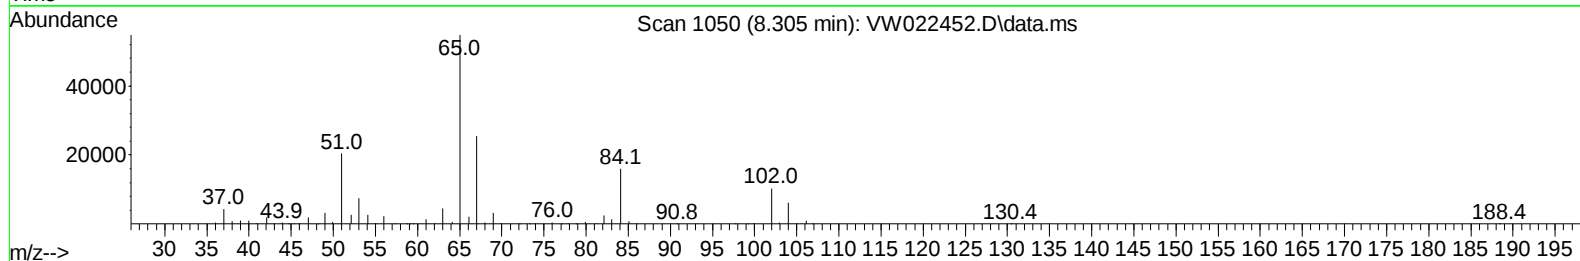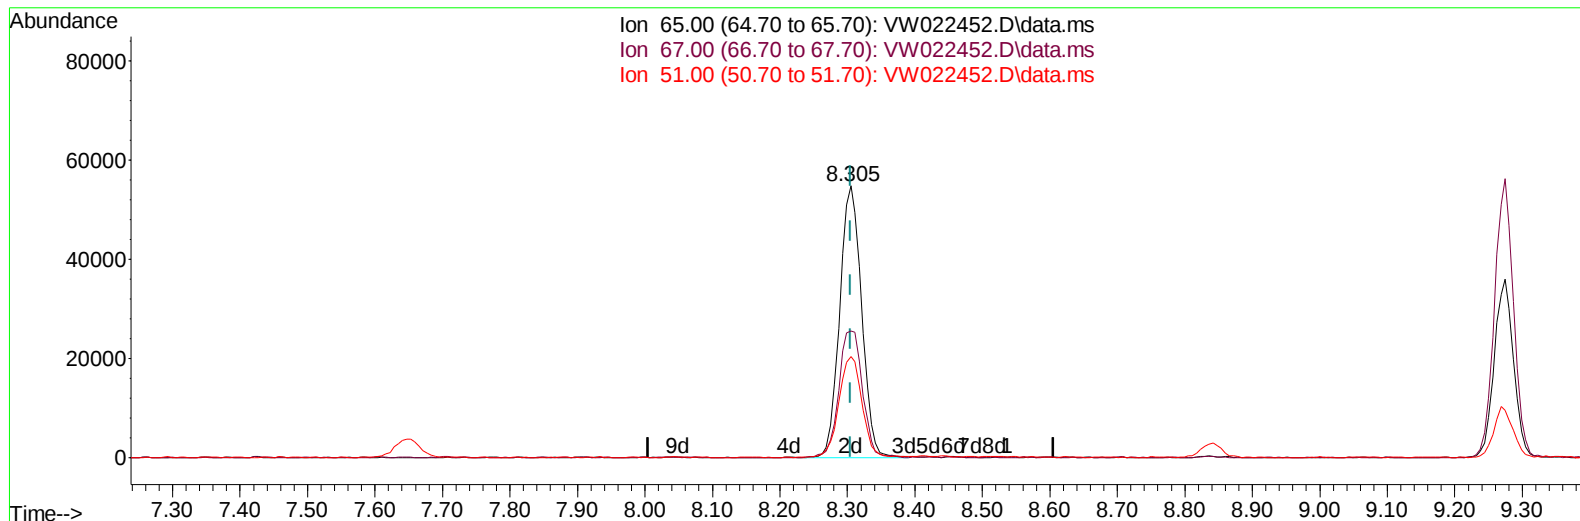

TIC: VW022452.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+ 0.000) 28.76 ug/L m

response 123416

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	49.70	0.05#
51.00	99.30	0.11#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040822\
 Data File : VW022452.D
 Acq On : 08 Apr 2022 10:24
 Operator : SY/VA
 Sample : N2262-14RE
 Misc : 5.95g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW6L4RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
 Supervised By :Mahesh Dadoda 04/11/2022

Quant Time: Apr 08 23:32:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 08 23:31:17 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		240307	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		202553	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		74728	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		118866	22.375	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	89.480%	
7) Chloroethane-d5	2.885	69		79377	23.841	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	95.360%	
11) 1,1-Dichloroethene-d2	4.019	63		115415	16.750	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	67.000%	
21) 2-Butanone-d5	7.074	46		68096m	73.420	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	146.840%#	
24) Chloroform-d	7.647	84		193960	25.823	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	103.280%	
26) 1,2-Dichloroethane-d4	8.305	65		123416m	28.757	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	115.040%	
32) Benzene-d6	8.275	84		340370	27.504	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	110.000%	
36) 1,2-Dichloropropane-d6	9.275	67		110206	30.773	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	123.080%#	
41) Toluene-d8	10.323	98		302675	24.973	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	99.880%	
43) trans-1,3-Dichloroprop...	10.579	79		47548	28.133	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	112.520%	
47) 2-Hexanone-d5	10.921	63		52100	78.193	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	156.380%#	
56) 1,1,2,2-Tetrachloroeth...	12.689	84		103074	33.849	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	135.400%#	
66) 1,2-Dichlorobenzene-d4	13.853	152		68948	26.049	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	104.200%	
Target Compounds							
13) Acetone	4.123	43		4773m	7.558	ug/L	
46) Tetrachloroethene	10.860	164		4253	1.571	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040822\
Data File : VW022452.D
Acq On : 08 Apr 2022 10:24
Operator : SY/VA
Sample : N2262-14RE
Misc : 5.95g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW6L4RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/09/2022
Supervised By :Mahesh Dadoda 04/11/2022

Quant Time: Apr 08 23:32:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 08 23:31:17 2022
Response via : Initial Calibration

