


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040822\
Data File : VW022449.D
Acq On : 08 Apr 2022 08:17
Operator : SY/VA
Sample : BFB530
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB530

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Title : SFAM01.0
Last Update : Fri Apr 08 23:31:17 2022

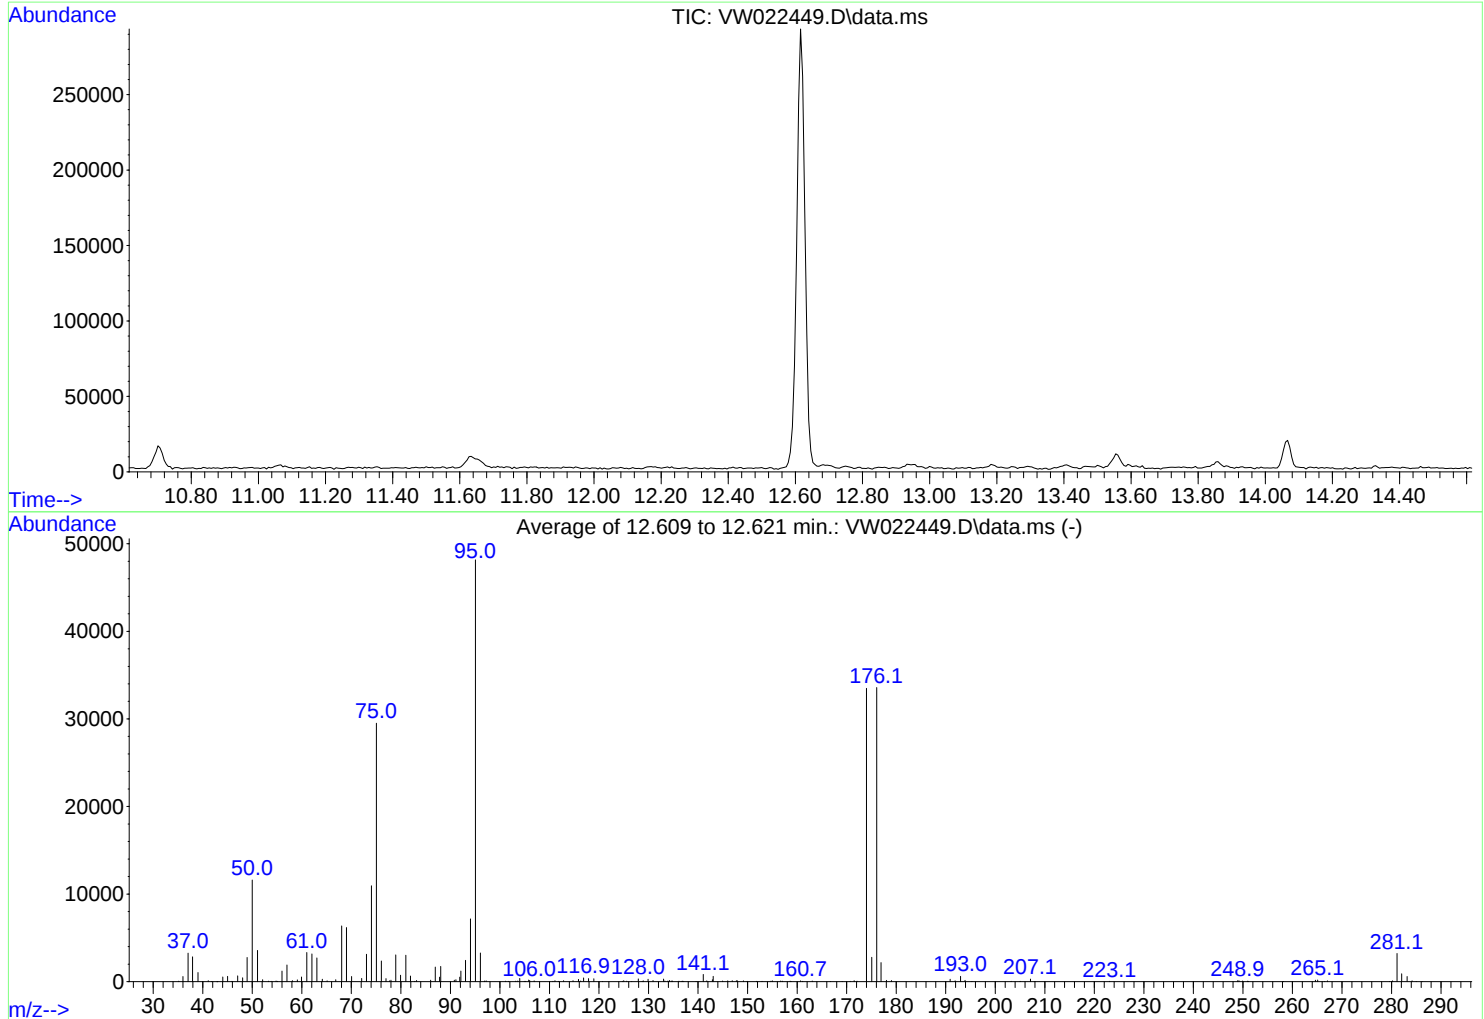

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	24.1	11602	PASS
75	95	30	80	61.3	29507	PASS
95	95	100	100	100.0	48163	PASS
96	95	5	9	6.8	3274	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	69.5	33480	PASS
175	174	5	9	8.3	2781	PASS
176	174	95	105	100.3	33584	PASS
177	176	5	10	6.5	2168	PASS

m/z	Abundance
35.70	56.0
36.40	107.0
37.10	66.0
37.90	127.0
38.60	140.0
39.10	114.0
39.90	294.0
40.80	157.0
41.40	75.0
41.90	63.0
42.80	144.0
44.10	311.0
45.80	65.0
46.40	77.0
48.90	63.0
49.70	59.0
55.10	127.0
55.70	55.0
56.90	238.0
62.30	67.0
62.70	76.0
66.10	57.0
71.10	135.0
73.10	56.0
83.40	53.0
100.90	84.0
136.90	53.0
281.20	63.0

Instrument :
MSVOA_W
ClientSampleId :
BFB530

m/z	Abundance
35.20	109.0
36.10	527.0
37.00	2763.0
38.00	2925.0
39.10	1270.0
40.00	272.0
41.10	130.0
41.90	55.0
43.00	221.0
44.10	782.0
45.00	567.0
46.00	184.0
47.20	565.0
48.10	546.0
49.00	2774.0
50.00	11097.0
51.10	3394.0
52.00	117.0
53.30	90.0
53.80	90.0
54.80	225.0
56.00	1218.0
57.00	2028.0
58.10	65.0
59.10	245.0
60.10	541.0
61.00	2800.0
62.00	2883.0
63.00	2398.0
64.20	309.0
66.90	160.0
68.00	5664.0
69.00	6327.0
70.10	537.0
71.10	75.0
72.10	366.0
73.00	3324.0
74.00	9985.0
75.10	27072.0
76.10	2519.0
77.00	385.0
77.70	284.0
79.00	3009.0
80.00	755.0
81.00	2792.0
81.90	661.0
82.80	102.0
83.10	81.0
86.00	194.0
87.00	1557.0
88.10	2019.0
90.80	235.0
91.90	1522.0
93.00	1939.0
94.00	6330.0
95.10	44224.0
96.10	3125.0
97.20	196.0
101.70	53.0
103.20	194.0
103.60	203.0
104.10	218.0
105.80	283.0
106.90	86.0
111.10	175.0
112.80	171.0
114.80	110.0
115.80	362.0
116.90	336.0
117.80	336.0
119.00	337.0
125.00	167.0
125.60	78.0
127.90	348.0
128.70	124.0
129.90	227.0
131.00	68.0
133.10	535.0
133.90	211.0
134.20	211.0
134.60	223.0
136.80	184.0
141.10	662.0
141.90	94.0
142.90	678.0
144.90	149.0
146.00	97.0
147.00	110.0
147.80	155.0
148.00	153.0
149.20	81.0
149.90	137.0

Instrument :
MSVOA_W
ClientSampleId :
BFB530

151.80	86.0
152.90	120.0
154.70	59.0
156.70	56.0
158.60	151.0
160.60	74.0
161.10	108.0
163.00	94.0
166.70	73.0
170.70	93.0
171.50	90.0
172.10	193.0
174.00	26000.0
175.00	2046.0
176.00	28296.0
176.90	2022.0
178.00	180.0
179.00	176.0
190.90	343.0
191.90	90.0
193.00	885.0
193.90	253.0
195.30	63.0
205.00	121.0
207.20	308.0
208.00	81.0
223.10	89.0
249.00	226.0
250.00	138.0
250.90	148.0
258.20	55.0
264.60	205.0
265.10	350.0
267.10	160.0
279.60	60.0
281.10	4719.0
282.00	1316.0
283.10	940.0
284.10	141.0
285.00	64.0

Instrument :
MSVOA_W
ClientSampleId :
BFB530

m/z	Abundance
35.90	655.0
37.10	3697.0
38.00	3393.0
39.00	1197.0
39.80	217.0
41.10	60.0
41.70	76.0
42.90	112.0
44.00	932.0
45.00	787.0
46.00	124.0
47.00	648.0
48.00	375.0
49.00	3519.0
50.00	12567.0
51.00	4038.0
52.10	301.0
53.30	91.0
55.10	235.0
56.10	1205.0
57.00	2550.0
58.20	105.0
59.10	207.0
59.90	609.0
61.00	4031.0
62.00	3426.0
63.00	2980.0
64.00	234.0
65.10	154.0
66.80	264.0
68.00	6844.0
69.00	6951.0
70.10	679.0
71.20	61.0
72.10	445.0
73.10	3221.0
74.10	11970.0
75.00	33096.0
76.10	2547.0
77.00	391.0
78.00	285.0
79.00	3204.0
79.90	640.0
81.00	3300.0
82.00	759.0
83.20	146.0
86.00	142.0
87.00	2096.0
87.80	1548.0
88.10	1368.0
90.80	264.0
91.20	294.0
92.10	1856.0
93.00	2431.0
94.10	8518.0
95.00	53656.0
96.00	3691.0
96.90	106.0
97.20	105.0
101.10	71.0
101.70	66.0
104.10	417.0
106.00	383.0
107.00	71.0
111.10	136.0
112.90	96.0
114.70	87.0
115.90	394.0
117.00	588.0
117.90	407.0
119.00	393.0
120.70	52.0
124.70	110.0
125.60	109.0
126.60	72.0
128.00	357.0
129.00	136.0
129.90	402.0
130.80	139.0
132.90	182.0
133.30	238.0
134.30	110.0
134.80	166.0
136.20	86.0
136.90	139.0
141.00	1155.0
141.70	80.0
143.10	921.0
145.00	83.0
146.10	79.0
146.90	172.0
147.70	166.0

Instrument :
MSVOA_W
ClientSampleId :
BFB530

149.10	116.0
154.70	130.0
156.70	144.0
160.70	73.0
163.10	80.0
171.50	146.0
174.00	37248.0
175.10	3336.0
176.10	34648.0
177.00	2180.0
178.10	98.0
179.10	199.0
190.90	348.0
191.90	175.0
193.00	534.0
193.90	160.0
203.20	83.0
207.00	196.0
249.20	245.0
249.90	59.0
251.20	67.0
264.70	264.0
267.00	128.0
280.20	188.0
281.10	3554.0
282.10	984.0
283.20	445.0
284.20	122.0
286.20	63.0

Instrument :
MSVOA_W
ClientSampleId :
BFB530

m/z	Abundance
35.10	87.0
36.00	573.0
37.10	3475.0
38.00	2550.0
39.00	1003.0
40.00	208.0
41.10	131.0
41.70	88.0
42.90	119.0
44.00	812.0
45.10	433.0
47.00	742.0
48.10	402.0
49.00	2171.0
50.00	11143.0
51.10	3251.0
52.20	253.0
55.00	240.0
55.90	1213.0
57.10	1821.0
58.10	180.0
59.00	140.0
59.90	458.0
61.00	3124.0
62.10	3184.0
63.10	2709.0
64.20	270.0
65.10	118.0
66.90	232.0
68.10	6568.0
69.00	5231.0
70.00	553.0
72.10	306.0
73.00	2984.0
74.00	10890.0
75.00	28352.0
76.00	2036.0
77.00	293.0
78.00	231.0
78.90	2935.0
79.90	814.0
81.00	2944.0
82.00	493.0
83.20	177.0
86.00	142.0
86.90	1366.0
88.00	1847.0
91.00	365.0
92.10	1765.0
93.10	2912.0
94.00	6615.0
95.00	46608.0
96.10	3005.0
96.90	117.0
101.20	84.0
103.90	444.0
104.90	113.0
105.20	116.0
105.80	277.0
106.80	108.0
110.70	111.0
111.80	89.0
112.90	81.0
114.70	129.0
116.30	218.0
116.80	354.0
118.00	316.0
118.80	267.0
125.00	185.0
127.90	219.0
128.90	164.0
129.90	213.0
131.00	170.0
133.00	167.0
134.20	57.0
134.80	72.0
136.10	59.0
136.60	137.0
137.10	126.0
139.60	51.0
141.00	646.0
141.70	81.0
143.00	876.0
145.90	108.0
146.80	72.0
147.90	108.0
149.20	100.0
155.00	260.0
157.00	189.0
158.80	81.0
160.80	125.0
163.10	73.0

Instrument :
MSVOA_W
ClientSampleId :
BFB530

169.10	51.0
171.50	120.0
174.00	37192.0
175.00	2962.0
176.00	37808.0
177.00	2302.0
178.00	187.0
191.00	125.0
193.10	399.0
206.90	196.0
207.20	209.0
248.80	104.0
249.20	77.0
251.10	55.0
265.10	189.0
266.50	55.0
280.20	113.0
281.20	1547.0
282.10	364.0
283.00	182.0
283.30	179.0

Instrument :
MSVOA_W
ClientSampleId :
BFB530