

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040924\
 Data File : VW028363.D
 Acq On : 09 Apr 2024 15:04
 Operator : SY/MD
 Sample : P2007-09
 Misc : 4.51g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BH2M1

Quant Time: Apr 10 01:18:01 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 10 01:16:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	460501	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	416394	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	196069	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	184732	25.023	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	100.080%
7) Chloroethane-d5	2.905	69	141923	25.364	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	101.440%
11) 1,1-Dichloroethene-d2	4.021	65	77358	24.744	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	98.960%
21) 2-Butanone-d5	7.075	46	60328	43.669	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.340%
24) Chloroform-d	7.654	84	290480	24.174	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.680%
26) 1,2-Dichloroethane-d4	8.307	65	158433	25.371	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	101.480%
32) Benzene-d6	8.276	84	593336	26.084	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	104.320%
36) 1,2-Dichloropropane-d6	9.270	67	172359	25.491	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.960%
41) Toluene-d8	10.319	98	543530	26.277	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	105.120%
43) trans-1,3-Dichloroprop...	10.575	79	66655	24.792	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	99.160%
47) 2-Hexanone-d5	10.922	63	41970	44.811	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.620%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	112455	23.573	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.280%
66) 1,2-Dichlorobenzene-d4	13.848	152	165847	26.746	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	107.000%
Target Compounds						
16) Methylene chloride	4.929	84	16026	2.300	ug/L	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040924\
Data File : VW028363.D
Acq On : 09 Apr 2024 15:04
Operator : SY/MD
Sample : P2007-09
Misc : 4.51g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BH2M1

Quant Time: Apr 10 01:18:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 10 01:16:29 2024
Response via : Initial Calibration

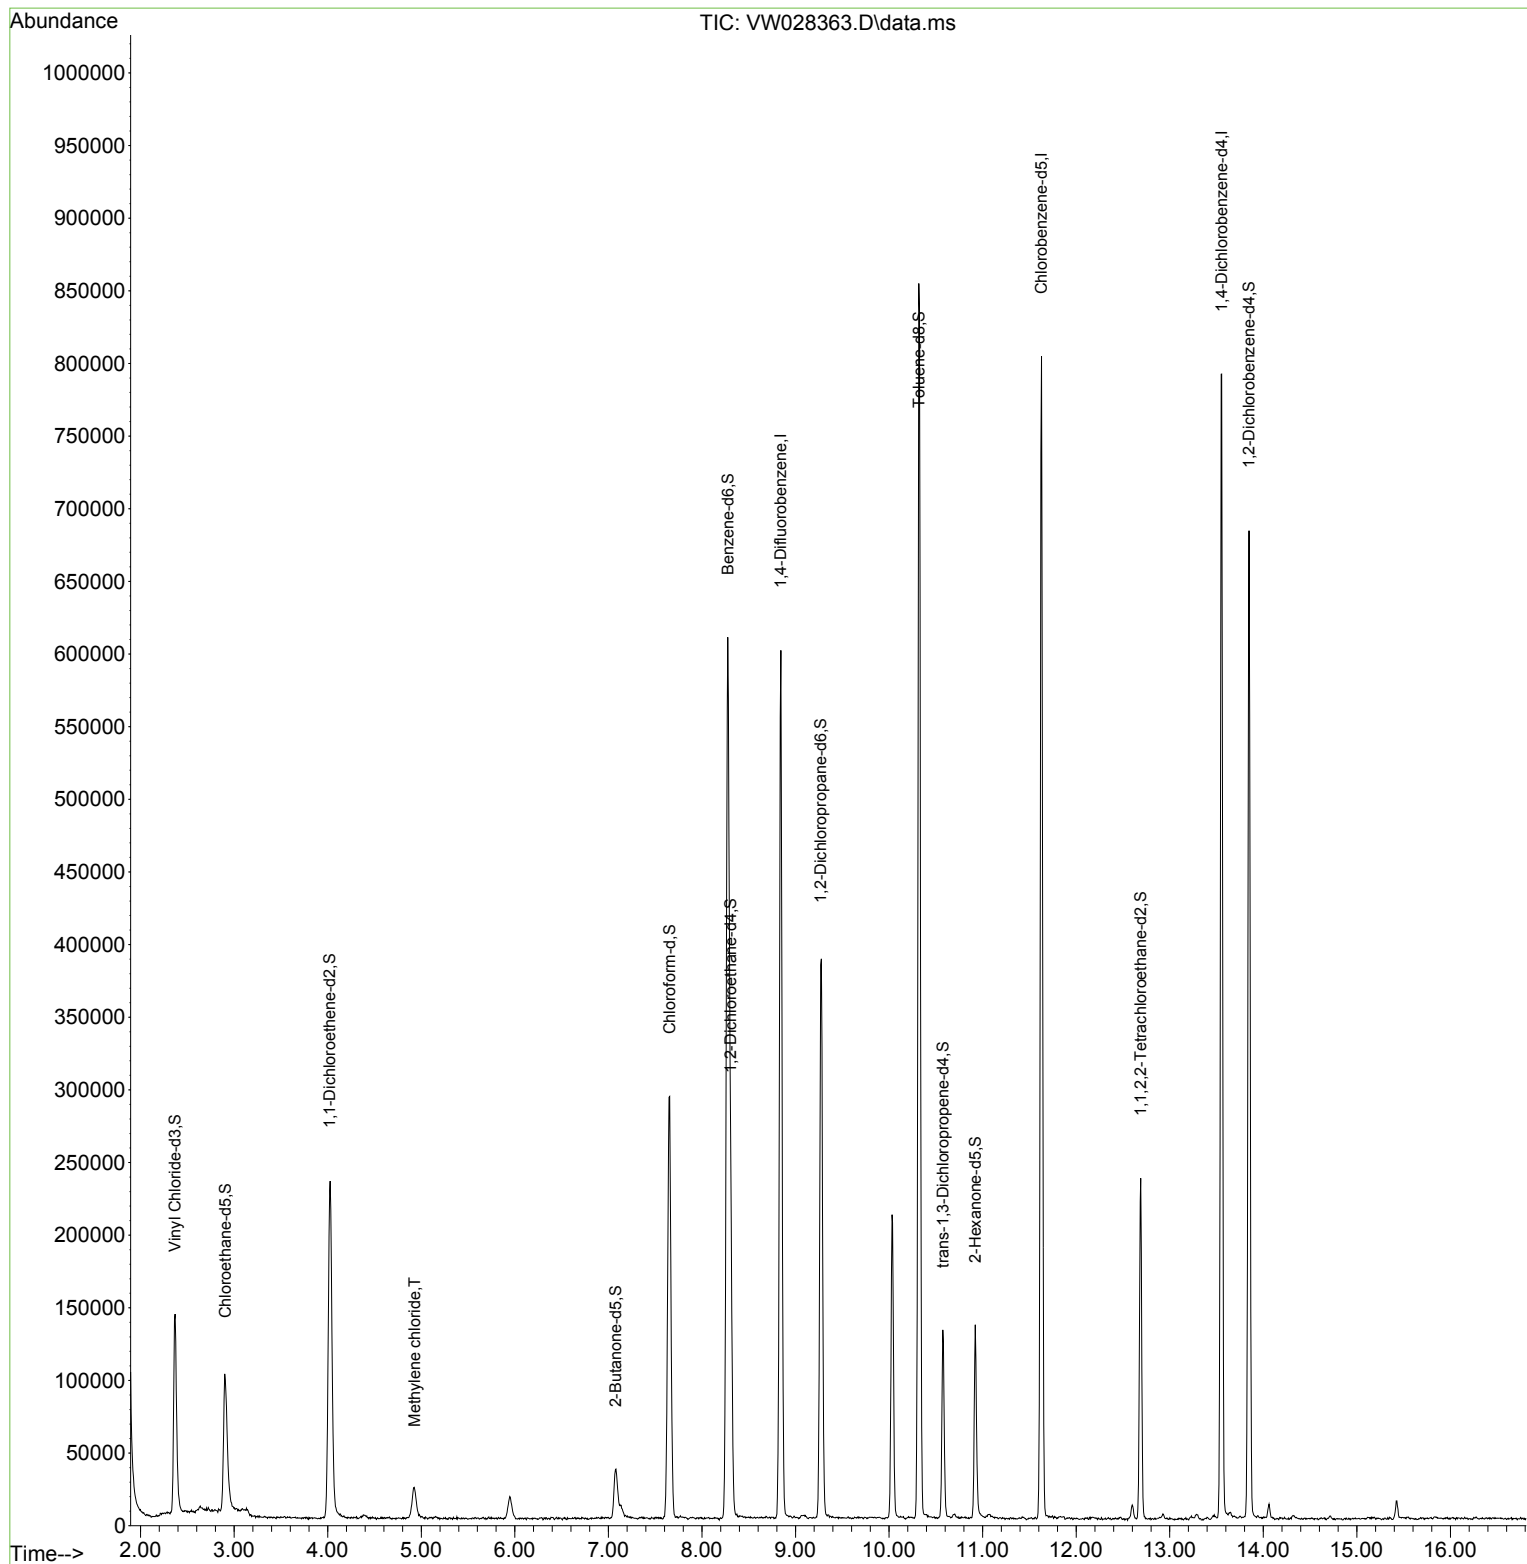

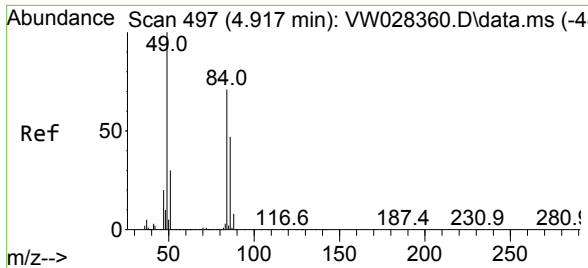

#16
Methylene chloride
Concen: 2.300 ug/L
RT: 4.929 min Scan# 499
Delta R.T. 0.012 min
Lab File: VW028363.D
Acq: 09 Apr 2024 15:04

Instrument :
MSVOA_W
ClientSampleId :
BH2M1

Tgt Ion:	84	Resp:	16026
Ion	Ratio	Lower	Upper
84	100		
86	61.0	44.2	82.0
49	137.3	95.0	176.4

