

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040924\
 Data File : VW028370.D
 Acq On : 09 Apr 2024 17:51
 Operator : SY/MD
 Sample : P2037-02
 Misc : 4.68g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E1CY1

Quant Time: Apr 10 01:19:48 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 10 01:16:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	421468	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	369516	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	151185	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	146243	21.644	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.560%
7) Chloroethane-d5	2.899	69	114492	22.357	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.440%
11) 1,1-Dichloroethene-d2	4.015	65	60206	21.041	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	84.160%
21) 2-Butanone-d5	7.075	46	56812	44.933	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.860%
24) Chloroform-d	7.648	84	250497	22.777	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.120%
26) 1,2-Dichloroethane-d4	8.307	65	137379	24.037	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.160%
32) Benzene-d6	8.276	84	506511	25.092	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	100.360%
36) 1,2-Dichloropropane-d6	9.270	67	149876	24.978	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.920%
41) Toluene-d8	10.319	98	443277	24.149	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	96.600%
43) trans-1,3-Dichloroprop...	10.575	79	55023	23.062	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	92.240%
47) 2-Hexanone-d5	10.922	63	36163	43.509	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.020%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	100364	23.707	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.840%
66) 1,2-Dichlorobenzene-d4	13.848	152	125175	26.180	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	104.720%
Target Compounds						
16) Methylene chloride	4.917	84	13909	2.181	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040924\
Data File : VW028370.D
Acq On : 09 Apr 2024 17:51
Operator : SY/MD
Sample : P2037-02
Misc : 4.68g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E1CY1

Quant Time: Apr 10 01:19:48 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 10 01:16:29 2024
Response via : Initial Calibration

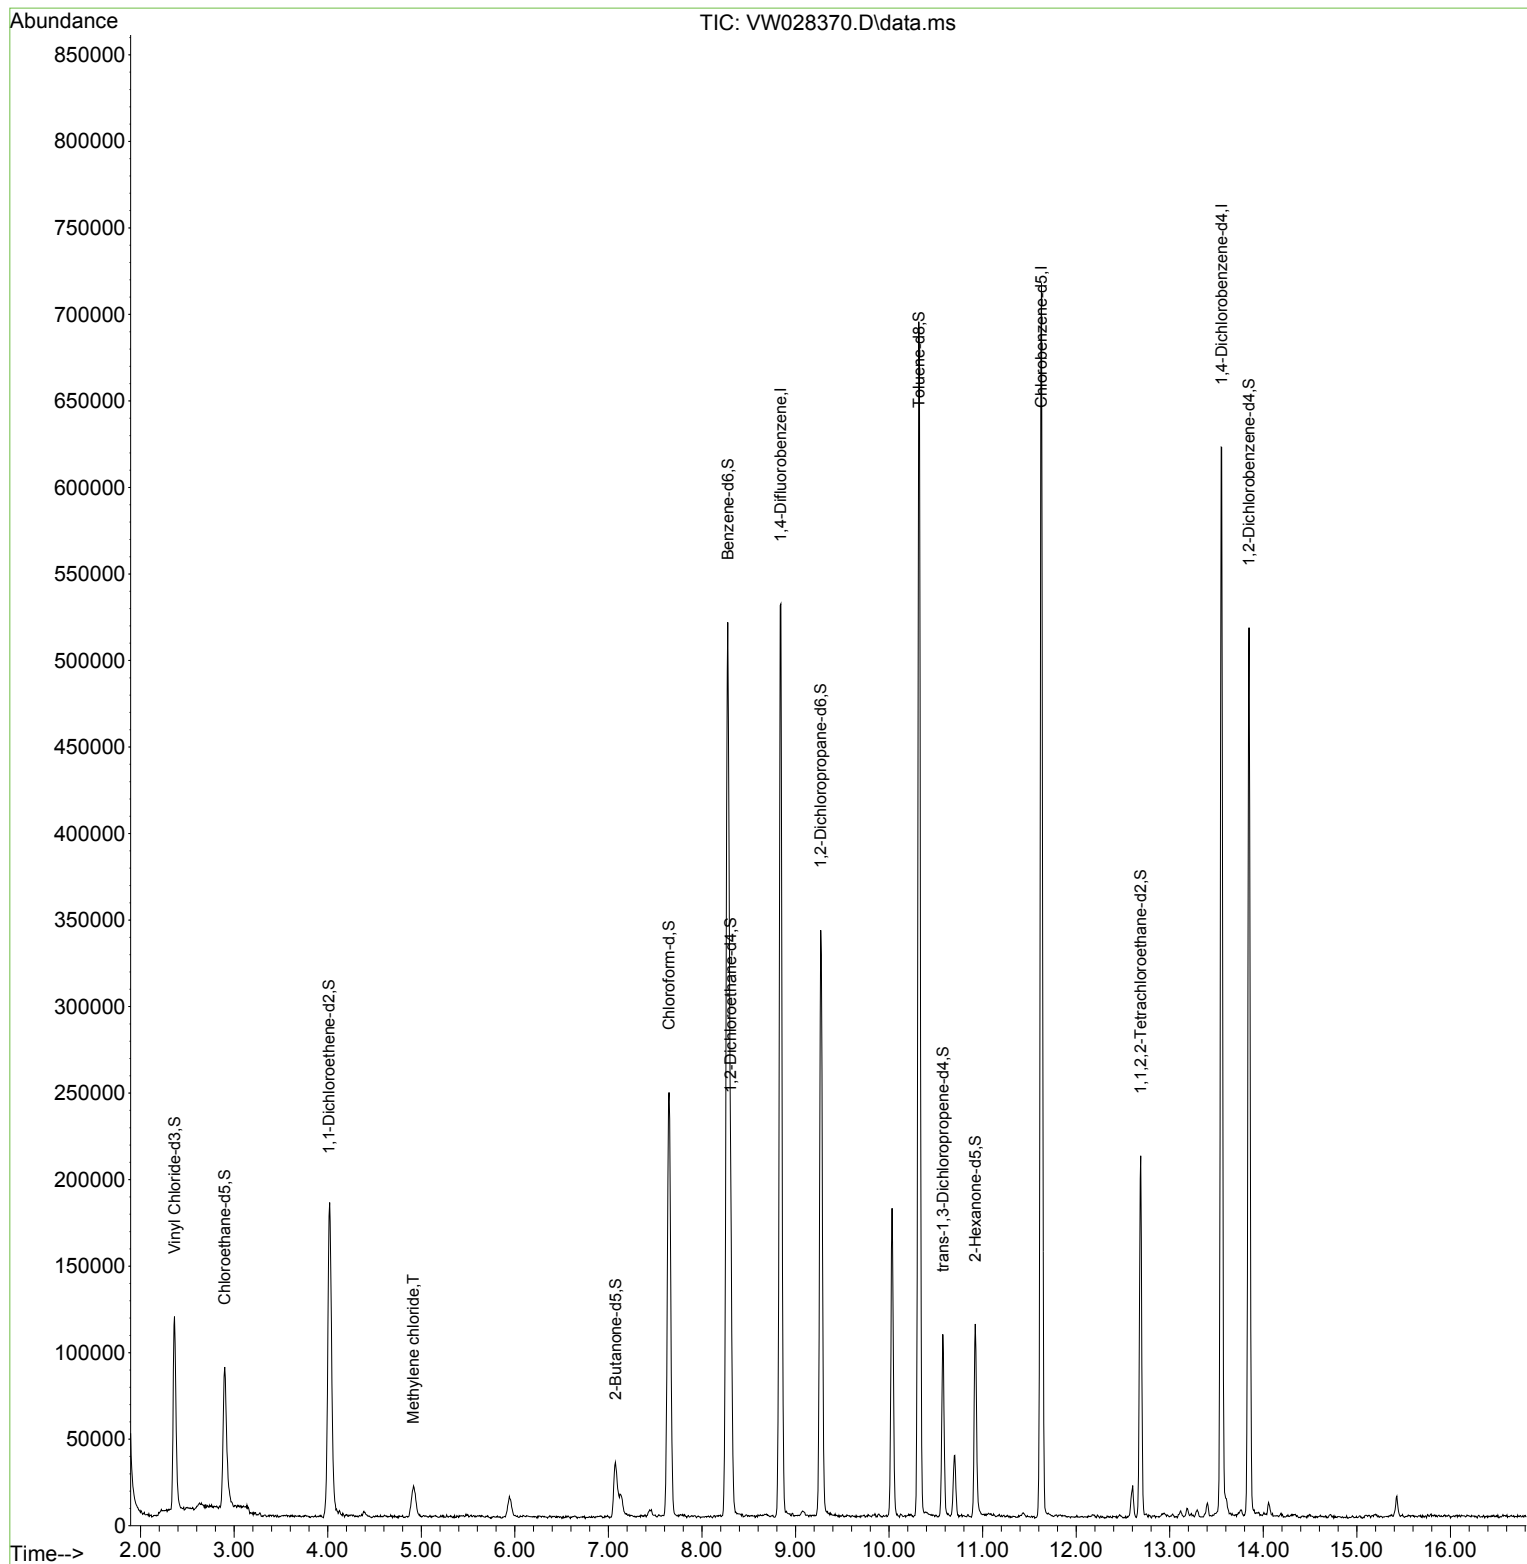

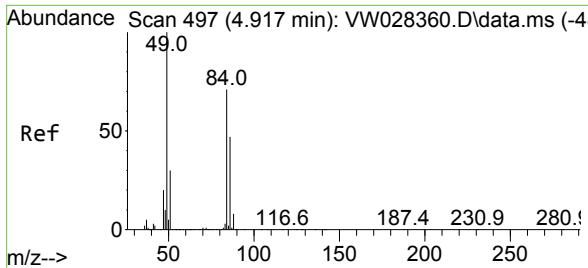

#16
Methylene chloride
Concen: 2.181 ug/L
RT: 4.917 min Scan# 49
Delta R.T. -0.000 min
Lab File: VW028370.D
Acq: 09 Apr 2024 17:51

Instrument :
MSVOA_W
ClientSampleId :
E1CY1

Tgt Ion:	84	Resp:	13909
Ion	Ratio	Lower	Upper
84	100		
86	66.1	44.2	82.0
49	135.4	95.0	176.4

