




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040924\
Data File : VW028366.D
Acq On : 09 Apr 2024 16:16
Operator : SY/MD
Sample : P2037-08
Misc : 3.04g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E1CY6

Manual IntegrationsAPPROVED

Quant Time: Apr 10 01:18:44 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 10 01:16:29 2024
Response via : Initial Calibration

Reviewed By :Semsettin
Yesilyurt

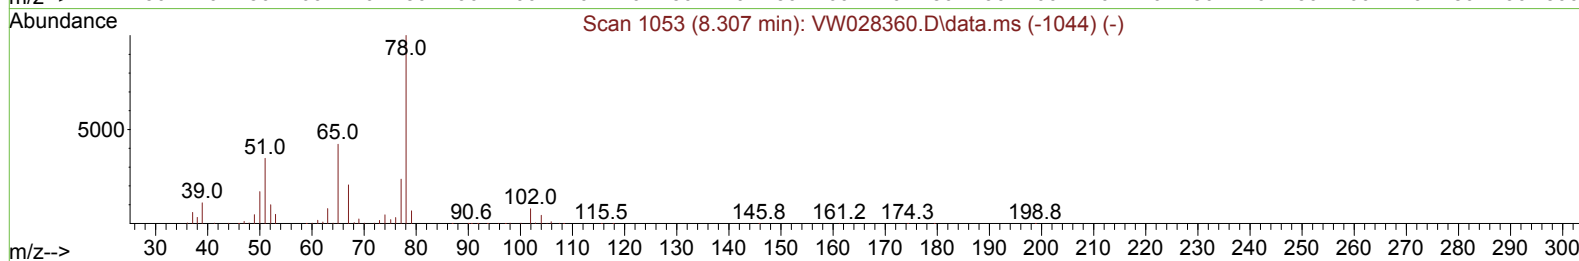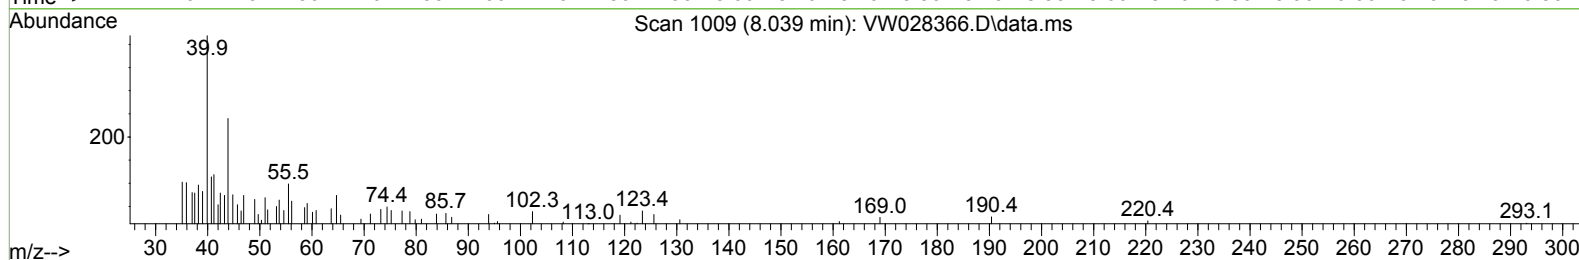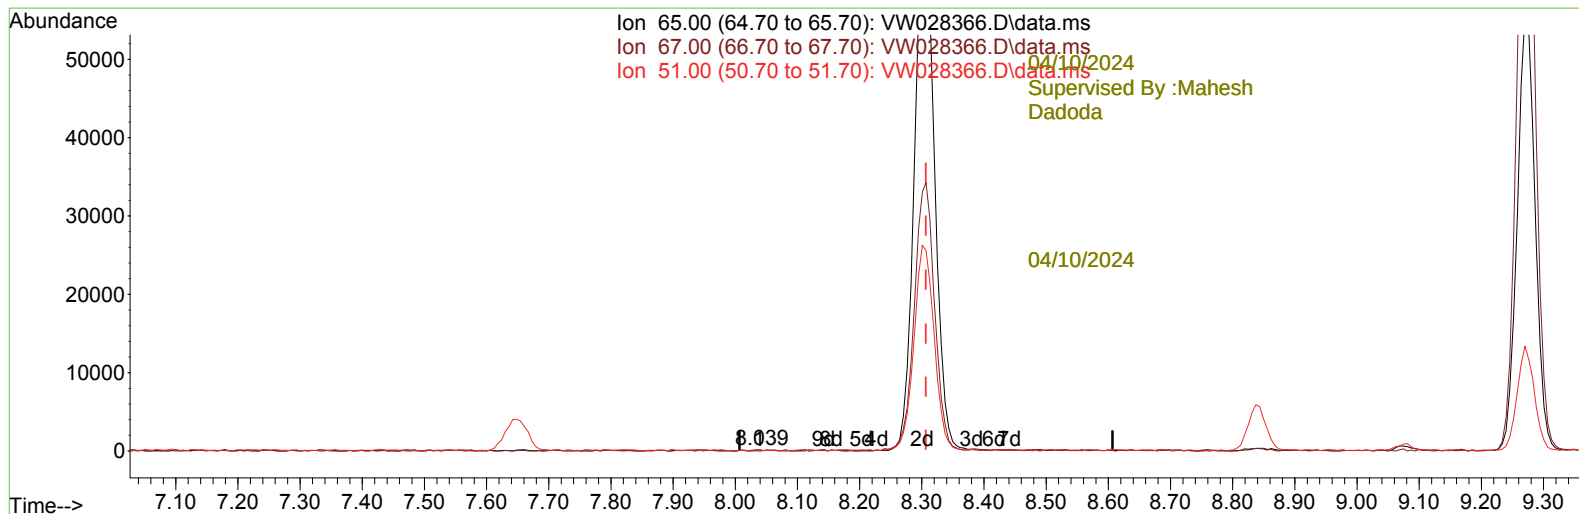

TIC: VW028366.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.039min (-0.268) 0.02 ug/L

response 109

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.10	46.79
51.00	108.40	93.58
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040924\
Data File : VW028366.D
Acq On : 09 Apr 2024 16:16
Operator : SY/MD
Sample : P2037-08
Misc : 3.04g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E1CY6




Manual IntegrationsAPPROVED

Quant Time: Apr 10 01:18:44 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 10 01:16:29 2024
Response via : Initial Calibration

Reviewed By :Semsettin
Yesilyurt

04/10/2024
Supervised By :Mahesh
Dadoda

04/10/2024

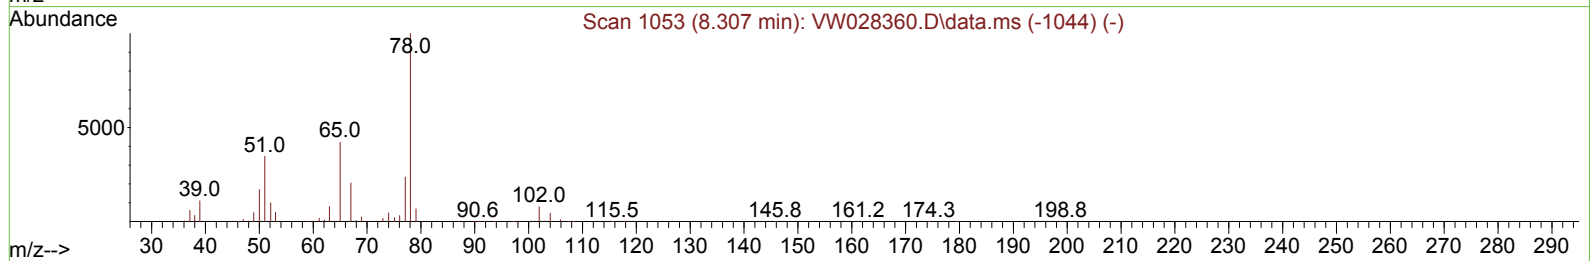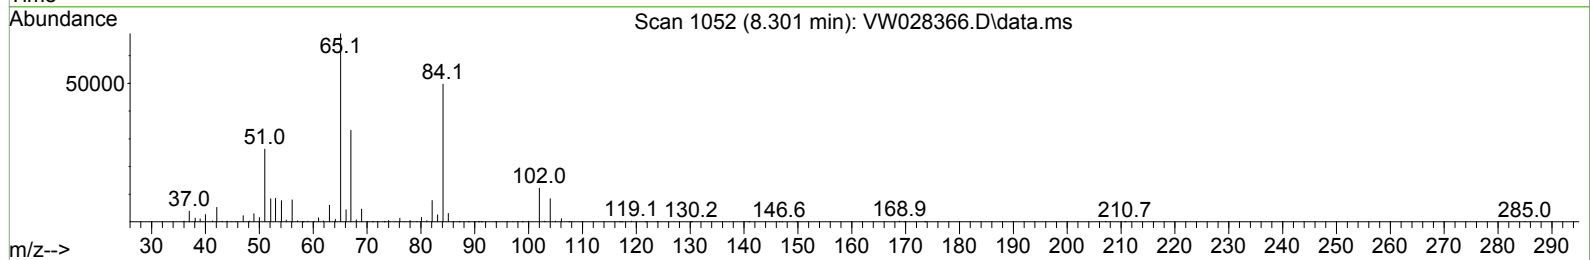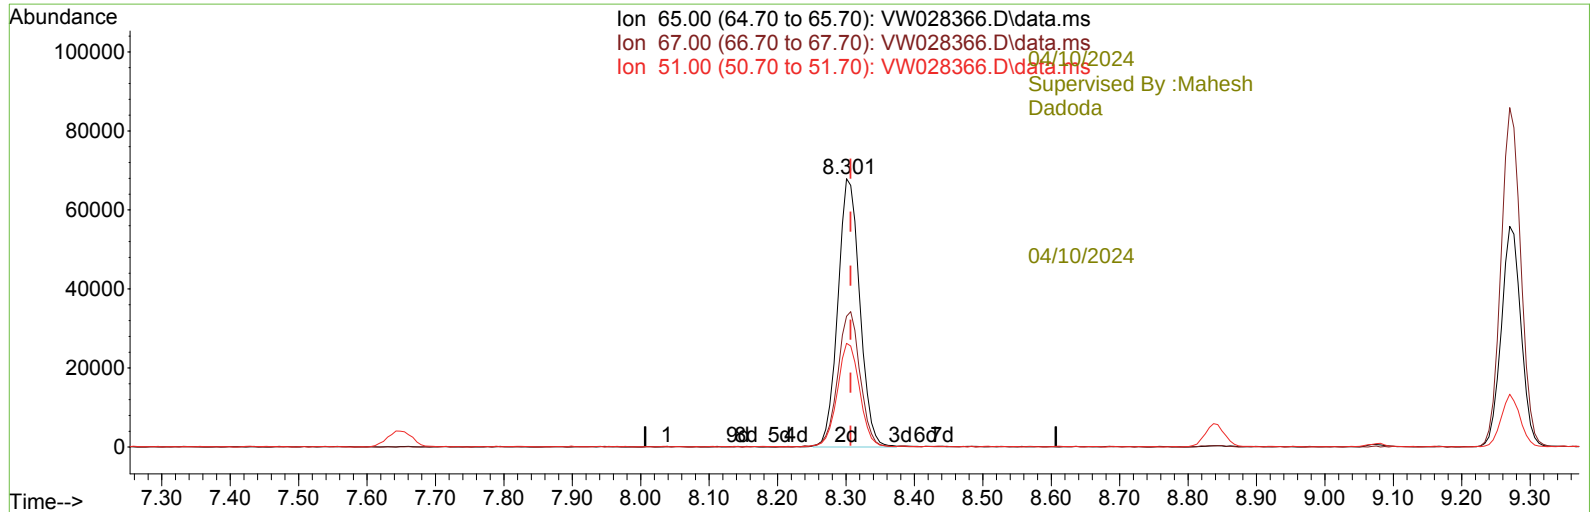

TIC: VW028366.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.301min (-0.006) 22.41 ug/L m

response 151292

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.10	0.03#
51.00	108.40	0.07#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040924\
 Data File : VW028366.D
 Acq On : 09 Apr 2024 16:16
 Operator : SY/MD
 Sample : P2037-08
 Misc : 3.04g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E1CY6

Manual IntegrationsAPPROVED

Quant Time: Apr 10 01:18:44 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 10 01:16:29 2024
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	497882	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	426843	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	172002	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	178445	22.356	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery =	89.440%		
7) Chloroethane-d5	2.899	69	138145	22.835	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery =	91.360%		
11) 1,1-Dichloroethene-d2	4.021	65	74596	22.069	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery =	88.280%		
21) 2-Butanone-d5	7.075	46	54473	36.471	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery =	72.940%		
24) Chloroform-d	7.648	84	238712	18.374	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery =	73.480%		
26) 1,2-Dichloroethane-d4	8.301	65	151292m	22.408	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery =	89.640%		
32) Benzene-d6	8.270	84	597964	25.644	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery =	102.560%		
36) 1,2-Dichloropropane-d6	9.270	67	172973	24.956	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery =	99.840%		
41) Toluene-d8	10.319	98	535249	25.243	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery =	100.960%		
43) trans-1,3-Dichloroprop...	10.575	79	61661	22.373	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery =	89.480%		
47) 2-Hexanone-d5	10.922	63	37682	39.248	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery =	78.500%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	62625	12.806	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery =	51.240%		
66) 1,2-Dichlorobenzene-d4	13.849	152	146658	26.961	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery =	107.840%		
Target Compounds						
16) Methylene chloride	4.923	84	19366	2.571	ug/L	98
25) Chloroform	7.673	83	54374	4.088	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040924\
Data File : VW028366.D
Acq On : 09 Apr 2024 16:16
Operator : SY/MD
Sample : P2037-08
Misc : 3.04g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E1CY6

Manual IntegrationsAPPROVED

Quant Time: Apr 10 01:18:44 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 10 01:16:29 2024
Response via : Initial Calibration

Reviewed By :Semsettin
Yesilyurt

