

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040924\
Data File : VW028369.D
Acq On : 09 Apr 2024 17:27
Operator : SY/MD
Sample : P2037-05
Misc : 3.18g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1




Instrument :
MSVOA_W
ClientSampleId :
E1CY3

Manual IntegrationsAPPROVED

Quant Time: Apr 10 01:19:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 10 01:16:29 2024
Response via : Initial Calibration

Reviewed By :Semsettin
Yesilyurt

04/10/2024
Supervised By :Mahesh
Dadoda

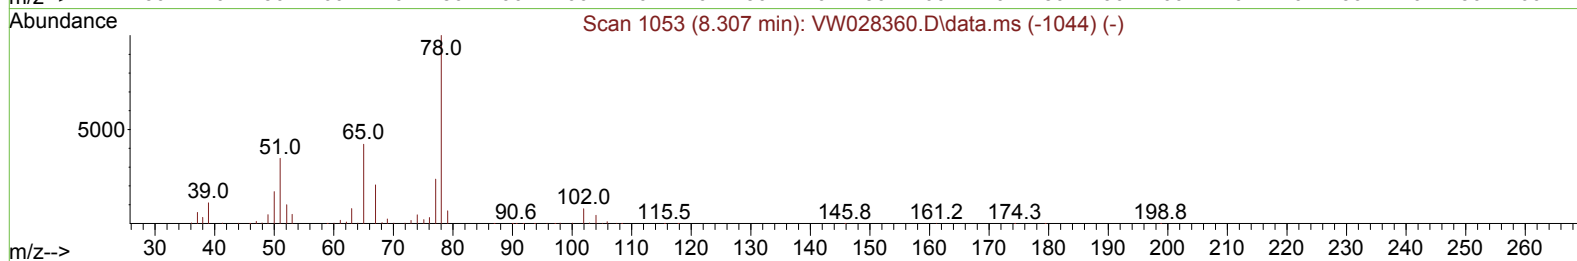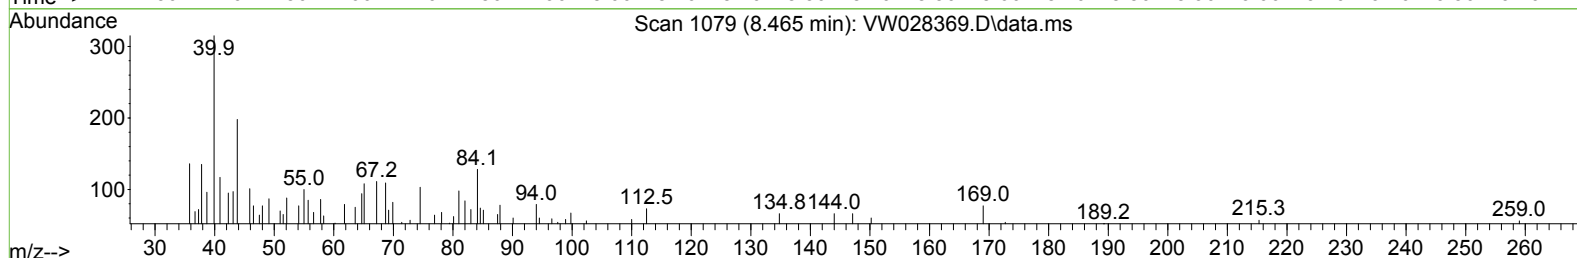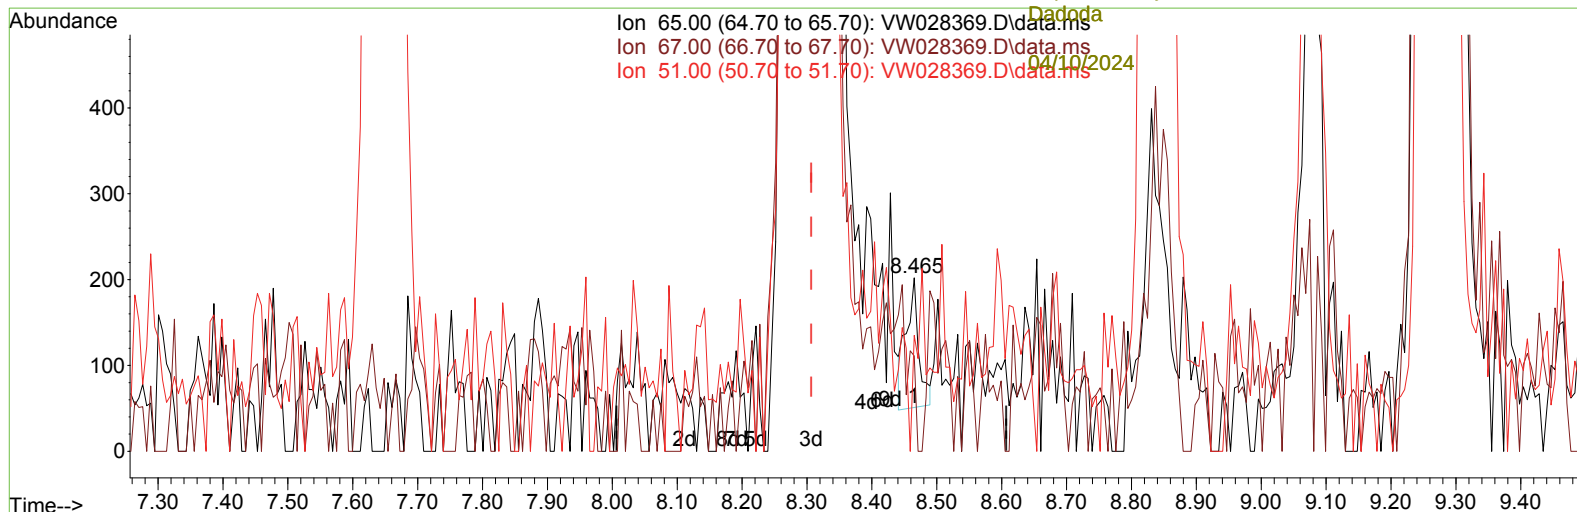

TIC: VW028369.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.465min (+ 0.158) 0.03 ug/L

response 209

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.10	39.71
51.00	108.40	95.22
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040924\
Data File : VW028369.D
Acq On : 09 Apr 2024 17:27
Operator : SY/MD
Sample : P2037-05
Misc : 3.18g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E1CY3


Manual IntegrationsAPPROVED

Quant Time: Apr 10 01:19:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 10 01:16:29 2024
Response via : Initial Calibration


Reviewed By :Semsettin
Yesilyurt

04/10/2024
Supervised By :Mahesh
Dadoda


Ion 65.00 (64.70 to 65.70): VW028369.D\data.ms
Ion 67.00 (66.70 to 67.70): VW028369.D\data.ms
Ion 51.00 (50.70 to 51.70): VW028369.D\data.ms

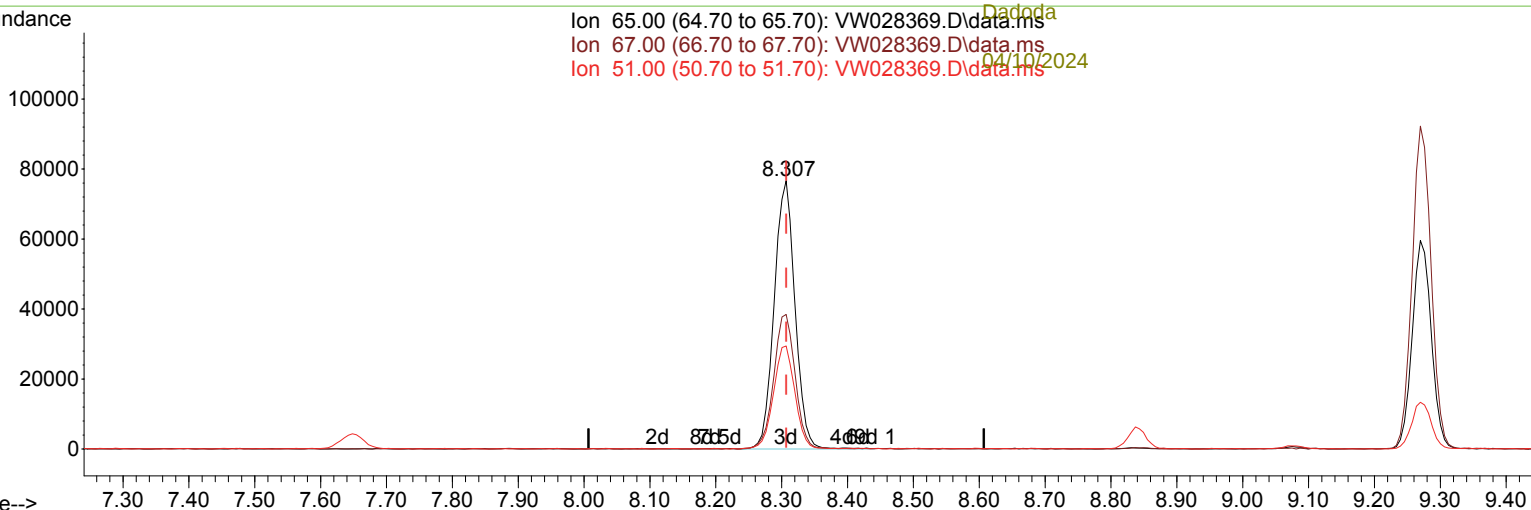

Scan 1053 (8.307 min): VW028369.D\data.ms

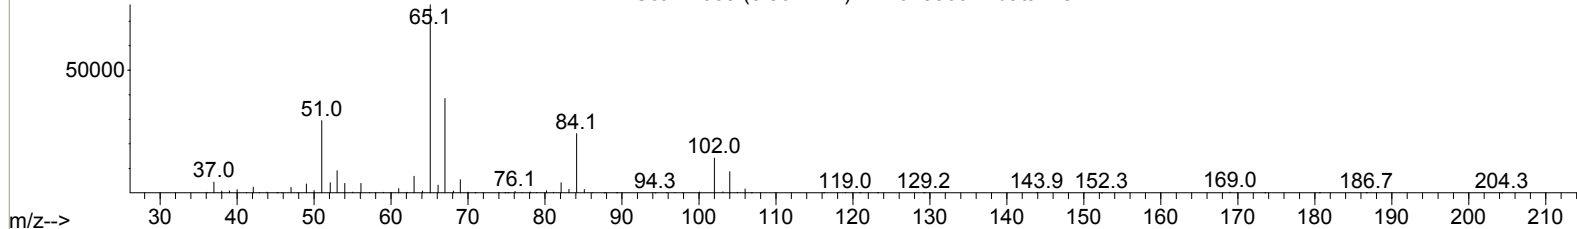

Scan 1053 (8.307 min): VW028360.D\data.ms (-1044) (-)

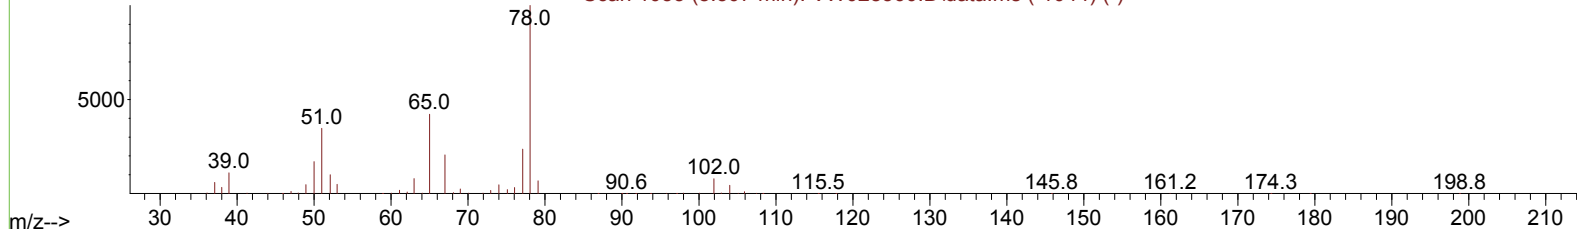

TIC: VW028369.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (-0.000) 23.78 ug/L m

response 168051

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.10	0.05#
51.00	108.40	0.12#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040924\
 Data File : VW028369.D
 Acq On : 09 Apr 2024 17:27
 Operator : SY/MD
 Sample : P2037-05
 Misc : 3.18g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E1CY3

Manual IntegrationsAPPROVED

Quant Time: Apr 10 01:19:31 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 10 01:16:29 2024
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

04/10/2024
 Supervised By :Mahesh
 Dadoda

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		521213	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		448396	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		188433	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		190708	22.823	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.280%	
7) Chloroethane-d5	2.899	69		144757	22.857	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.440%	
11) 1,1-Dichloroethene-d2	4.021	65		76128	21.514	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	86.040%	
21) 2-Butanone-d5	7.075	46		67802	43.363	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.720%	
24) Chloroform-d	7.648	84		241638	17.767	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	71.080%	
26) 1,2-Dichloroethane-d4	8.307	65		168051m	23.776	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.120%	
32) Benzene-d6	8.276	84		629305	25.691	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	102.760%	
36) 1,2-Dichloropropane-d6	9.270	67		185414	25.465	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.840%	
41) Toluene-d8	10.319	98		557726	25.039	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	100.160%	
43) trans-1,3-Dichloroprop...	10.575	79		67898	23.452	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	93.800%	
47) 2-Hexanone-d5	10.922	63		47321	46.918	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.840%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		66312	12.908	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	51.640%	
66) 1,2-Dichlorobenzene-d4	13.848	152		157929	26.502	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	106.000%	
Target Compounds							
25) Chloroform	7.679	83		68879	4.946	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040924\
Data File : VW028369.D
Acq On : 09 Apr 2024 17:27
Operator : SY/MD
Sample : P2037-05
Misc : 3.18g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E1CY3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
Yesilyurt

04/10/2024
Supervised By :Mahesh
Dadoda

04/10/2024

