

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040924\
 Data File : VW028364.D
 Acq On : 09 Apr 2024 15:28
 Operator : SY/MD
 Sample : P2007-10
 Misc : 4.75g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BH2M2

Quant Time: Apr 10 01:18:16 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Apr 10 01:16:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	486672	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	431545	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	201063	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	191885	24.594	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	98.360%
7) Chloroethane-d5	2.905	69	146715	24.810	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	99.240%
11) 1,1-Dichloroethene-d2	4.027	65	79713	24.126	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	96.520%
21) 2-Butanone-d5	7.075	46	66673	45.667	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.340%
24) Chloroform-d	7.648	84	304944	24.013	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.040%
26) 1,2-Dichloroethane-d4	8.307	65	163869	24.830	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	99.320%
32) Benzene-d6	8.276	84	624054	26.471	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	105.880%
36) 1,2-Dichloropropane-d6	9.276	67	178953	25.537	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	102.160%
41) Toluene-d8	10.319	98	568007	26.496	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	106.000%
43) trans-1,3-Dichloroprop...	10.575	79	70186	25.189	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	100.760%
47) 2-Hexanone-d5	10.922	63	45367	46.737	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.480%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	121113	24.496	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.000%
66) 1,2-Dichlorobenzene-d4	13.848	152	172220	27.084	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	108.320%
Target Compounds						
16) Methylene chloride	4.929	84	16869	2.291	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040924\
Data File : VW028364.D
Acq On : 09 Apr 2024 15:28
Operator : SY/MD
Sample : P2007-10
Misc : 4.75g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BH2M2

Quant Time: Apr 10 01:18:16 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Apr 10 01:16:29 2024
Response via : Initial Calibration

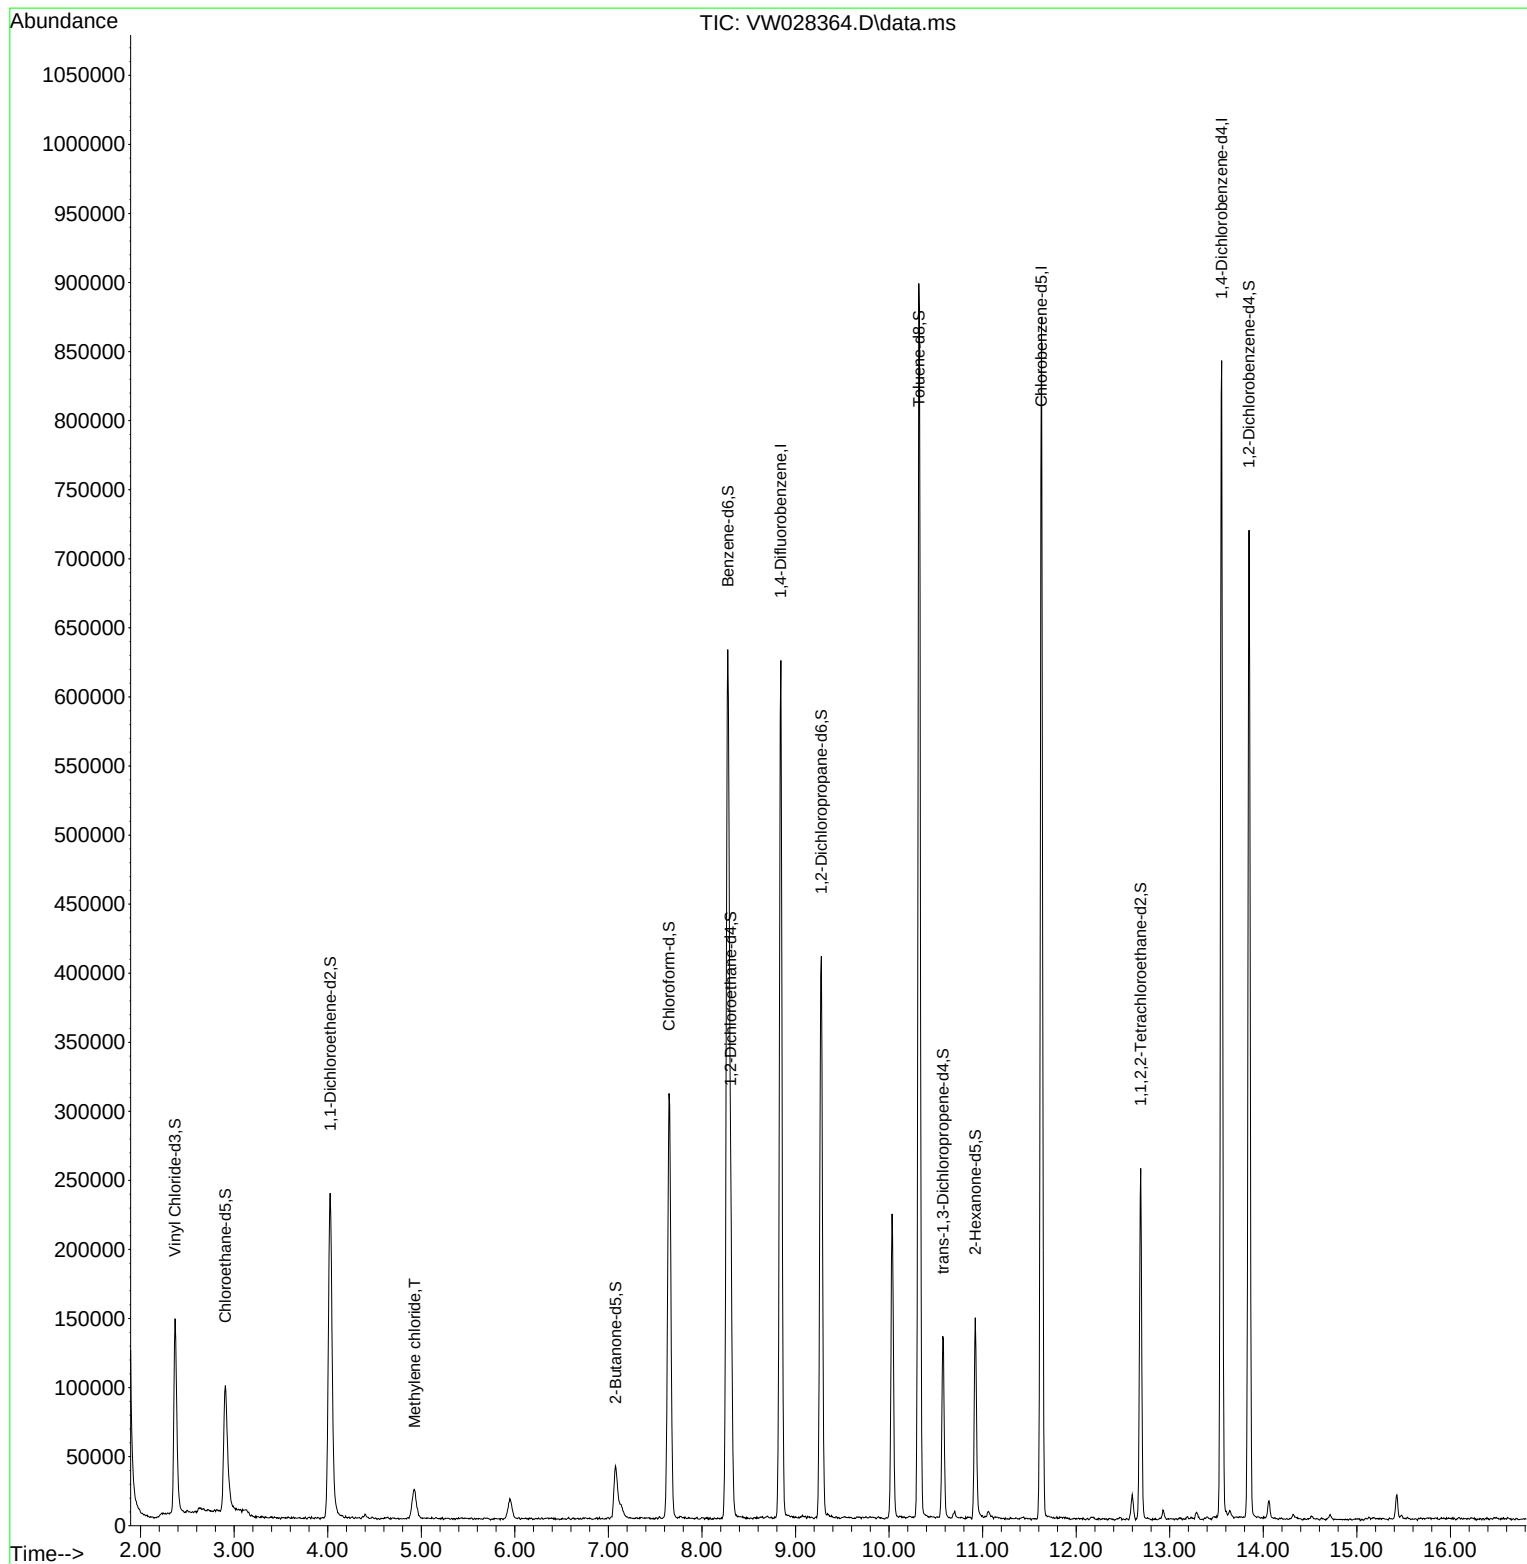

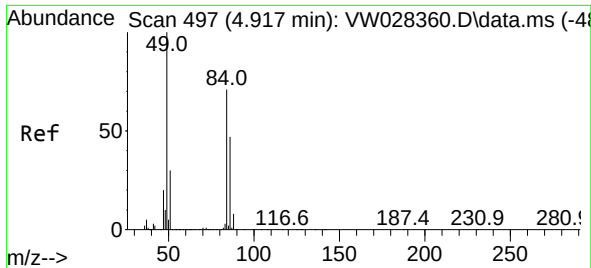

#16
Methylene chloride
Concen: 2.291 ug/L
RT: 4.929 min Scan# 499
Delta R.T. 0.012 min
Lab File: VW028364.D
Acq: 09 Apr 2024 15:28

Instrument :
MSVOA_W
ClientSampleId :
BH2M2

Tgt Ion: 84 Resp: 16869
Ion Ratio Lower Upper
84 100
86 61.2 44.2 82.0
49 135.2 95.0 176.4

