

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041124\
 Data File : VW028396.D
 Acq On : 11 Apr 2024 12:13
 Operator : SY/MD
 Sample : P2052-10
 Misc : 5.92g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AD4

Quant Time: Apr 12 00:57:01 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 12 00:55:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	530011	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	458807	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	209231	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	191894	22.584	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.320%
7) Chloroethane-d5	2.899	69	150862	23.426	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.720%
11) 1,1-Dichloroethene-d2	4.027	65	80476	22.365	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	89.480%
21) 2-Butanone-d5	7.075	46	69711	43.843	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.680%
24) Chloroform-d	7.807	84	130	0.009	ug/L	0.16
Spiked Amount	25.000	Range	40 - 150	Recovery	=	0.0400#
26) 1,2-Dichloroethane-d4	8.307	65	172615	24.017	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.080%
32) Benzene-d6	8.276	84	650914	25.970	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	103.880%
36) 1,2-Dichloropropane-d6	9.270	67	191414	25.692	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	102.760%
41) Toluene-d8	10.325	98	589534	25.866	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	103.480%
43) trans-1,3-Dichloroprop...	10.575	79	70651	23.849	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	95.400%
47) 2-Hexanone-d5	10.922	63	48645	47.137	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.280%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	126622	24.089	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	96.360%
66) 1,2-Dichlorobenzene-d4	13.848	152	168978	25.537	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.160%
Target Compounds					Qvalue	
48) 2-Hexanone	10.922	43	6606	2.224	ug/L #	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041124\
Data File : VW028396.D
Acq On : 11 Apr 2024 12:13
Operator : SY/MD
Sample : P2052-10
Misc : 5.92g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AD4


Quant Time: Apr 12 00:57:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 12 00:55:02 2024
Response via : Initial Calibration

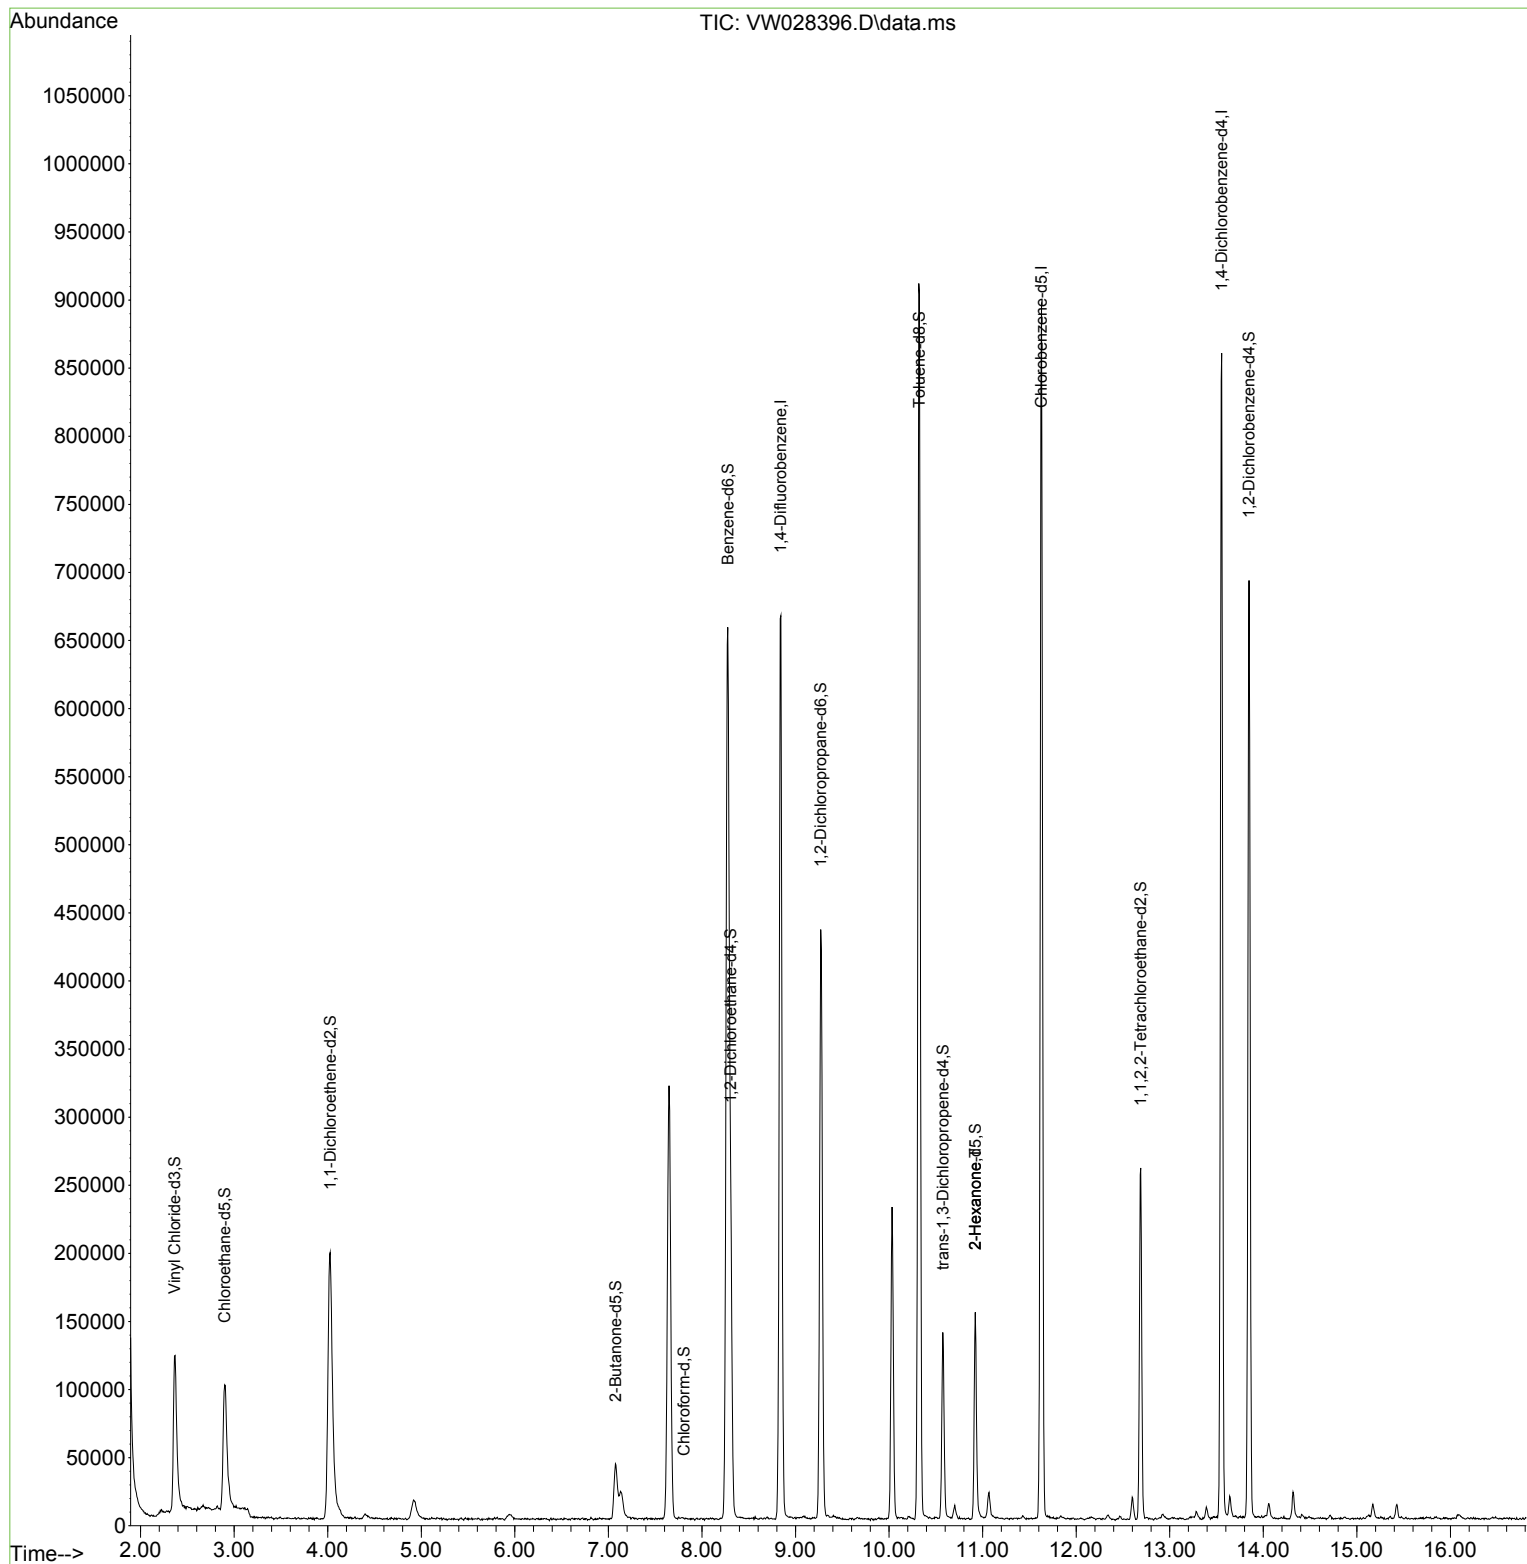

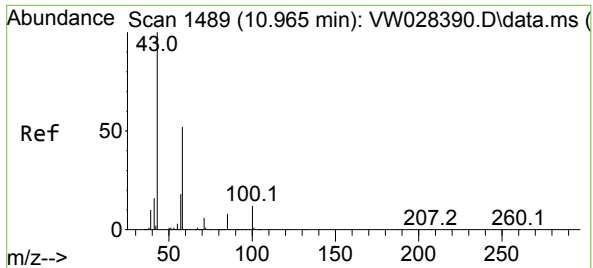

#48
2-Hexanone
Concen: 2.224 ug/L
RT: 10.922 min Scan# 14
Delta R.T. -0.043 min
Lab File: VW028396.D
Acq: 11 Apr 2024 12:13

Instrument :
MSVOA_W
ClientSampleId :
C0AD4

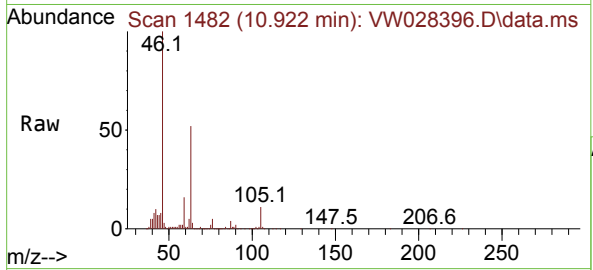

Tgt Ion:	43	Resp:	6606
Ion	Ratio	Lower	Upper
43	100		
58	20.3	38.9	58.3#
57	31.0	14.4	21.6#
100	2.2	8.7	13.1#

