

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041124\
 Data File : VW028401.D
 Acq On : 11 Apr 2024 14:13
 Operator : SY/MD
 Sample : P2052-13
 Misc : 4.23g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AF1

Quant Time: Apr 12 00:58:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 12 00:55:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	503548	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	456316	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	210526	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	186040	23.046	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.200%
7) Chloroethane-d5	2.899	69	148396	24.254	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	97.000%
11) 1,1-Dichloroethene-d2	4.021	65	78350	22.919	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	91.680%
21) 2-Butanone-d5	7.075	46	99053	65.571	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	131.140%
24) Chloroform-d	7.648	84	340164	25.888	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	103.560%
26) 1,2-Dichloroethane-d4	8.300	65	197273	28.890	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	115.560%
32) Benzene-d6	8.270	84	680124	27.283	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	109.120%
36) 1,2-Dichloropropane-d6	9.270	67	206550	27.875	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	111.520%
41) Toluene-d8	10.325	98	600774	26.504	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	106.000%
43) trans-1,3-Dichloroprop...	10.574	79	83509	28.344	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	113.360%
47) 2-Hexanone-d5	10.922	63	69843	68.047	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	136.100%#
56) 1,1,2,2-Tetrachloroeth...	12.690	84	166095	31.771	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	127.080%#
66) 1,2-Dichlorobenzene-d4	13.848	152	192096	28.852	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	115.400%
Target Compounds					Qvalue	
13) Acetone	4.130	43	8118	4.377	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041124\
Data File : VW028401.D
Acq On : 11 Apr 2024 14:13
Operator : SY/MD
Sample : P2052-13
Misc : 4.23g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AF1

Quant Time: Apr 12 00:58:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 12 00:55:02 2024
Response via : Initial Calibration

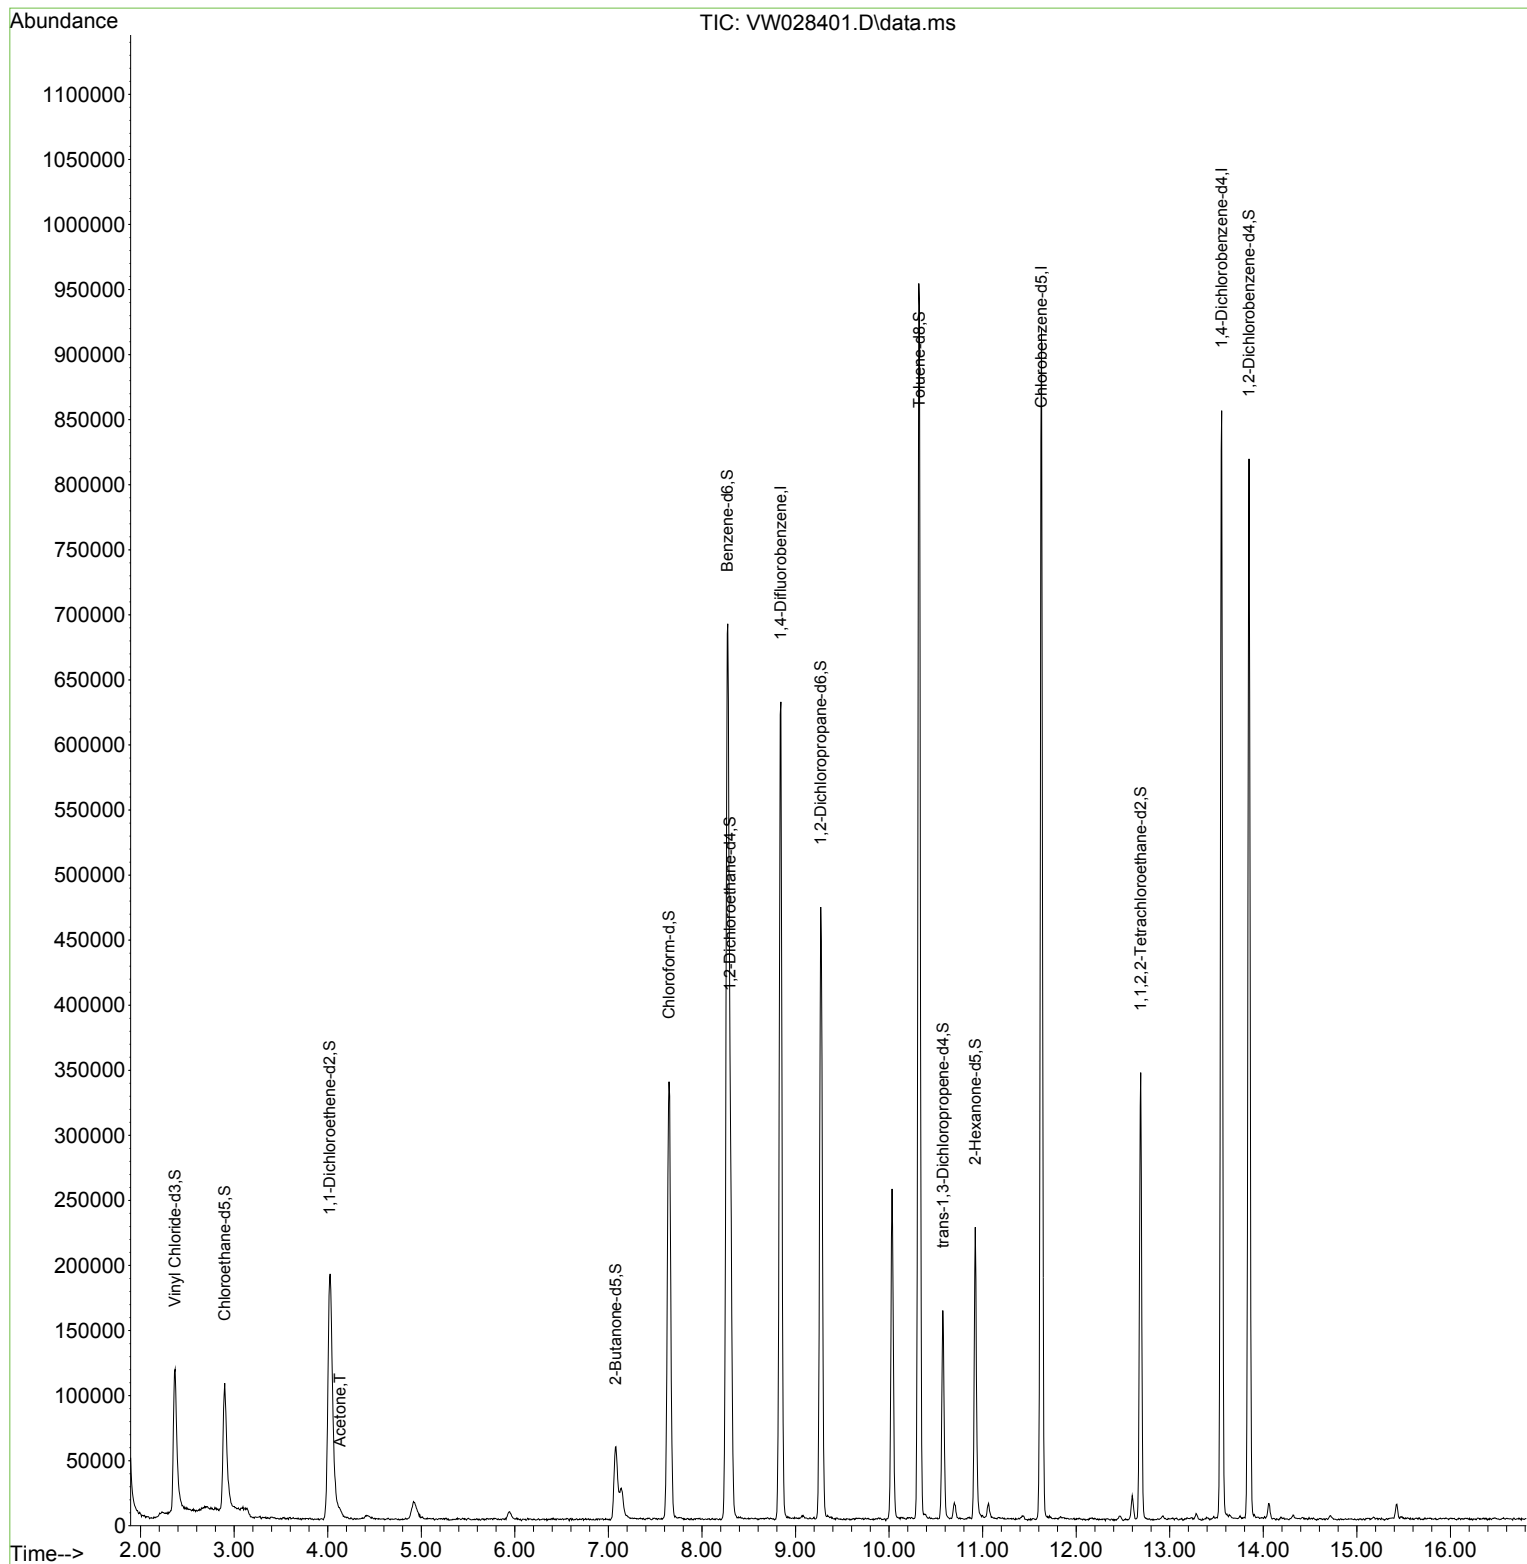

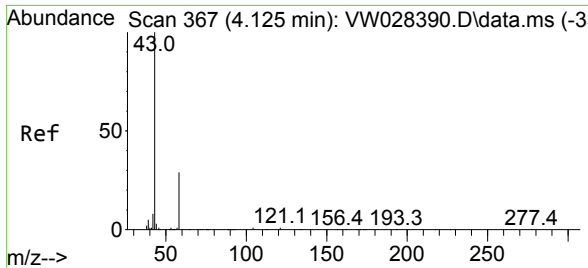

#13
 Acetone
 Concen: 4.377 ug/L
 RT: 4.130 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW028401.D
 Acq: 11 Apr 2024 14:13

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AF1

Tgt Ion:	43	Resp:	8118
Ion	Ratio	Lower	Upper
43	100		
58	29.2	0.0	53.4

