

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041124\
Data File : VW028413.D
Acq On : 11 Apr 2024 19:00
Operator : SY/MD
Sample : P2078-10
Misc : 3.76g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AC7




Manual IntegrationsAPPROVED

Quant Time: Apr 12 01:01:33 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 12 00:55:02 2024
Response via : Initial Calibration

Reviewed By :Semsettin
Yesilyurt

04/12/2024
Supervised By :Mahesh
Dadoda

04/13/2024

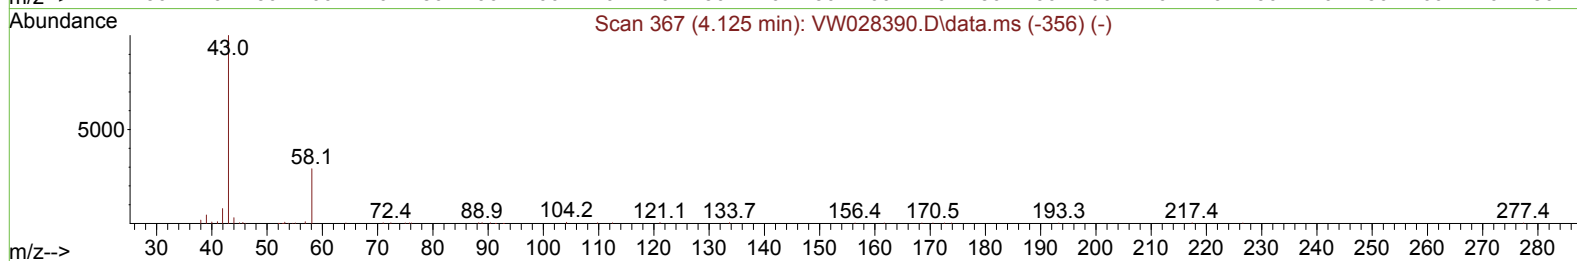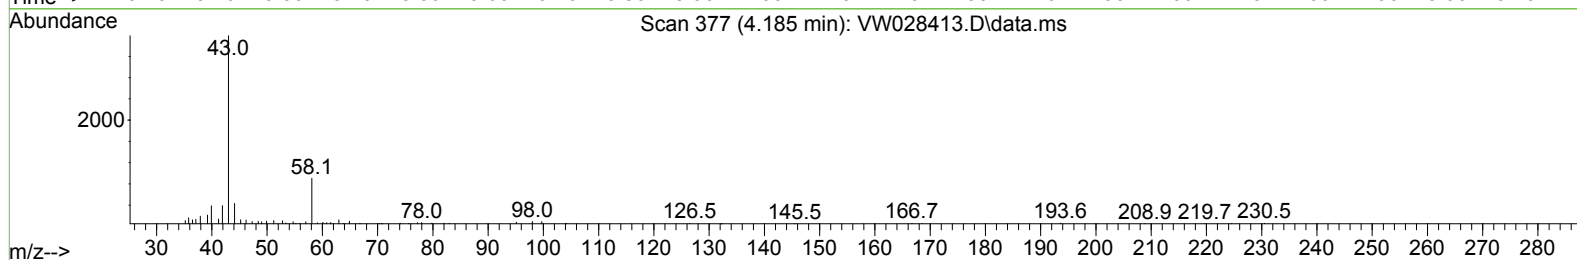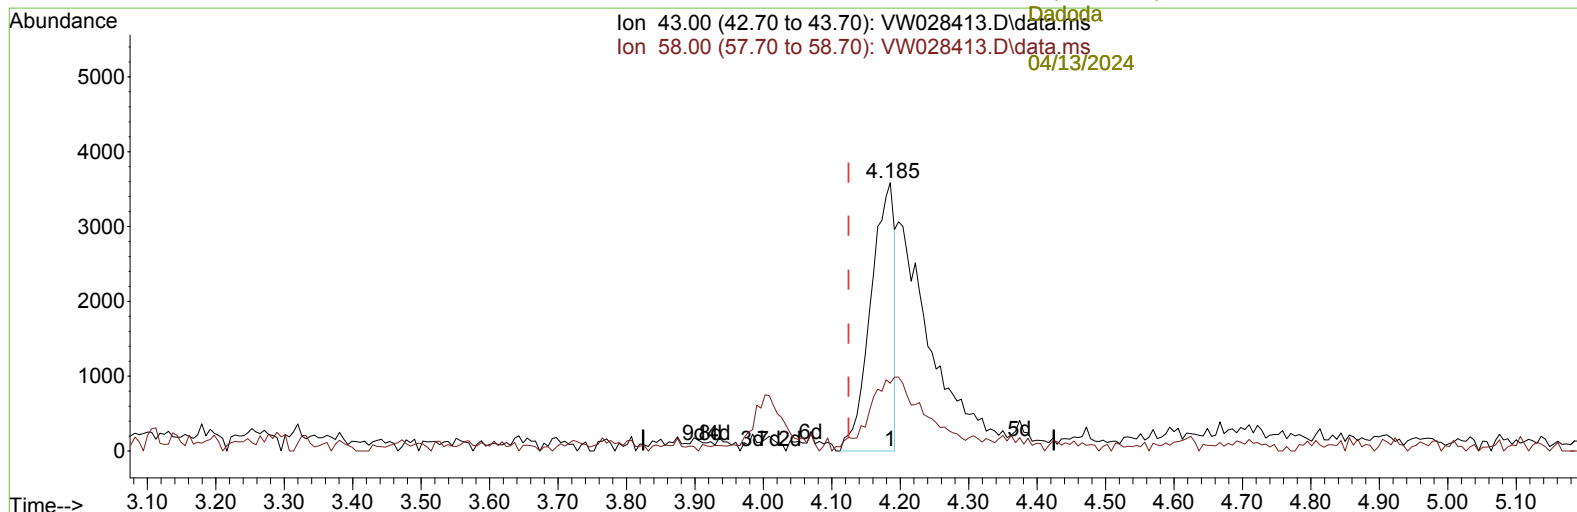

TIC: VW028413.D\data.ms

(13) Acetone (T)

4.185min (+ 0.061) 5.42 ug/L

response 8616

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.70	31.60
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041124\
Data File : VW028413.D
Acq On : 11 Apr 2024 19:00
Operator : SY/MD
Sample : P2078-10
Misc : 3.76g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AC7




Manual IntegrationsAPPROVED

Quant Time: Apr 12 01:01:33 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 12 00:55:02 2024
Response via : Initial Calibration

Reviewed By :Semsettin
Yesilyurt

04/12/2024
Supervised By :Mahesh
Dadoda

04/13/2024

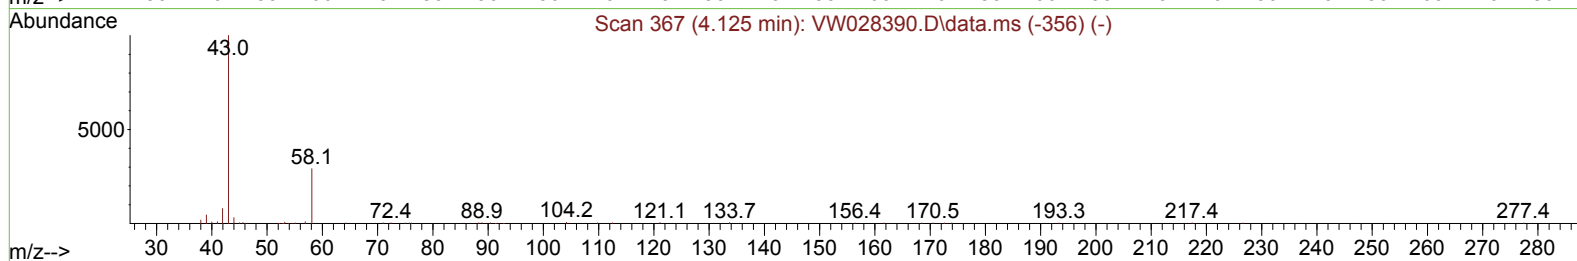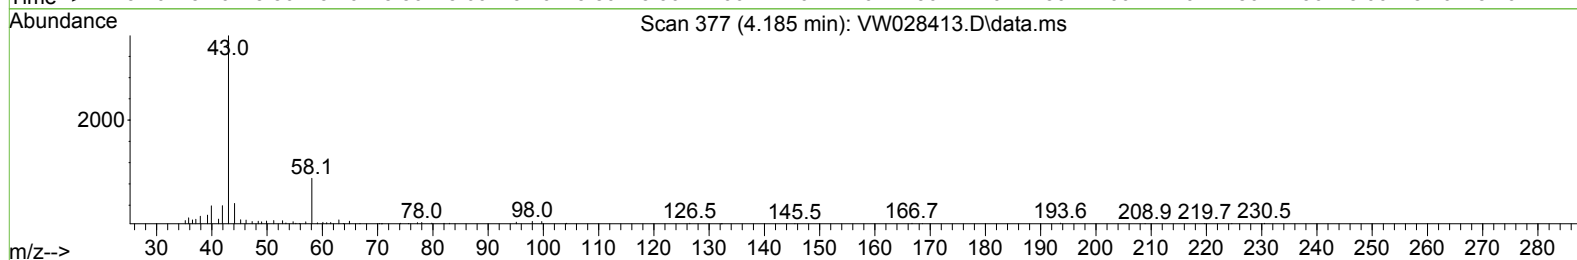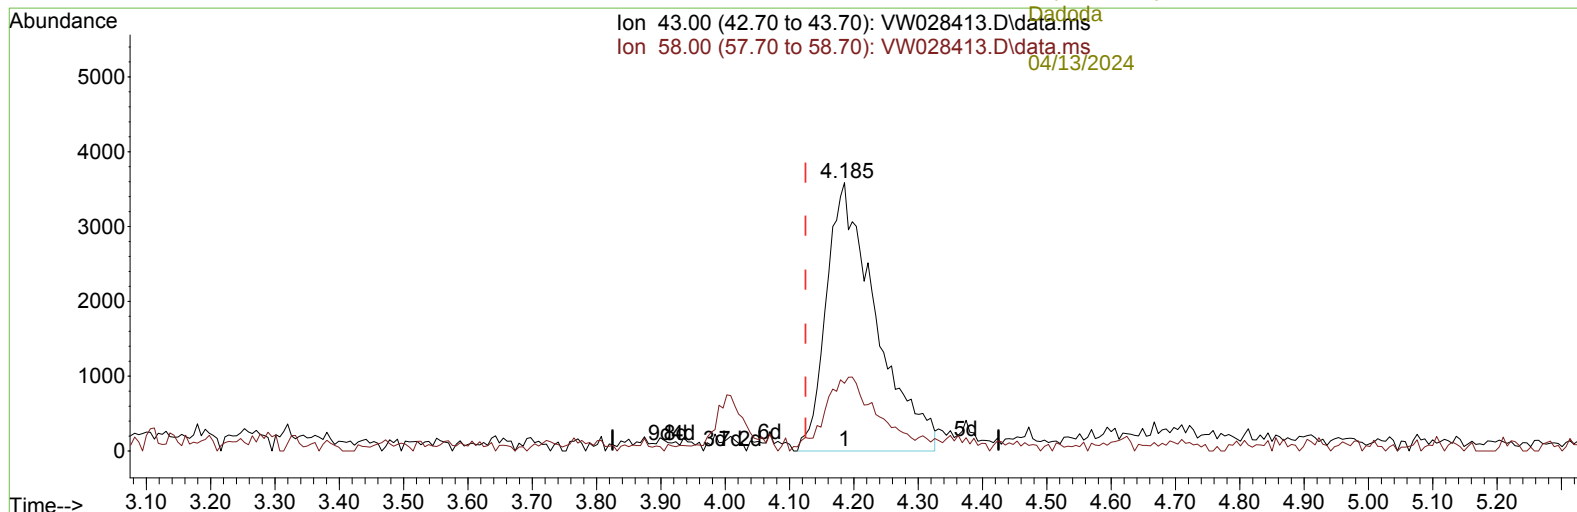

TIC: VW028413.D\data.ms

(13) Acetone (T)

4.185min (+ 0.061) 12.04 ug/L m

response 19147

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.70	14.22
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041124\
 Data File : VW028413.D
 Acq On : 11 Apr 2024 19:00
 Operator : SY/MD
 Sample : P2078-10
 Misc : 3.76g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AC7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
 Yesilyurt

04/12/2024
 Supervised By :Mahesh
 Dadoda

04/13/2024

Quant Time: Apr 12 01:01:33 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 12 00:55:02 2024
 Response via : Initial Calibration

Compound		R.T.	Q	Ion	Response	Conc	Units	Dev(Min)	Qvalue

Internal Standards									
1) 1,4-Difluorobenzene		8.843	114		431846	25.000	ug/L	0.00	
28) Chlorobenzene-d5		11.629	117		357521	25.000	ug/L	0.00	
58) 1,4-Dichlorobenzene-d4		13.556	152		111347	25.000	ug/L	0.00	
System Monitoring Compounds									
4) Vinyl Chloride-d3		2.350	65		186487	26.937	ug/L	-0.02	
Spiked Amount	25.000	Range	30	- 150	Recovery	= 107.760%			
7) Chloroethane-d5		2.887	69		139776	26.638	ug/L	-0.02	
Spiked Amount	25.000	Range	30	- 150	Recovery	= 106.560%			
11) 1,1-Dichloroethene-d2		4.009	65		66925	22.827	ug/L	-0.01	
Spiked Amount	25.000	Range	45	- 110	Recovery	= 91.320%			
21) 2-Butanone-d5		7.099	46		77118	59.527	ug/L	0.02	
Spiked Amount	50.000	Range	20	- 135	Recovery	= 119.060%			
24) Chloroform-d		7.648	84		273703	24.289	ug/L	0.00	
Spiked Amount	25.000	Range	40	- 150	Recovery	= 97.160%			
26) 1,2-Dichloroethane-d4		8.307	65		166437	28.421	ug/L	0.00	
Spiked Amount	25.000	Range	70	- 130	Recovery	= 113.680%			
32) Benzene-d6		8.270	84		552610	28.294	ug/L	0.00	
Spiked Amount	25.000	Range	20	- 135	Recovery	= 113.160%			
36) 1,2-Dichloropropane-d6		9.270	67		171206	29.490	ug/L	0.00	
Spiked Amount	25.000	Range	70	- 120	Recovery	= 117.960%			
41) Toluene-d8		10.318	98		468992	26.407	ug/L	0.00	
Spiked Amount	25.000	Range	30	- 130	Recovery	= 105.640%			
43) trans-1,3-Dichloroprop...		10.574	79		62822	27.214	ug/L	0.00	
Spiked Amount	25.000	Range	30	- 135	Recovery	= 108.840%			
47) 2-Hexanone-d5		10.922	63		54250	67.461	ug/L	0.00	
Spiked Amount	50.000	Range	20	- 135	Recovery	= 134.920%			
56) 1,1,2,2-Tetrachloroeth...		12.690	84		123575	30.169	ug/L	0.00	
Spiked Amount	25.000	Range	45	- 120	Recovery	= 120.680%#			
66) 1,2-Dichlorobenzene-d4		13.848	152		102573	29.129	ug/L	0.00	
Spiked Amount	25.000	Range	75	- 120	Recovery	= 116.520%			
Target Compounds								Qvalue	
13) Acetone		4.185	43		19147m	12.037	ug/L		

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041124\
Data File : VW028413.D
Acq On : 11 Apr 2024 19:00
Operator : SY/MD
Sample : P2078-10
Misc : 3.76g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AC7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
Yesilyurt

04/12/2024
Supervised By :Mahesh
Dadoda

04/13/2024

