

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041124\
 Data File : VW028402.D
 Acq On : 11 Apr 2024 14:37
 Operator : SY/MD
 Sample : P2052-14
 Misc : 3.48g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AF2

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/12/2024
 Supervised By :Mahesh Dadoda 04/13/2024

Quant Time: Apr 12 00:58:44 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 12 00:55:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	362026	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	306803	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.550	152	104196	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	126690	21.829	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	87.320%		
7) Chloroethane-d5	2.893	69	102186	23.230	ug/L	-0.01
Spiked Amount 25.000	Range 30 - 150		Recovery =	92.920%		
11) 1,1-Dichloroethene-d2	4.021	65	51633	21.008	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	84.040%		
21) 2-Butanone-d5	7.081	46	51292	47.228	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	94.460%		
24) Chloroform-d	7.648	84	216574	22.926	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	91.720%		
26) 1,2-Dichloroethane-d4	8.307	65	122558m	24.964	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	99.840%		
32) Benzene-d6	8.276	84	433533	25.866	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	103.480%		
36) 1,2-Dichloropropane-d6	9.270	67	131639	26.423	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	105.680%		
41) Toluene-d8	10.319	98	364319	23.905	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	95.600%		
43) trans-1,3-Dichloroprop...	10.575	79	42685	21.548	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	86.200%		
47) 2-Hexanone-d5	10.922	63	34750	50.355	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	100.720%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	91152	25.932	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	103.720%		
66) 1,2-Dichlorobenzene-d4	13.848	152	86863	26.360	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	105.440%		
Target Compounds					Qvalue	
13) Acetone	4.125	43	10001	7.500	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041124\
Data File : VW028402.D
Acq On : 11 Apr 2024 14:37
Operator : SY/MD
Sample : P2052-14
Misc : 3.48g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
C0AF2

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 04/12/2024
Supervised By :Mahesh Dadoda 04/13/2024

Quant Time: Apr 12 00:58:44 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 12 00:55:02 2024
Response via : Initial Calibration

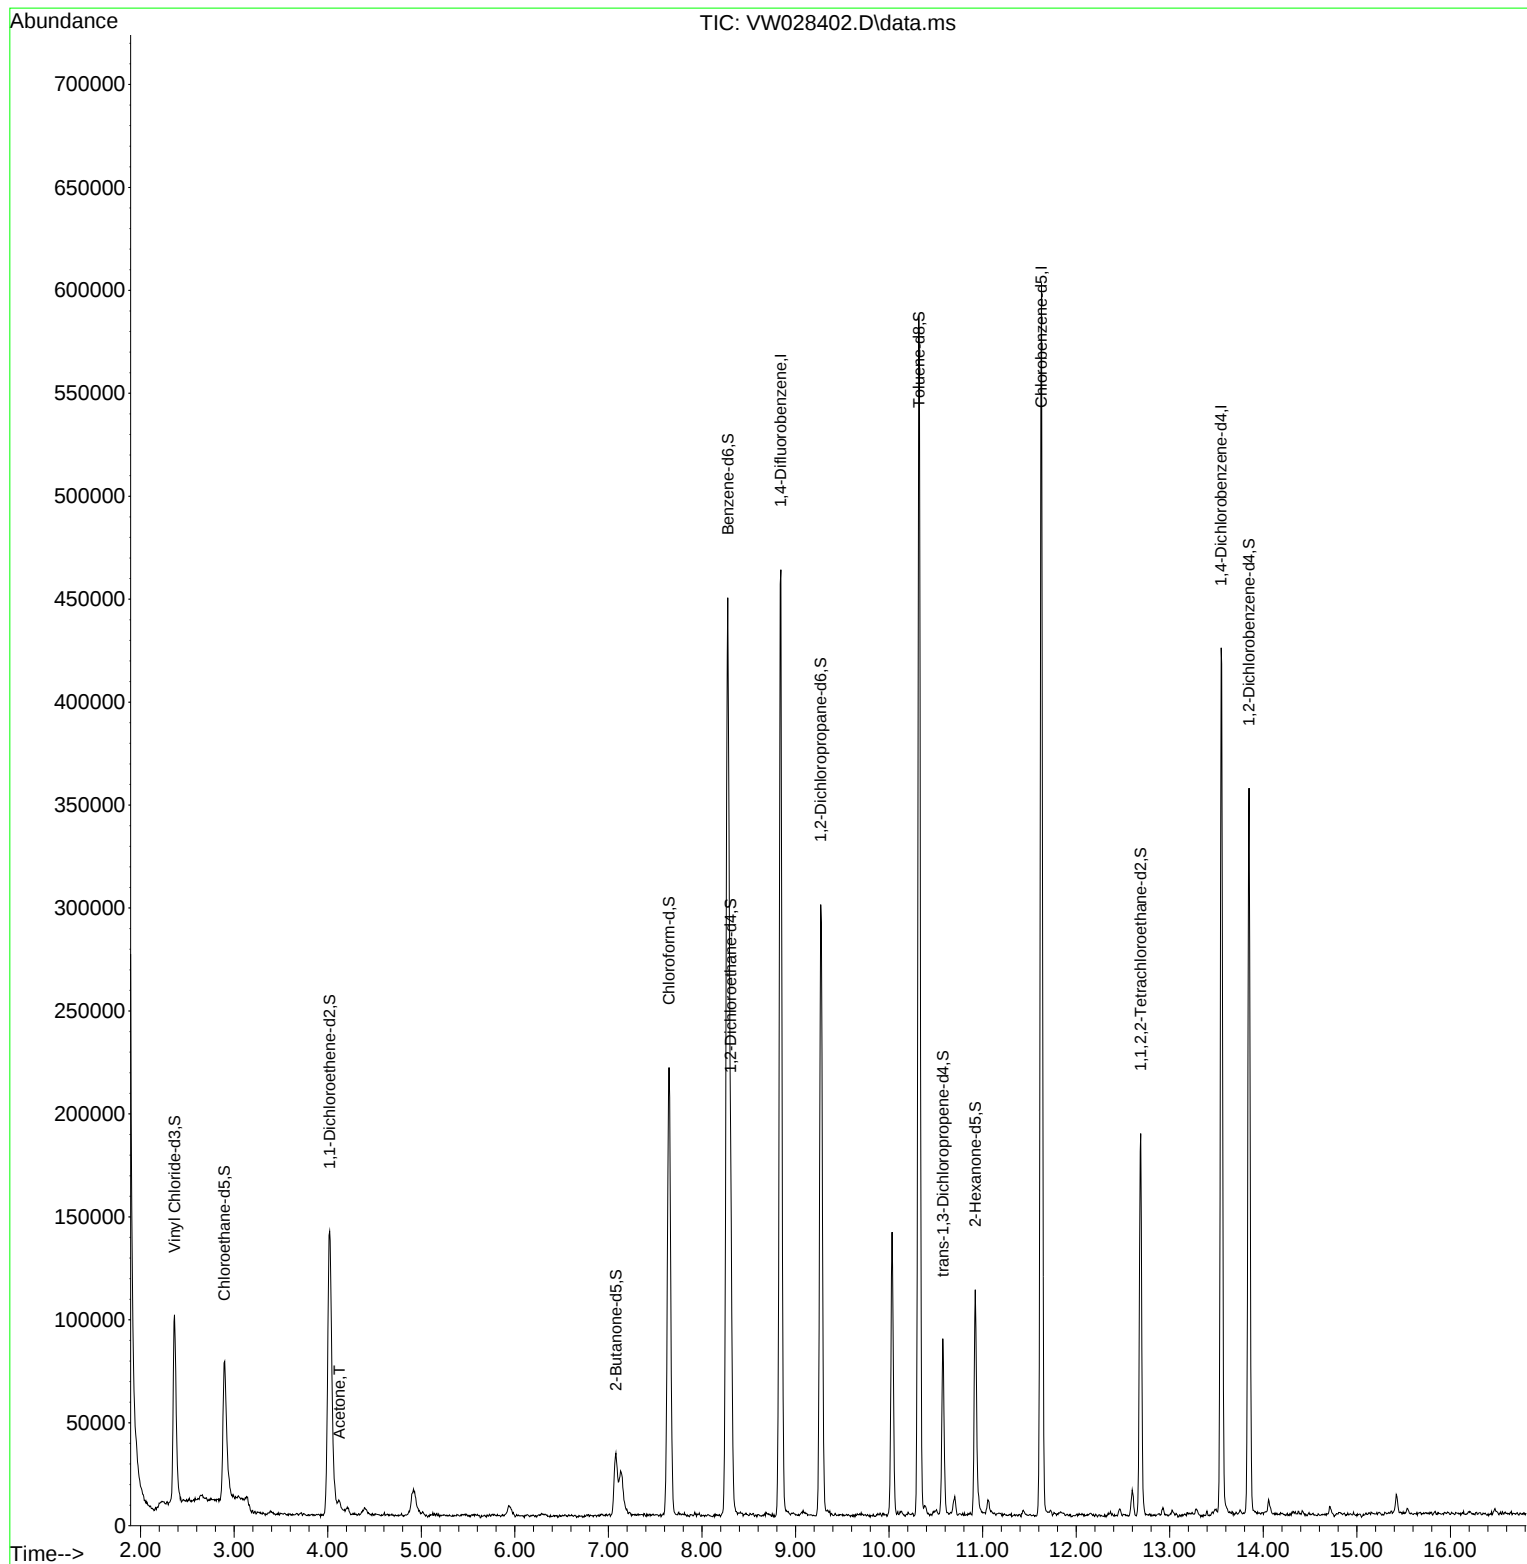

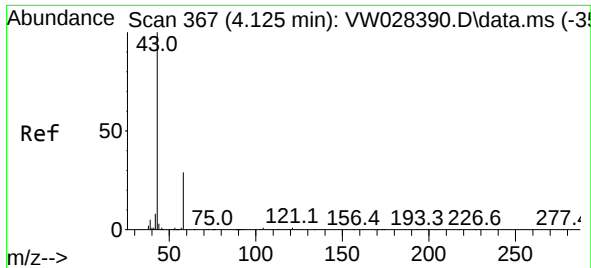

#13
 Acetone
 Concen: 7.500 ug/L
 RT: 4.125 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: VW028402.D
 Acq: 11 Apr 2024 14:37

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AF2

Tgt Ion: 43 Resp: 1000
 Ion Ratio Lower Upper
 43 100
 58 29.0 0.0 53.4

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/12/2024
 Supervised By :Mahesh Dadoda 04/13/2024

