

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041124\
 Data File : VW028410.D
 Acq On : 11 Apr 2024 17:48
 Operator : SY/MD
 Sample : P2078-05
 Misc : 4.08g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AA9

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/12/2024
 Supervised By :Mahesh Dadoda 04/13/2024

Quant Time: Apr 12 01:00:47 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 12 00:55:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	197344	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	175673	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	69380	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	76396	24.147	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	96.600%		
7) Chloroethane-d5	2.905	69	60630	25.285	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	101.120%		
11) 1,1-Dichloroethene-d2	4.021	65	32007	23.890	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	95.560%		
21) 2-Butanone-d5	7.081	46	30393	51.338	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	102.680%		
24) Chloroform-d	7.648	84	127740	24.806	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	99.240%		
26) 1,2-Dichloroethane-d4	8.307	65	74249m	27.745	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	111.000%		
32) Benzene-d6	8.276	84	253929	26.459	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	105.840%		
36) 1,2-Dichloropropane-d6	9.276	67	77260	27.084	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	108.320%		
41) Toluene-d8	10.325	98	219477	25.150	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	100.600%		
43) trans-1,3-Dichloroprop...	10.575	79	27007	23.810	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	95.240%		
47) 2-Hexanone-d5	10.922	63	20258	51.268	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	102.540%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	55993	27.821	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	111.280%		
66) 1,2-Dichlorobenzene-d4	13.849	152	62101	28.303	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	113.200%		
Target Compounds					Qvalue	
13) Acetone	4.131	43	9362	12.879	ug/L	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041124\
Data File : VW028410.D
Acq On : 11 Apr 2024 17:48
Operator : SY/MD
Sample : P2078-05
Misc : 4.08g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
C0AA9

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 04/12/2024
Supervised By :Mahesh Dadoda 04/13/2024


Quant Time: Apr 12 01:00:47 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 12 00:55:02 2024
Response via : Initial Calibration

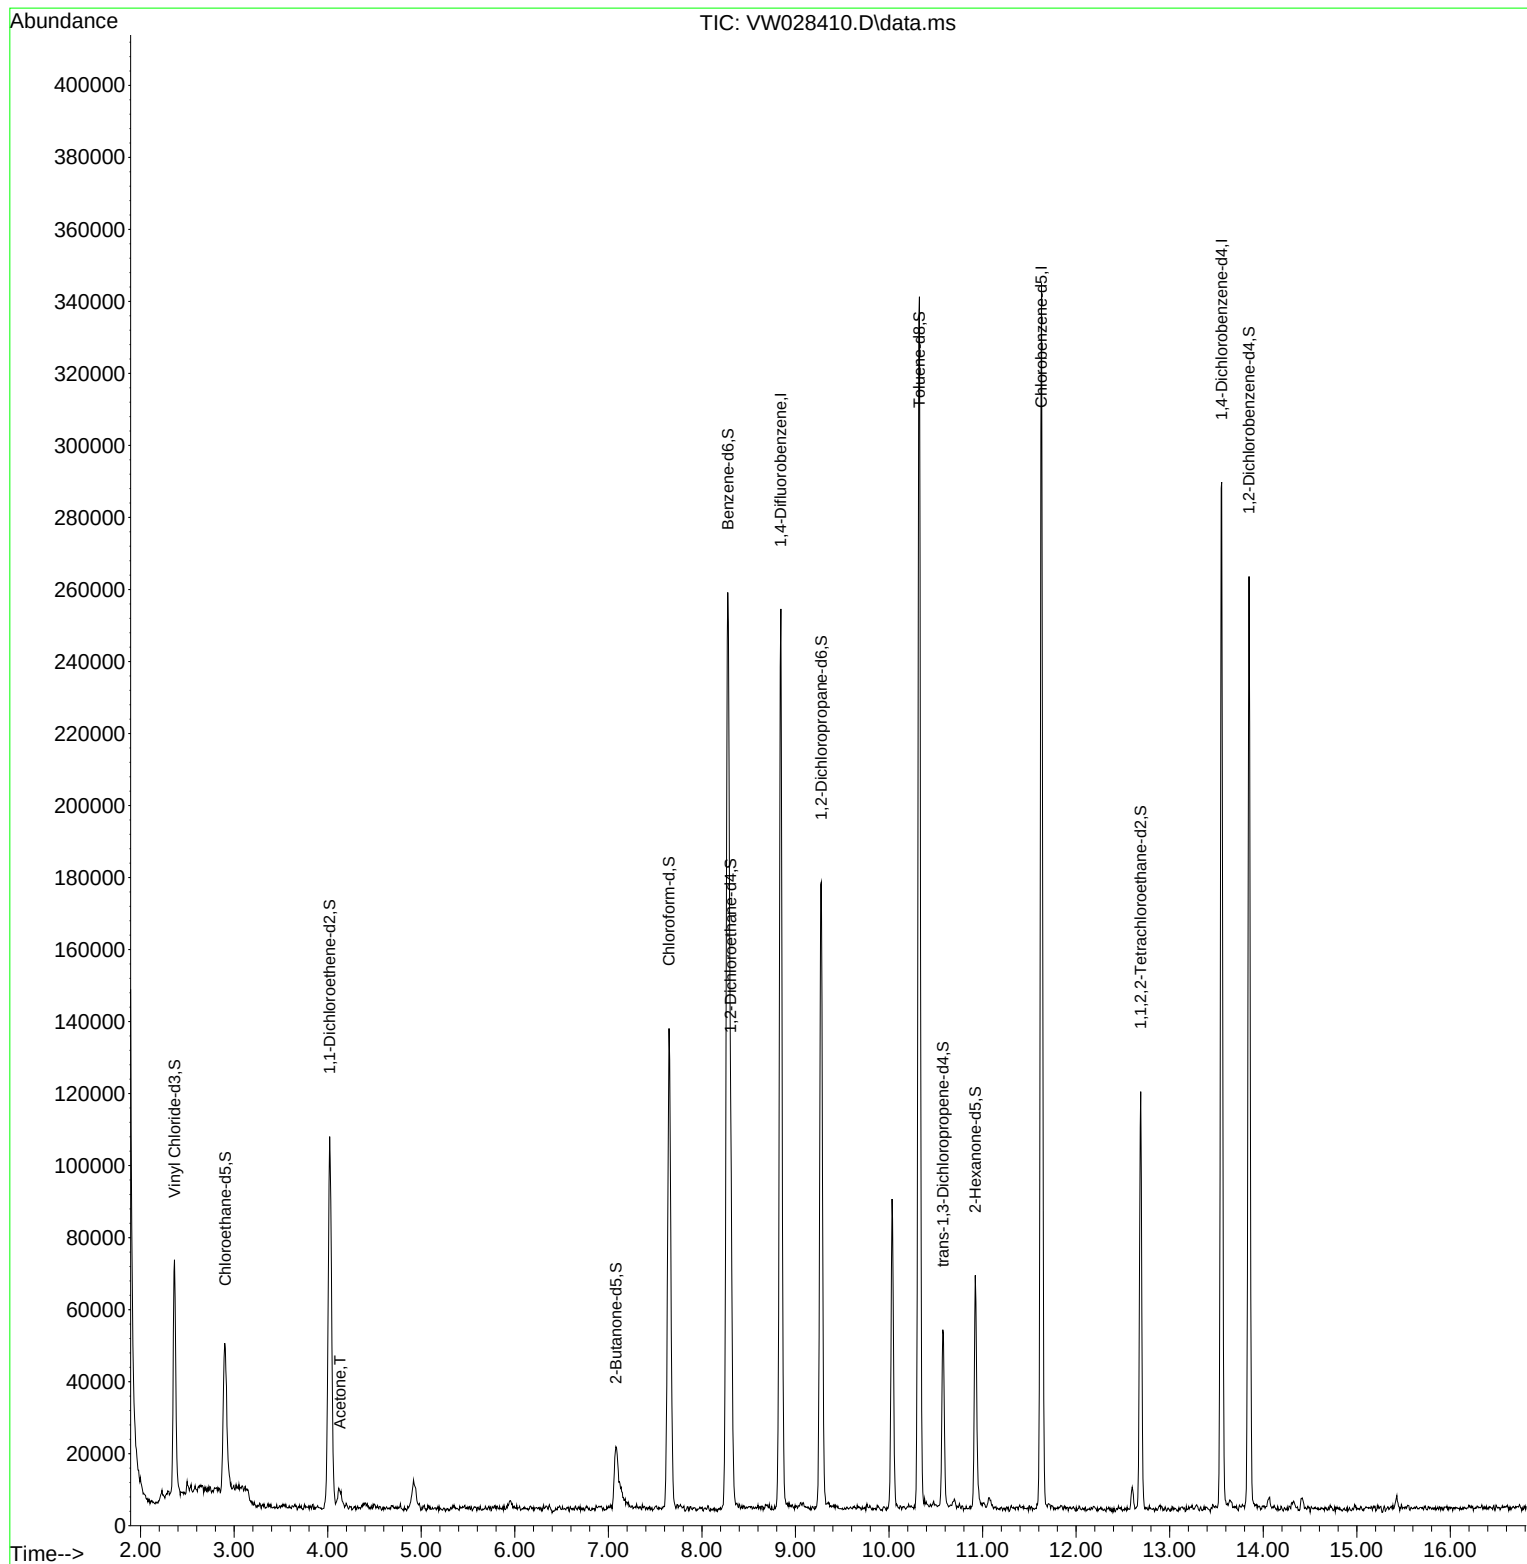

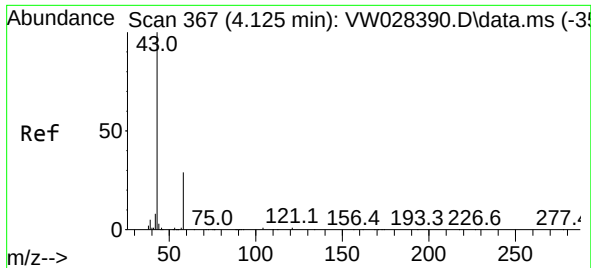

#13
 Acetone
 Concen: 12.879 ug/L
 RT: 4.131 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW028410.D
 Acq: 11 Apr 2024 17:48

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AA9

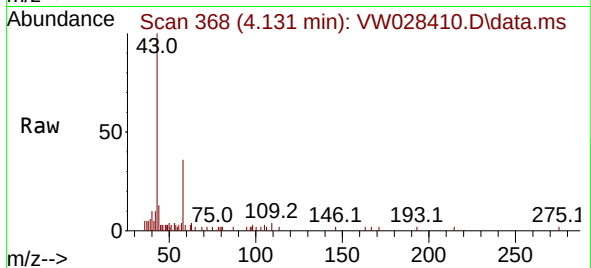

Tgt Ion: 43 Resp: 936
 Ion Ratio Lower Upper
 43 100
 58 33.6 0.0 53.4

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/12/2024
 Supervised By :Mahesh Dadoda 04/13/2024

