

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041124\
 Data File : VW028414.D
 Acq On : 11 Apr 2024 19:23
 Operator : SY/MD
 Sample : P2078-12
 Misc : 5.26g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AC9

Quant Time: Apr 12 01:01:54 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 12 00:55:02 2024
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		8.843	114	272796	25.000	ug/L	0.00
28) Chlorobenzene-d5		11.629	117	245135	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.556	152	94259	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.350	65	127766	29.215	ug/L	-0.02
Spiked Amount	25.000	Range	30 - 150	Recovery	=	116.840%	
7) Chloroethane-d5		2.887	69	100010	30.172	ug/L	-0.02
Spiked Amount	25.000	Range	30 - 150	Recovery	=	120.680%	
11) 1,1-Dichloroethene-d2		4.003	65	46371	25.038	ug/L	-0.02
Spiked Amount	25.000	Range	45 - 110	Recovery	=	100.160%	
21) 2-Butanone-d5		7.100	46	51106	62.448	ug/L	0.02
Spiked Amount	50.000	Range	20 - 135	Recovery	=	124.900%	
24) Chloroform-d		7.648	84	196129	27.552	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	110.200%	
26) 1,2-Dichloroethane-d4		8.307	65	112443	30.396	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	121.600%	
32) Benzene-d6		8.270	84	380238	28.394	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	113.560%	
36) 1,2-Dichloropropane-d6		9.270	67	118485	29.766	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	119.080%	
41) Toluene-d8		10.325	98	328450	26.973	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	107.880%	
43) trans-1,3-Dichloroprop...		10.575	79	40800	25.778	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	103.120%	
47) 2-Hexanone-d5		10.922	63	33426	60.622	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	121.240%	
56) 1,1,2,2-Tetrachloroeth...		12.690	84	86517	30.806	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	123.240%#	
66) 1,2-Dichlorobenzene-d4		13.848	152	85771	28.773	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	115.080%	
Target Compounds							Qvalue
13) Acetone		4.173	43	8631	8.589	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041124\
Data File : VW028414.D
Acq On : 11 Apr 2024 19:23
Operator : SY/MD
Sample : P2078-12
Misc : 5.26g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AC9

Quant Time: Apr 12 01:01:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 12 00:55:02 2024
Response via : Initial Calibration

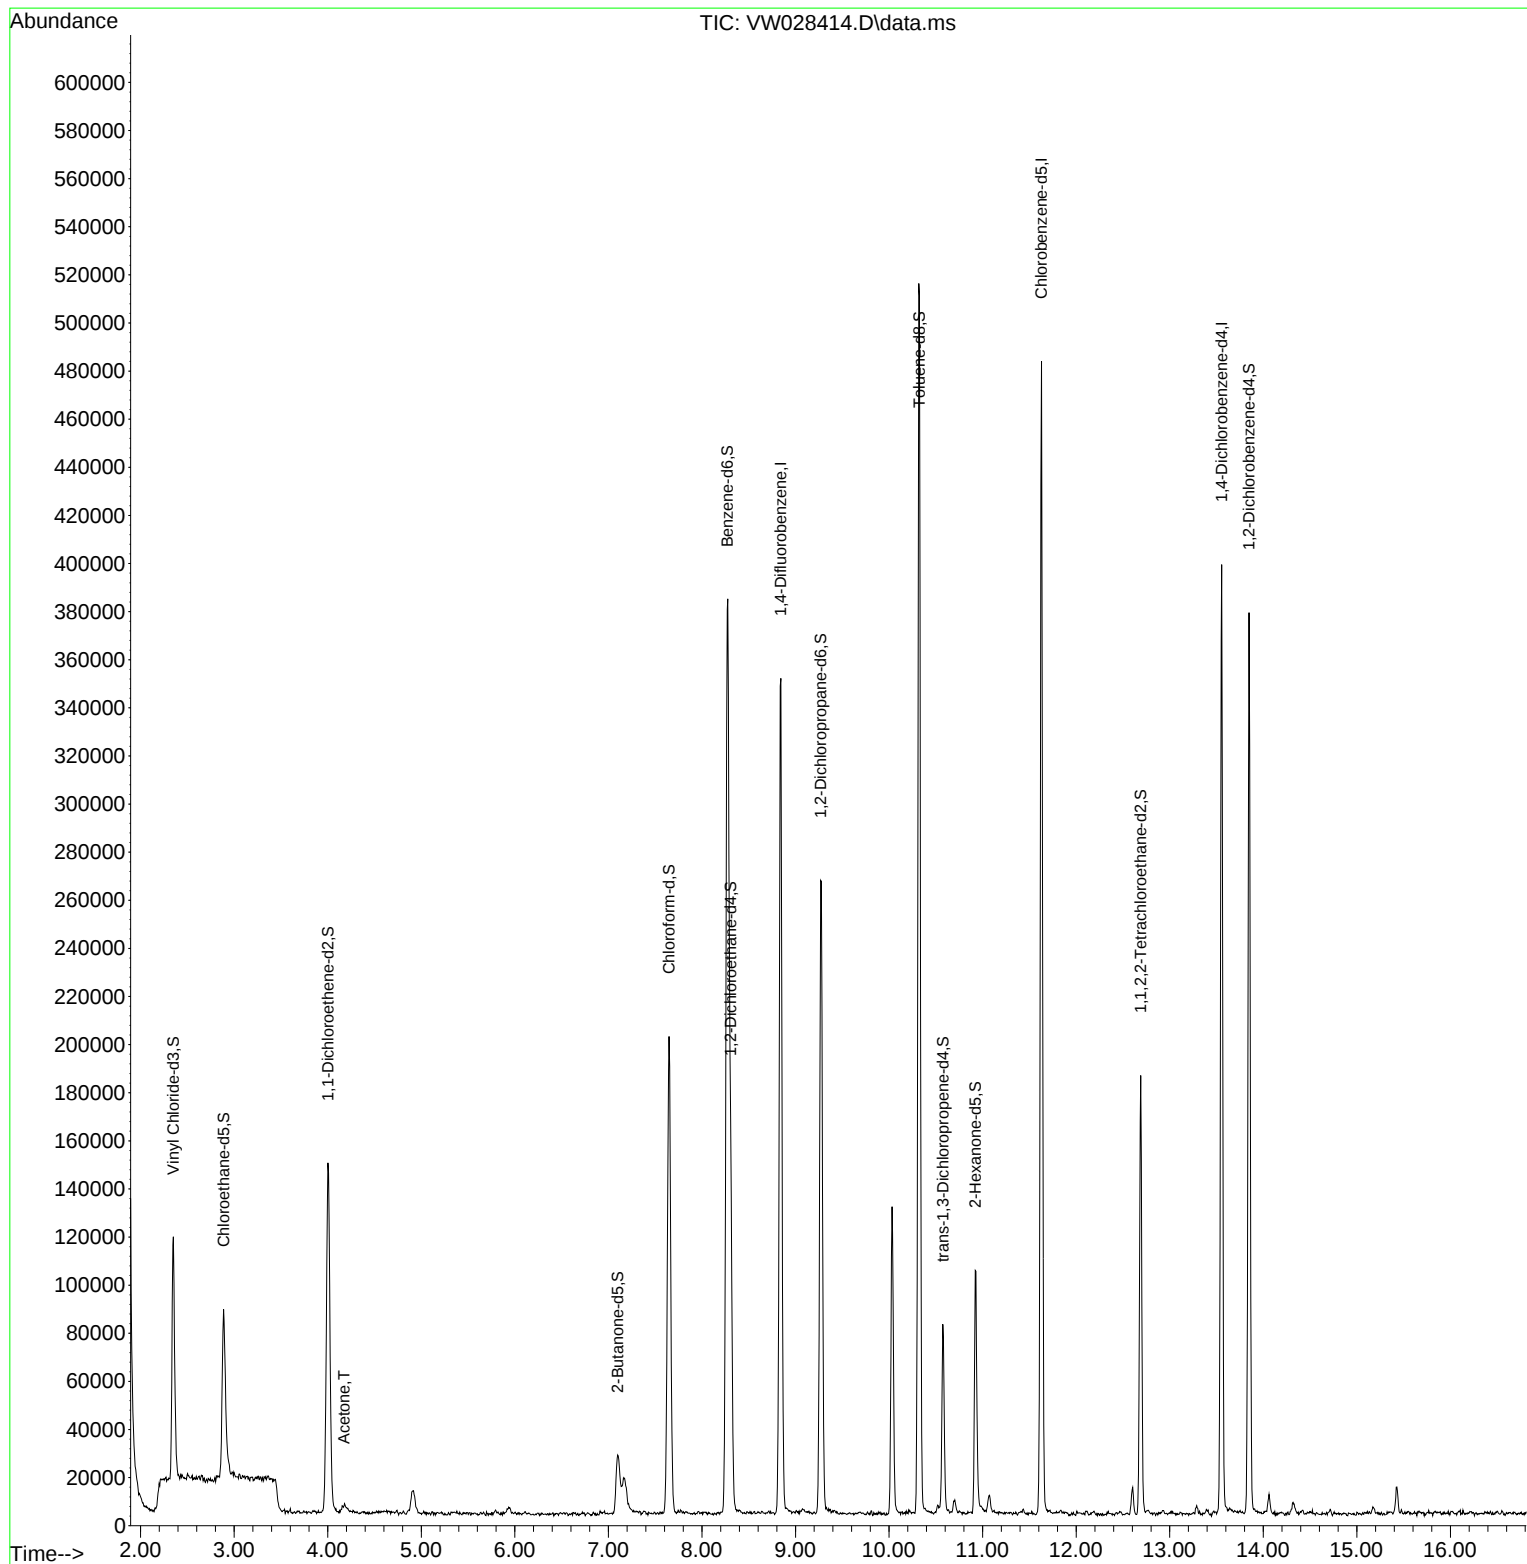

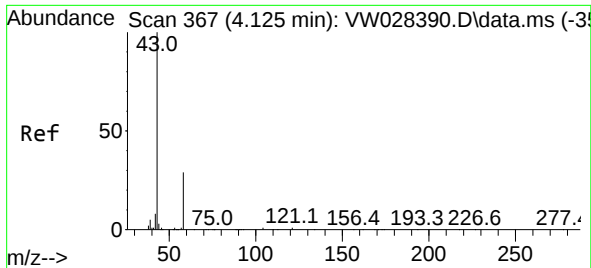

#13
 Acetone
 Concen: 8.589 ug/L
 RT: 4.173 min Scan# 31
 Delta R.T. 0.049 min
 Lab File: VW028414.D
 Acq: 11 Apr 2024 19:23

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AC9

Tgt Ion: 43 Resp: 8631
 Ion Ratio Lower Upper
 43 100
 58 24.0 0.0 53.4

