




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041224\
Data File : VW028432.D
Acq On : 12 Apr 2024 15:39
Operator : SY/MD
Sample : P2078-17RE
Misc : 4.67g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
COAL8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/15/2024
Supervised By :Mahesh Dadoda 04/15/2024

Quant Time: Apr 12 23:15:40 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 12 23:09:31 2024
Response via : Initial Calibration

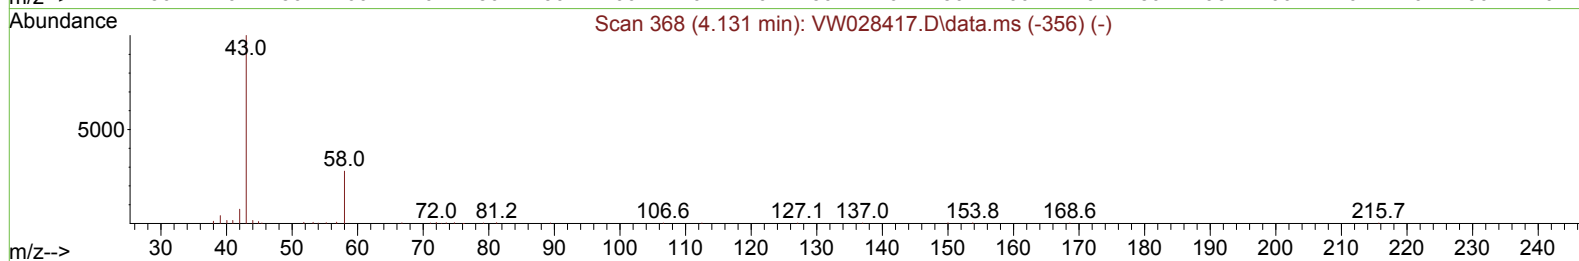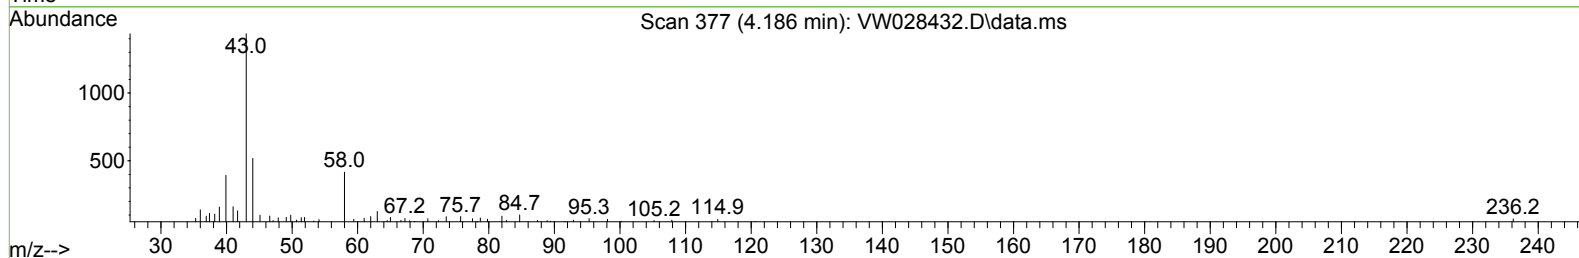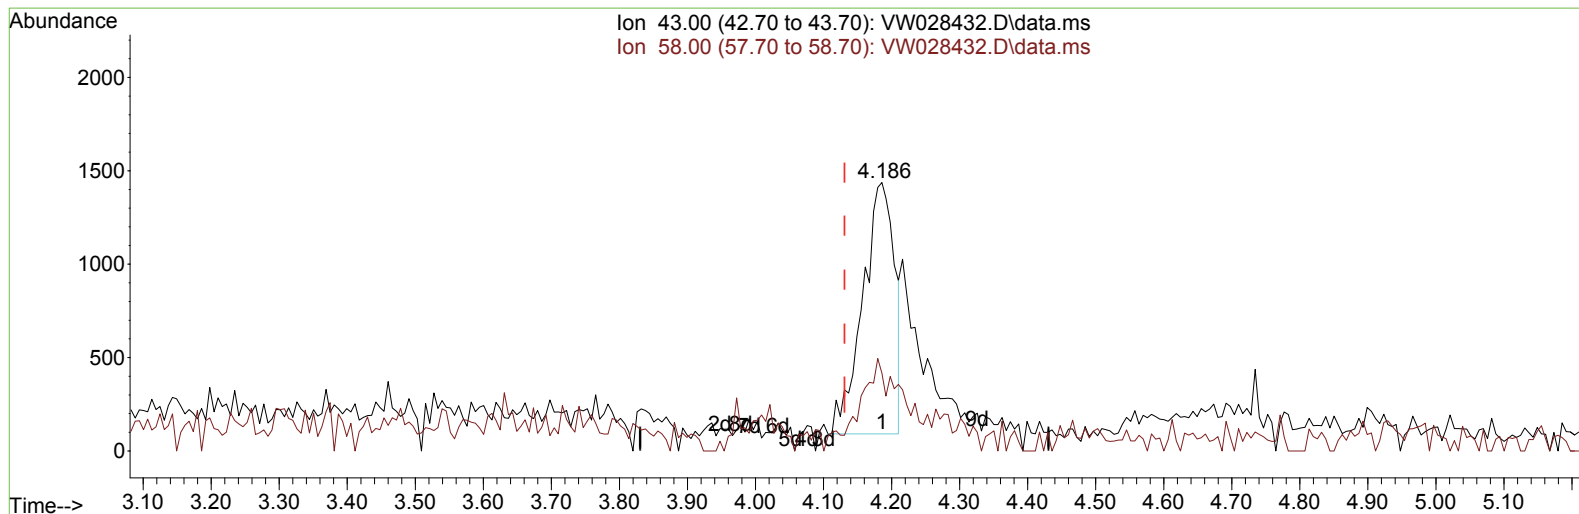

TIC: VW028432.D\data.ms

(13) Acetone (T)

4.186min (+ 0.055) 2.72 ug/L

response 4353

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.70	2.92
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041224\
Data File : VW028432.D
Acq On : 12 Apr 2024 15:39
Operator : SY/MD
Sample : P2078-17RE
Misc : 4.67g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AL8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/15/2024
Supervised By :Mahesh Dadoda 04/15/2024

Quant Time: Apr 12 23:15:40 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 12 23:09:31 2024
Response via : Initial Calibration

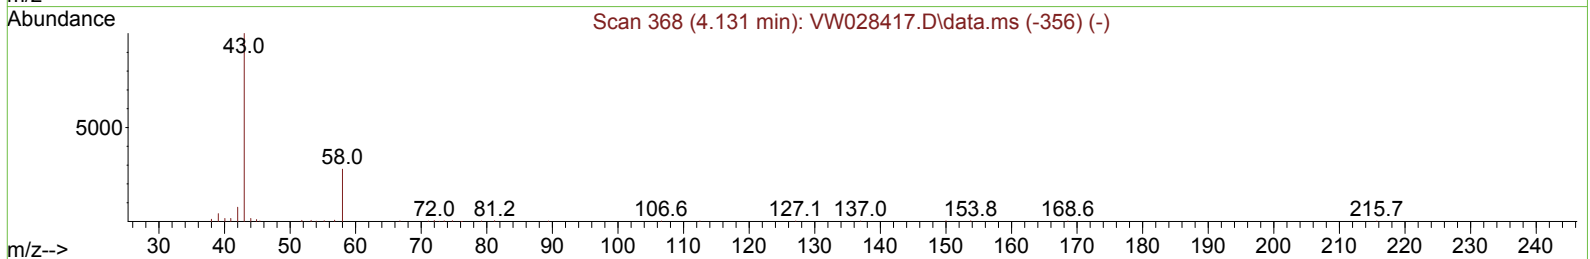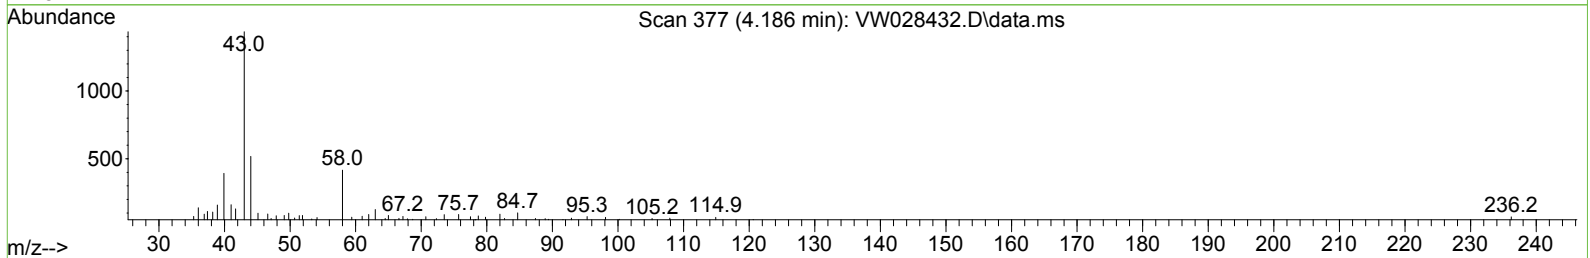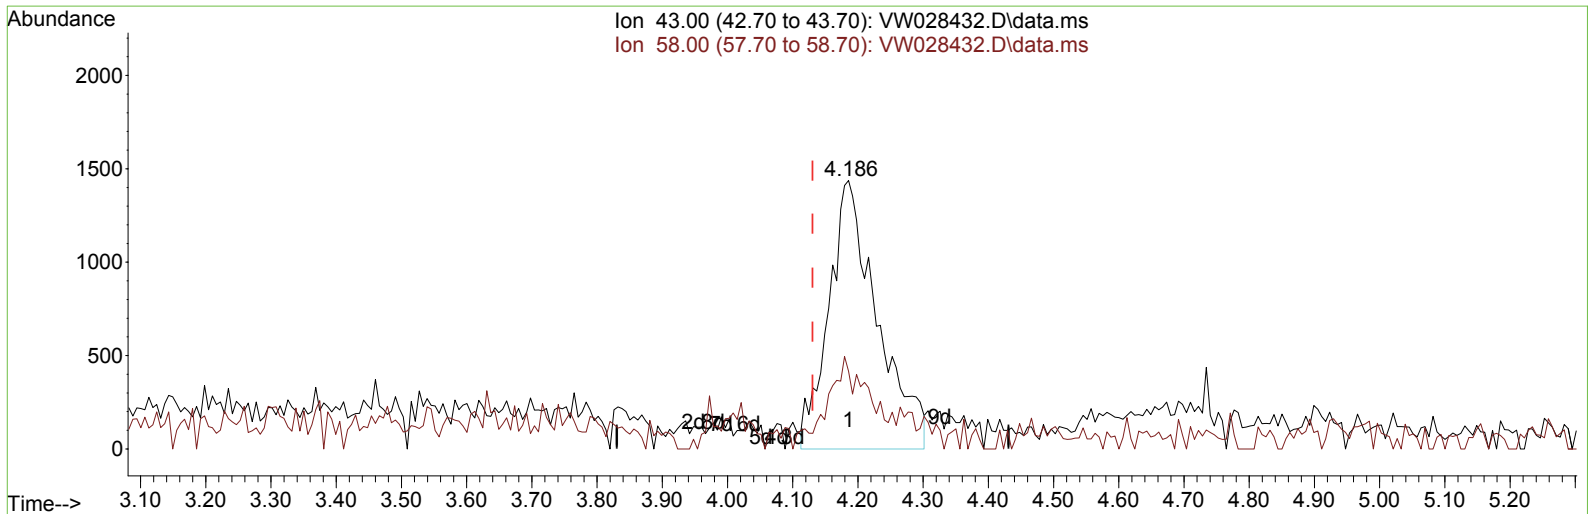

TIC: VW028432.D\data.ms

(13) Acetone (T)

4.186min (+ 0.055) 4.63 ug/L m

response 7425

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.70	1.71
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041224\
Data File : VW028432.D
Acq On : 12 Apr 2024 15:39
Operator : SY/MD
Sample : P2078-17RE
Misc : 4.67g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AL8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/15/2024
Supervised By :Mahesh Dadoda 04/15/2024

Quant Time: Apr 12 23:15:40 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 12 23:09:31 2024
Response via : Initial Calibration

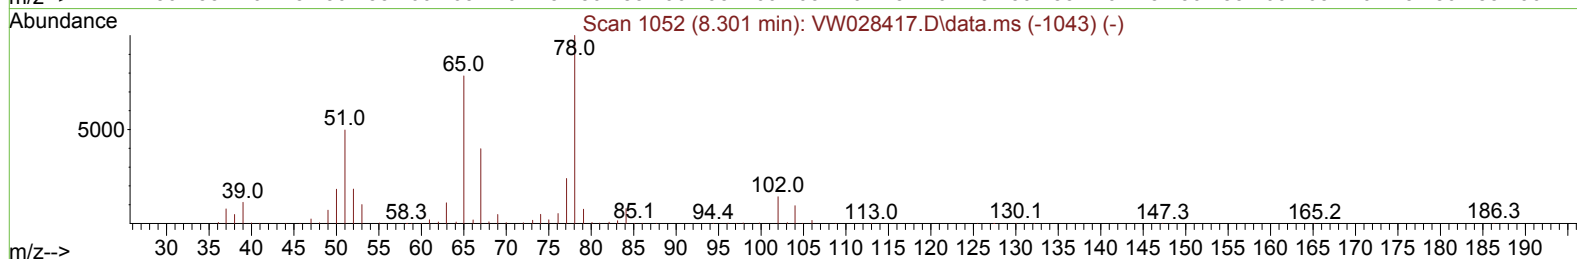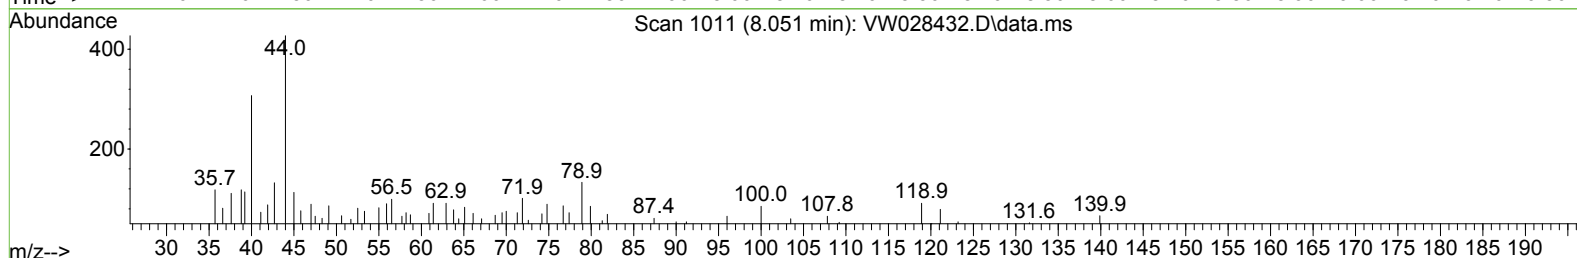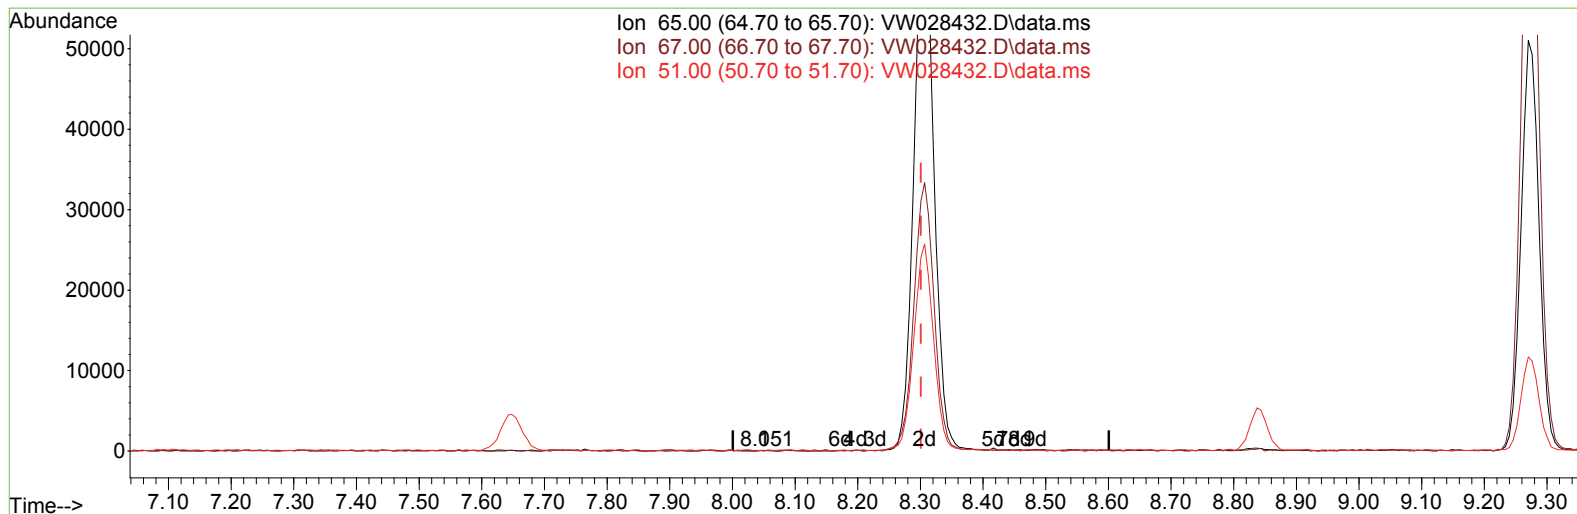

TIC: VW028432.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.051min (-0.250) 0.02 ug/L

response 99

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.10	54.55
51.00	108.40	121.21
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041224\
Data File : VW028432.D
Acq On : 12 Apr 2024 15:39
Operator : SY/MD
Sample : P2078-17RE
Misc : 4.67g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
COAL8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/15/2024
Supervised By :Mahesh Dadoda 04/15/2024

Quant Time: Apr 12 23:15:40 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 12 23:09:31 2024
Response via : Initial Calibration

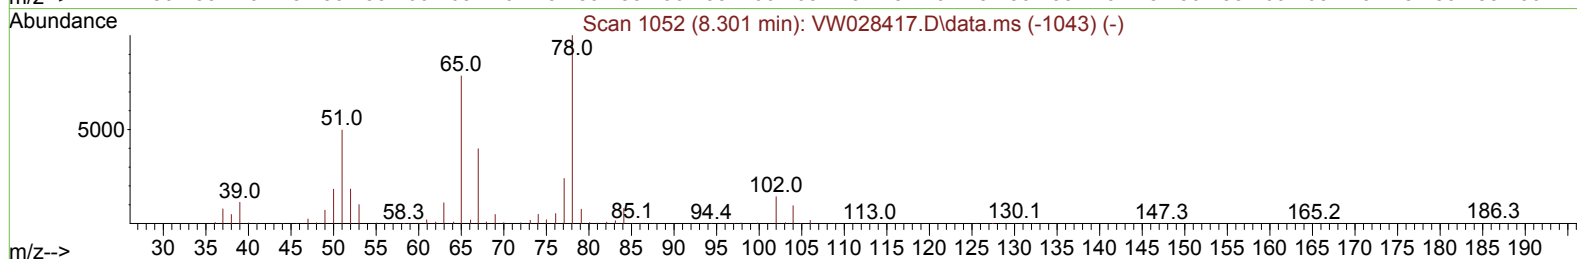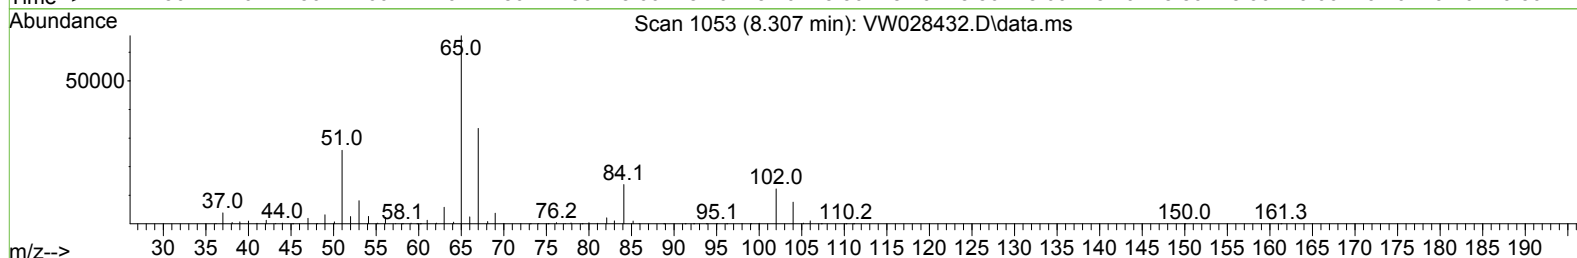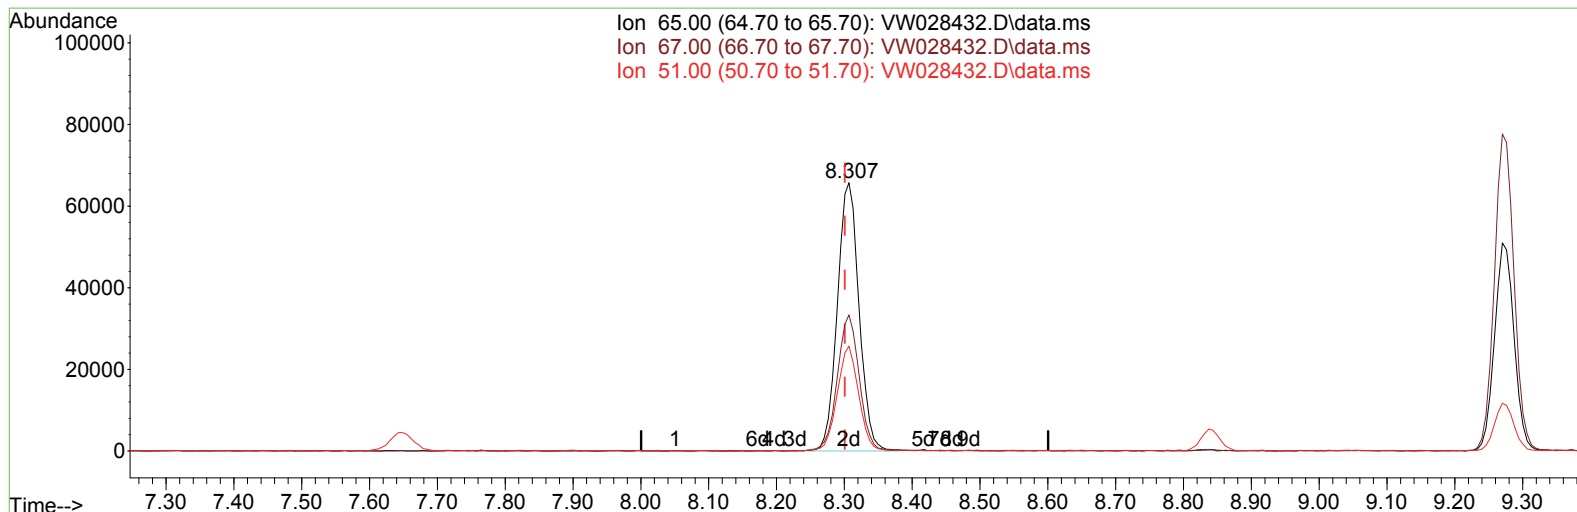

TIC: VW028432.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.006) 24.73 ug/L m

response 145922

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.10	0.04#
51.00	108.40	0.08#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041224\
 Data File : VW028432.D
 Acq On : 12 Apr 2024 15:39
 Operator : SY/MD
 Sample : P2078-17RE
 Misc : 4.67g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 COAL8

Manual IntegrationsAPPROVED

Quant Time: Apr 12 23:15:40 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 12 23:09:31 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/15/2024
 Supervised By :Mahesh Dadoda 04/15/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	435115	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	342929	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.550	152	124635	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.351	65	152372	21.844	ug/L	-0.02
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.360%
7) Chloroethane-d5	2.887	69	119152	22.537	ug/L	-0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.160%
11) 1,1-Dichloroethene-d2	3.997	65	59400	20.108	ug/L	-0.02
Spiked Amount	25.000	Range	45 - 110	Recovery	=	80.440%
21) 2-Butanone-d5	7.106	46	66508	50.952	ug/L	0.02
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.900%
24) Chloroform-d	7.648	84	251747	22.172	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.680%
26) 1,2-Dichloroethane-d4	8.307	65	145922m	24.731	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.920%
32) Benzene-d6	8.270	84	505579	26.987	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	107.960%
36) 1,2-Dichloropropane-d6	9.270	67	155743	27.968	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	111.880%
41) Toluene-d8	10.319	98	432899	25.412	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	101.640%
43) trans-1,3-Dichloroprop...	10.575	79	49495	22.353	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.400%
47) 2-Hexanone-d5	10.928	63	48417	62.769	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	125.540%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	113007	28.763	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	115.040%
66) 1,2-Dichlorobenzene-d4	13.849	152	112341	28.501	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	114.000%
Target Compounds					Qvalue	
13) Acetone	4.186	43	7425m	4.633	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041224\
Data File : VW028432.D
Acq On : 12 Apr 2024 15:39
Operator : SY/MD
Sample : P2078-17RE
Misc : 4.67g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AL8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/15/2024
Supervised By :Mahesh Dadoda 04/15/2024

Quant Time: Apr 12 23:15:40 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 12 23:09:31 2024
Response via : Initial Calibration

