

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041224\
 Data File : VW028428.D
 Acq On : 12 Apr 2024 14:04
 Operator : SY/MD
 Sample : P2052-03RE
 Misc : 4.56g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AB2RE

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/15/2024
 Supervised By :Mahesh Dadoda 04/15/2024

Quant Time: Apr 12 23:14:38 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 12 23:09:31 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	84651	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	68240	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	18020	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	30866	22.744	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	90.960%		
7) Chloroethane-d5	2.893	69	25240	24.539	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	98.160%		
11) 1,1-Dichloroethene-d2	4.027	65	12188	21.208	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	84.840%		
21) 2-Butanone-d5	7.087	46	15857m	62.442	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	124.880%		
24) Chloroform-d	7.654	84	53371	24.162	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	96.640%		
26) 1,2-Dichloroethane-d4	8.307	65	32618	28.415	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	113.640%		
32) Benzene-d6	8.276	84	102102	27.389	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	109.560%		
36) 1,2-Dichloropropane-d6	9.276	67	33340	30.088	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	120.360%#		
41) Toluene-d8	10.325	98	83331	24.582	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	98.320%		
43) trans-1,3-Dichloroprop...	10.574	79	9751	22.131	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	88.520%		
47) 2-Hexanone-d5	10.922	63	9642	62.817	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	125.640%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	25287	32.344	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	129.360%#		
66) 1,2-Dichlorobenzene-d4	13.848	152	18982	33.308	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	133.240%#		
Target Compounds					Qvalue	
13) Acetone	4.137	43	3530m	11.321	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041224\
Data File : VW028428.D
Acq On : 12 Apr 2024 14:04
Operator : SY/MD
Sample : P2052-03RE
Misc : 4.56g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
C0AB2RE

Quant Time: Apr 12 23:14:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 12 23:09:31 2024
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 04/15/2024
Supervised By :Mahesh Dadoda 04/15/2024

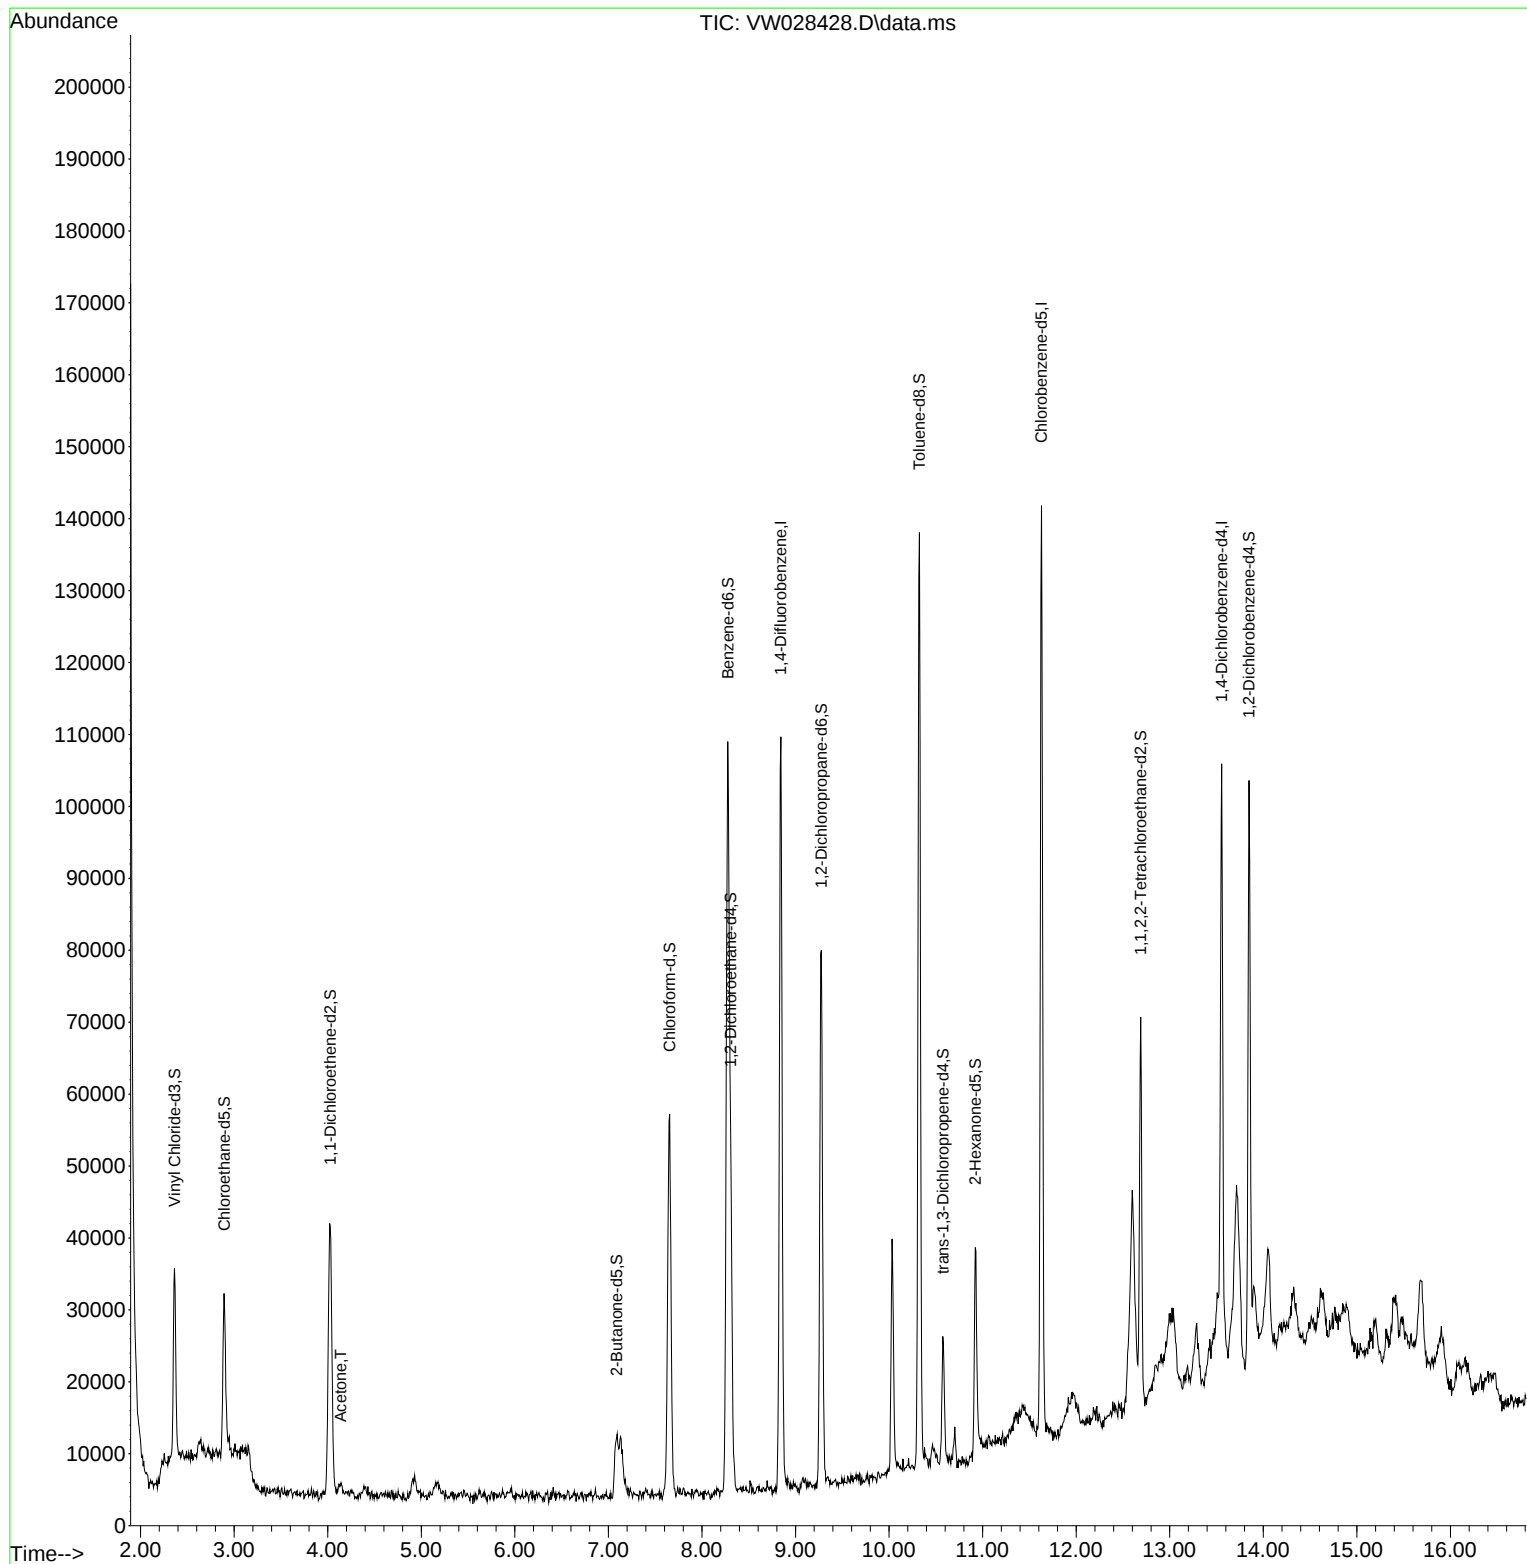

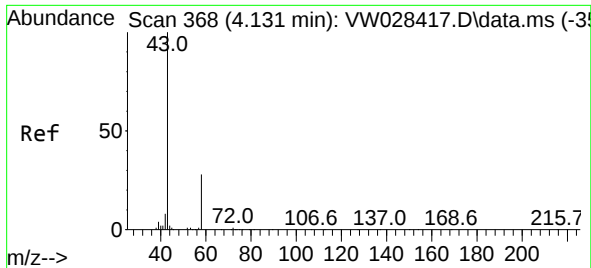

#13
 Acetone
 Concen: 11.321 ug/L m
 RT: 4.137 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW028428.D
 Acq: 12 Apr 2024 14:04

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AB2RE

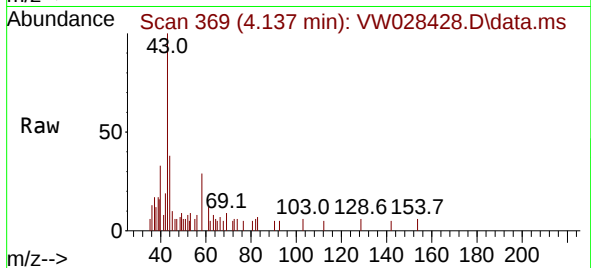

Tgt Ion: 43 Resp: 3530
 Ion Ratio Lower Upper
 43 100
 58 3.4 0.0 53.4

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/15/2024
 Supervised By :Mahesh Dadoda 04/15/2024

