

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041322\
 Data File : VW022525.D
 Acq On : 13 Apr 2022 12:29
 Operator : SY/VA
 Sample : N2373-02RE
 Misc : 5.85g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFD3RE

Quant Time: Apr 14 01:32:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 14 01:27:44 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	295955	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	211985	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	64500	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	117689	17.988	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.960%
7) Chloroethane-d5	2.885	69	86054	20.987	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.960%
11) 1,1-Dichloroethene-d2	4.013	63	120917	14.249	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.000%
21) 2-Butanone-d5	7.080	46	89235	78.121	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	156.240%#
24) Chloroform-d	7.647	84	234058	25.302	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	101.200%
26) 1,2-Dichloroethane-d4	8.305	65	148021	28.006	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	112.040%
32) Benzene-d6	8.275	84	405272	31.292	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	125.160%
36) 1,2-Dichloropropane-d6	9.274	67	132513	35.356	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	141.440%#
41) Toluene-d8	10.323	98	315654	24.885	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	99.520%
43) trans-1,3-Dichloroprop...	10.579	79	47110	26.633	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	106.520%
47) 2-Hexanone-d5	10.927	63	69086	99.073	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	198.140%#
56) 1,1,2,2-Tetrachloroeth...	12.688	84	121669	38.178	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	152.720%#
66) 1,2-Dichlorobenzene-d4	13.847	152	60367	26.424	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	105.680%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.036	75	4394	0.803	ug/L #	46


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041322\
Data File : VW022525.D
Acq On : 13 Apr 2022 12:29
Operator : SY/VA
Sample : N2373-02RE
Misc : 5.85g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFFD3RE


Quant Time: Apr 14 01:32:16 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 14 01:27:44 2022
Response via : Initial Calibration

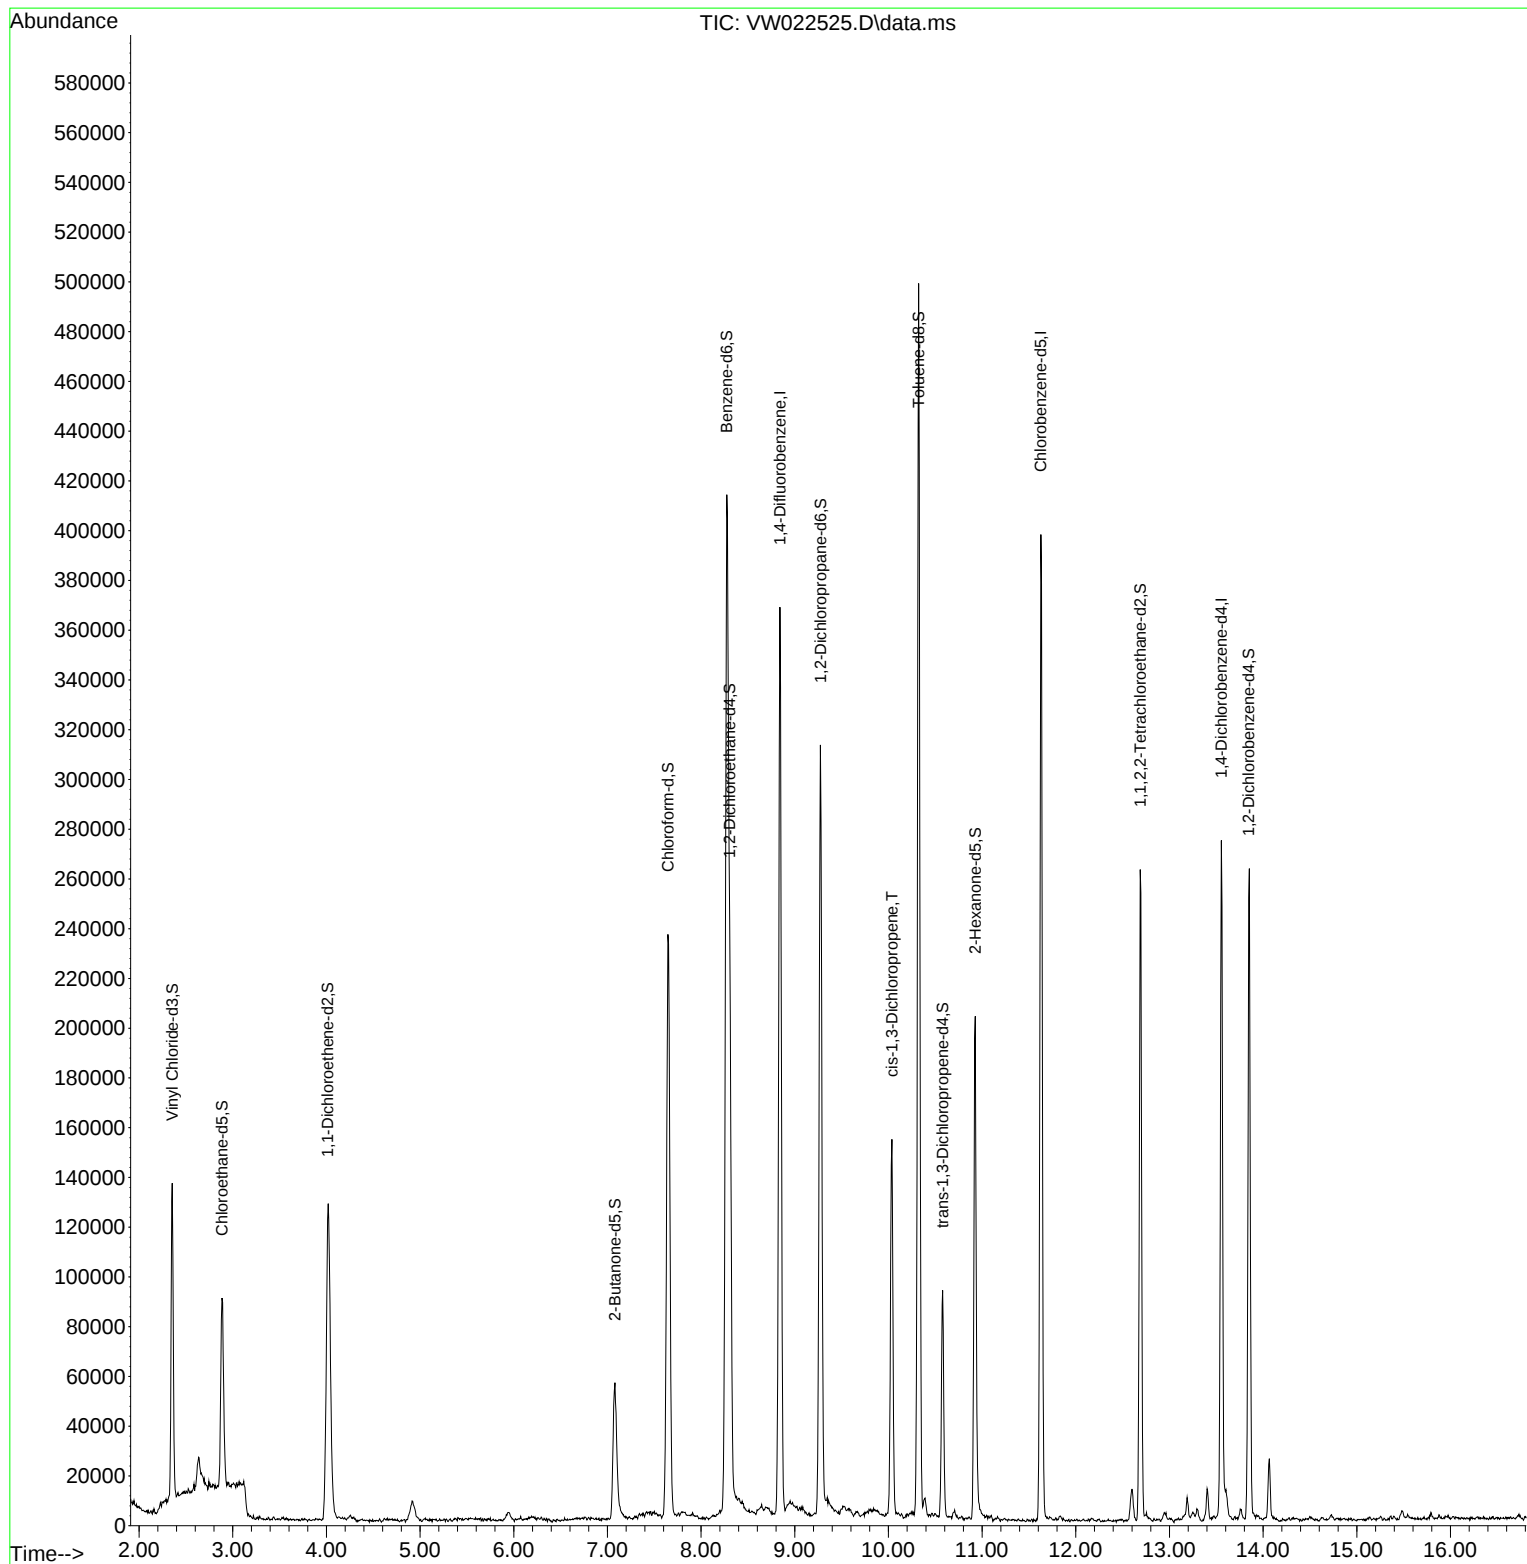

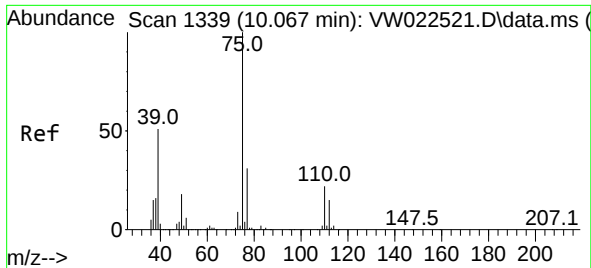

#39
 cis-1,3-Dichloropropene
 Concen: 0.803 ug/L
 RT: 10.036 min Scan# 11
 Delta R.T. -0.030 min
 Lab File: VW022525.D
 Acq: 13 Apr 2022 12:29

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFD3RE

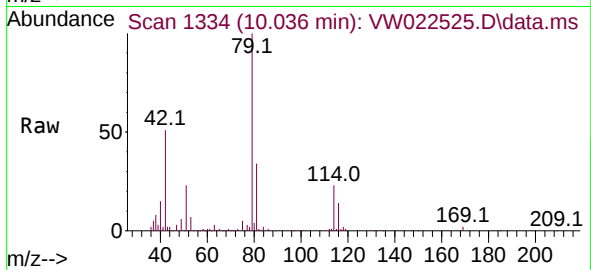

Tgt Ion: 75 Resp: 4394
 Ion Ratio Lower Upper
 75 100
 77 62.3 22.6 42.0#

