




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041322\
 Data File : VW022527.D
 Acq On : 13 Apr 2022 13:17
 Operator : SY/VA
 Sample : N2374-01RE
 Misc : 3.08g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFD4RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/14/2022
 Supervised By :Mahesh Dadoda 04/18/2022

Quant Time: Apr 14 01:32:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 14 01:27:44 2022
 Response via : Initial Calibration

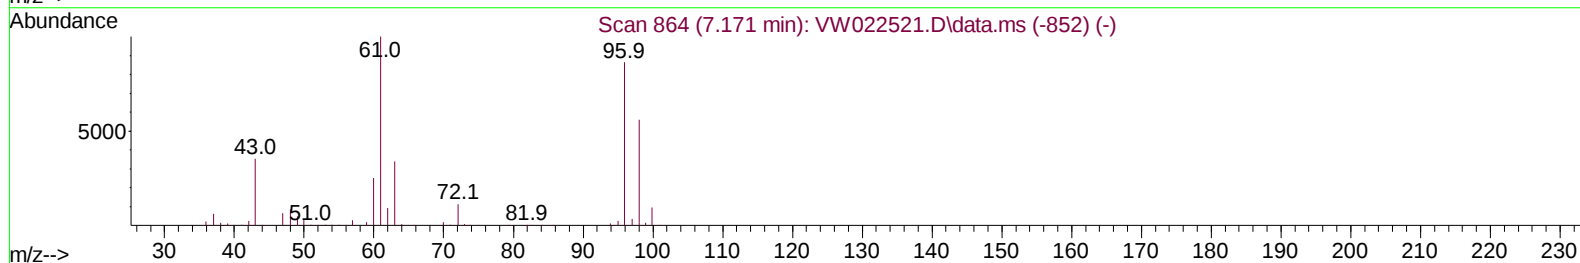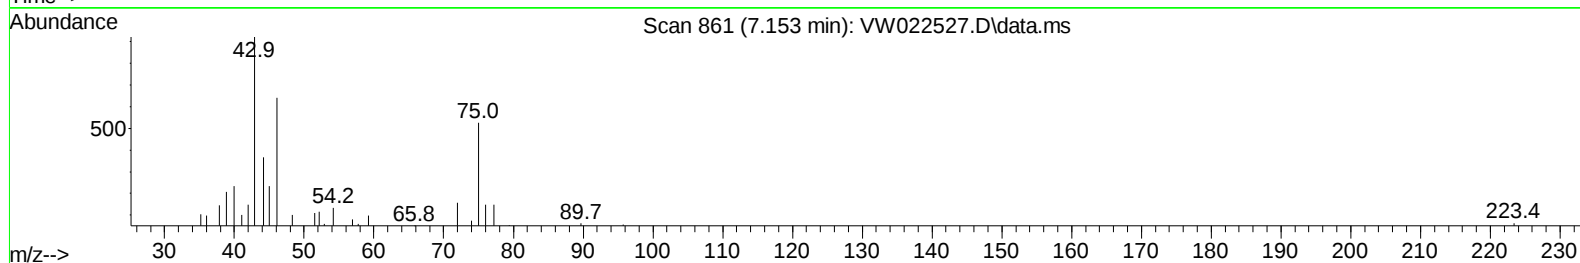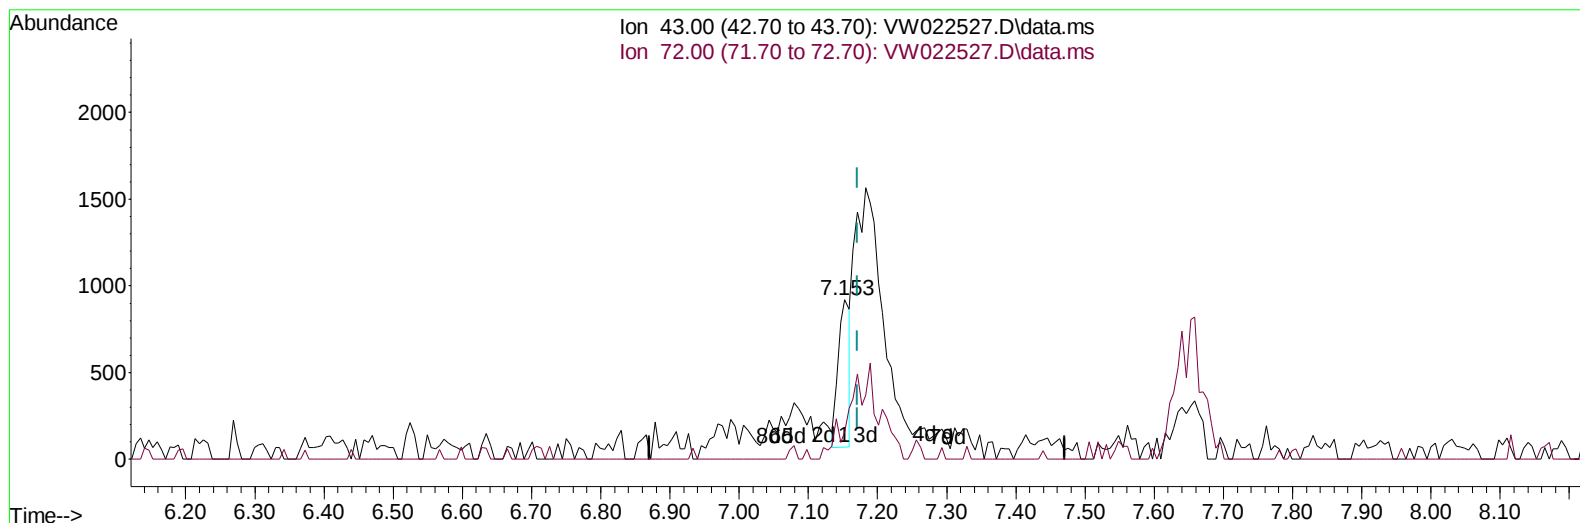

TIC: VW022527.D\data.ms

(22) 2-Butanone (T)

7.153min (-0.018) 0.85 ug/L

response 996

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	28.00	14.96
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041322\
 Data File : VW022527.D
 Acq On : 13 Apr 2022 13:17
 Operator : SY/VA
 Sample : N2374-01RE
 Misc : 3.08g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFD4RE

Manual IntegrationsAPPROVED

Quant Time: Apr 14 01:32:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 14 01:27:44 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/14/2022
 Supervised By :Mahesh Dadoda 04/18/2022

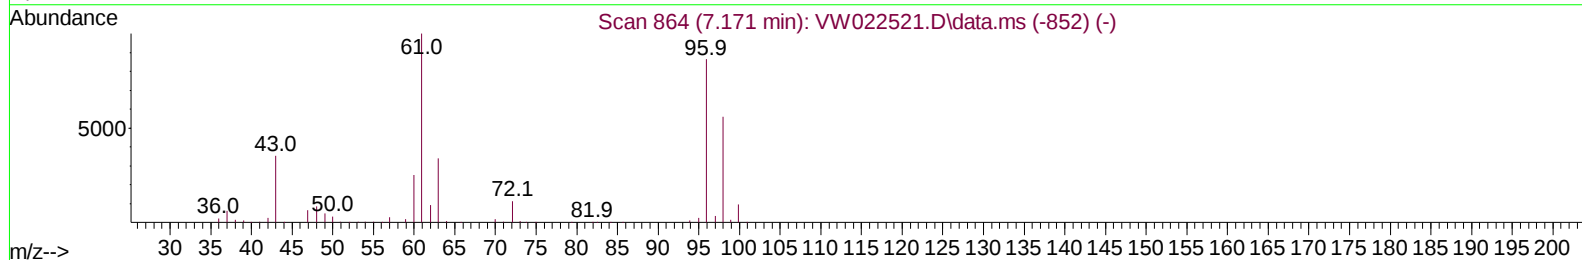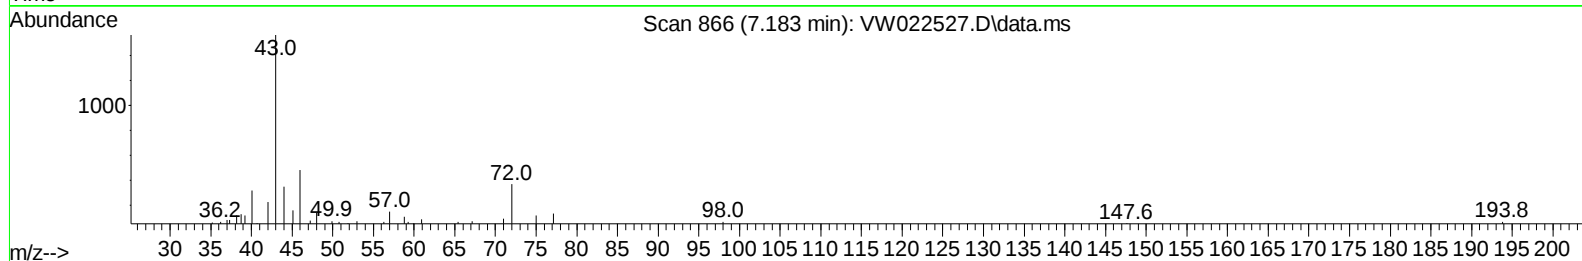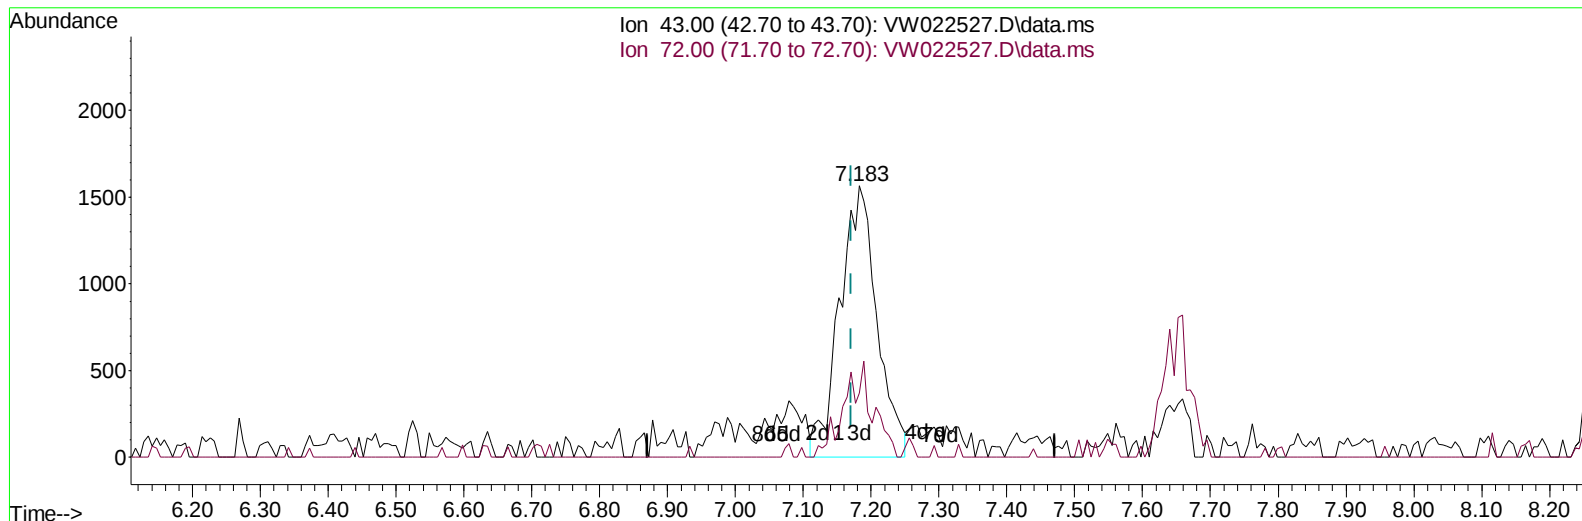

TIC: VW022527.D\data.ms

(22) 2-Butanone (T)

7.183min (+ 0.012) 5.08 ug/L m

response 5965

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	28.00	2.50#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041322\
 Data File : VW022527.D
 Acq On : 13 Apr 2022 13:17
 Operator : SY/VA
 Sample : N2374-01RE
 Misc : 3.08g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFD4RE

Manual IntegrationsAPPROVED

Quant Time: Apr 14 01:32:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 14 01:27:44 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/14/2022
 Supervised By :Mahesh Dadoda 04/18/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.841	114		296103	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117		232197	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		78604	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		116296	17.766	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	71.080%	
7) Chloroethane-d5	2.885	69		87820	21.407	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	85.640%	
11) 1,1-Dichloroethene-d2	4.013	63		118700	13.981	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	55.920%	
21) 2-Butanone-d5	7.073	46		81343	71.177	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	142.360%#	
24) Chloroform-d	7.646	84		220603	23.836	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	95.360%	
26) 1,2-Dichloroethane-d4	8.305	65		137499	26.002	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	104.000%	
32) Benzene-d6	8.274	84		395186	27.857	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	111.440%	
36) 1,2-Dichloropropane-d6	9.274	67		122709	29.890	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	119.560%	
41) Toluene-d8	10.323	98		312194	22.470	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	89.880%	
43) trans-1,3-Dichloroprop...	10.579	79		45381	23.422	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	93.680%	
47) 2-Hexanone-d5	10.926	63		63713	83.414	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	166.820%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		109681	31.421	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	125.680%#	
66) 1,2-Dichlorobenzene-d4	13.853	152		67539	24.258	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	97.040%	
Target Compounds							
13) Acetone	4.129	43		11886	15.275	ug/L	92
22) 2-Butanone	7.183	43		5965m	5.076	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041322\
Data File : VW022527.D
Acq On : 13 Apr 2022 13:17
Operator : SY/VA
Sample : N2374-01RE
Misc : 3.08g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFFD4RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/14/2022
Supervised By :Mahesh Dadoda 04/18/2022

Quant Time: Apr 14 01:32:37 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 14 01:27:44 2022
Response via : Initial Calibration

