




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041322\
 Data File : VW022530.D
 Acq On : 13 Apr 2022 14:35
 Operator : SY/VA
 Sample : N2373-07
 Misc : 5.65g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFD8

Manual IntegrationsAPPROVED

Quant Time: Apr 14 01:33:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 14 01:27:44 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/14/2022
 Supervised By :Mahesh Dadoda 04/18/2022

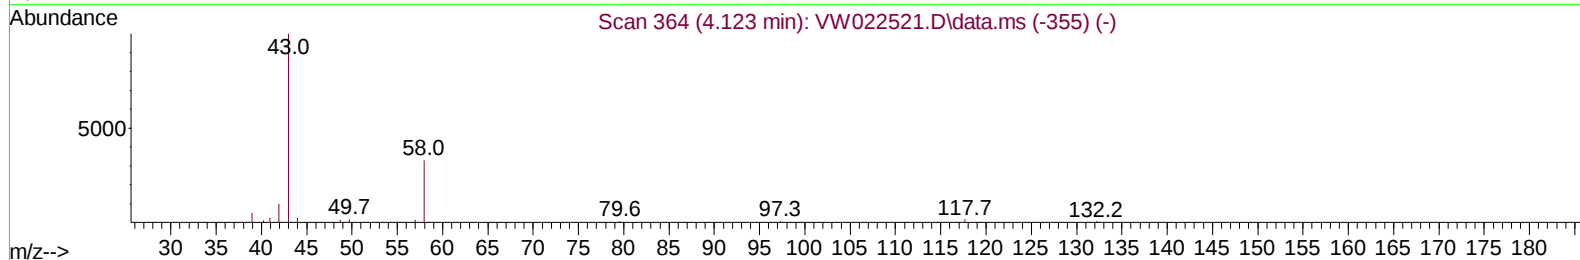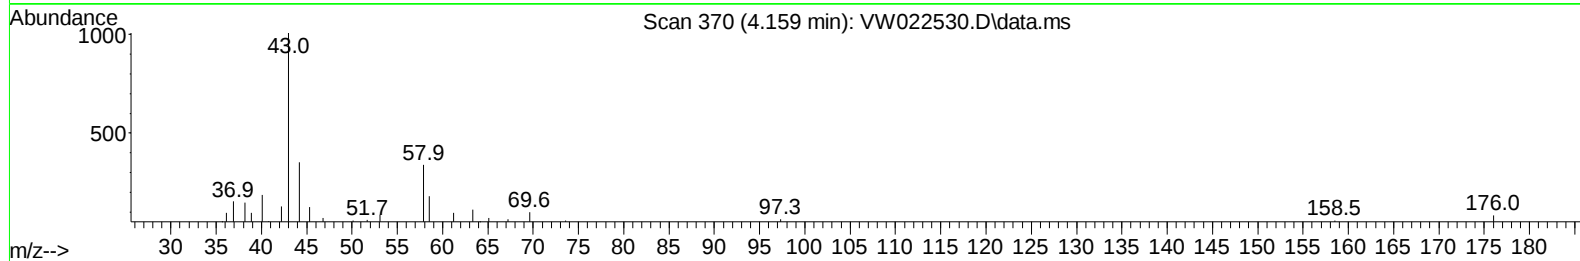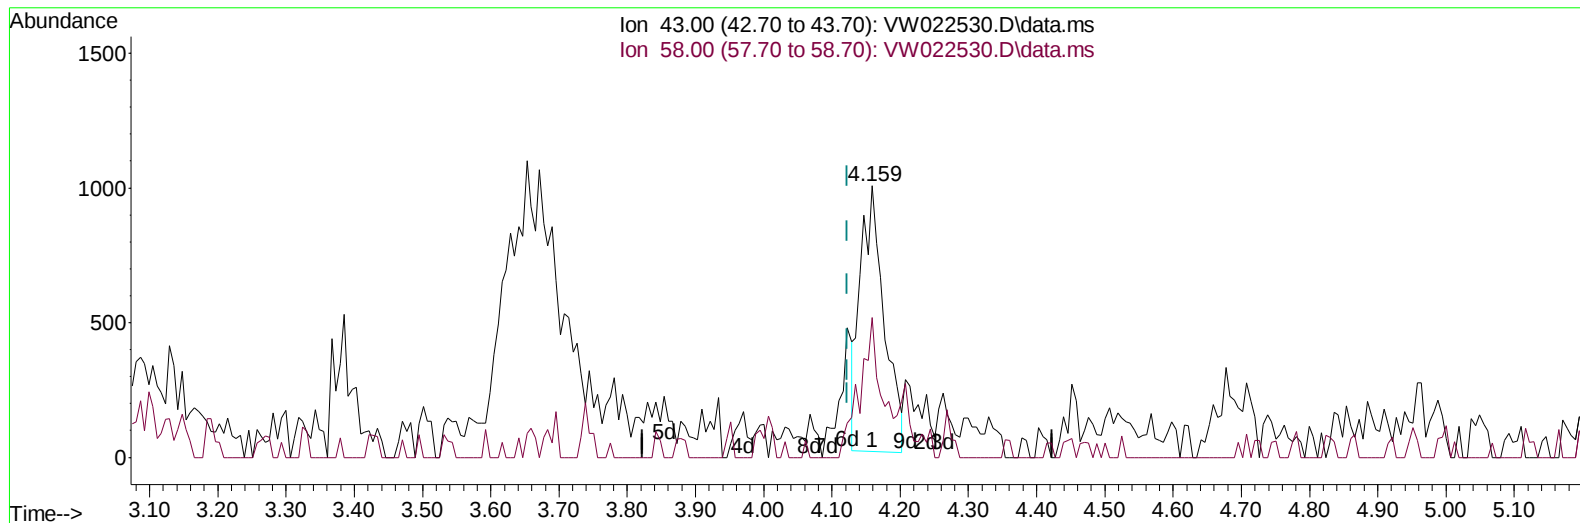

TIC: VW022530.D\data.ms

(13) Acetone (T)

4.159min (+ 0.037) 3.92 ug/L

response 2400

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	35.25
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041322\
 Data File : VW022530.D
 Acq On : 13 Apr 2022 14:35
 Operator : SY/VA
 Sample : N2373-07
 Misc : 5.65g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFD8

Manual IntegrationsAPPROVED

Quant Time: Apr 14 01:33:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 14 01:27:44 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/14/2022
 Supervised By :Mahesh Dadoda 04/18/2022

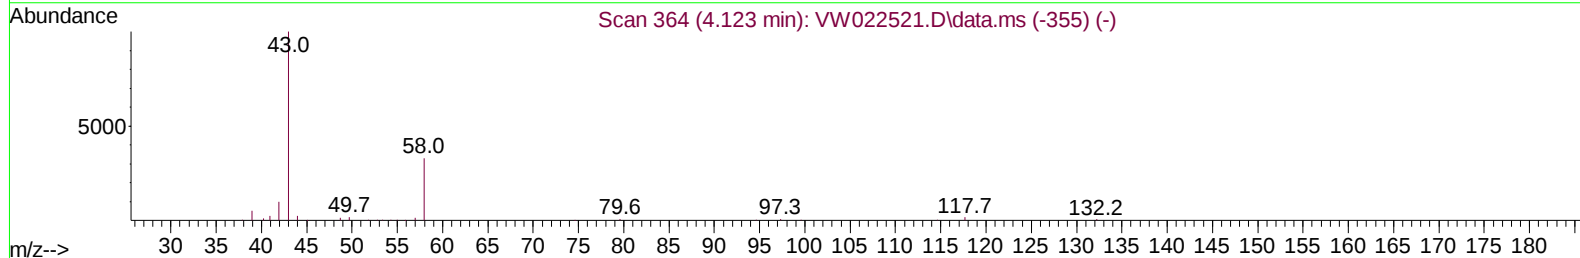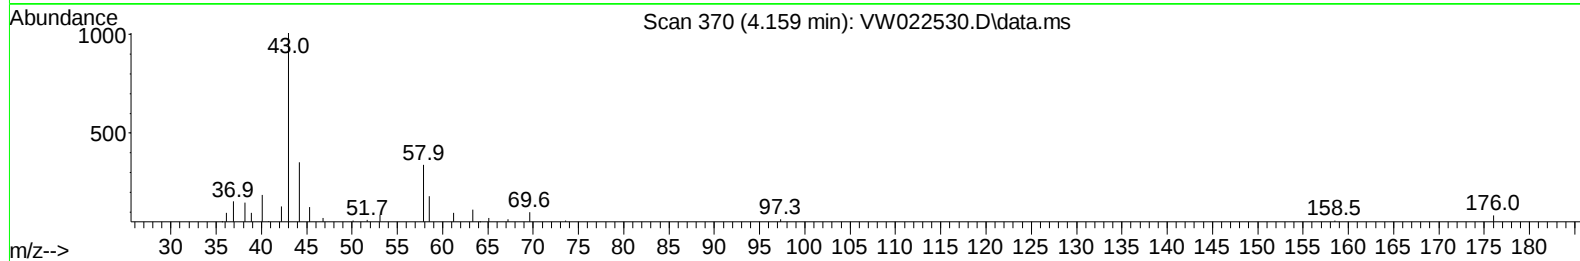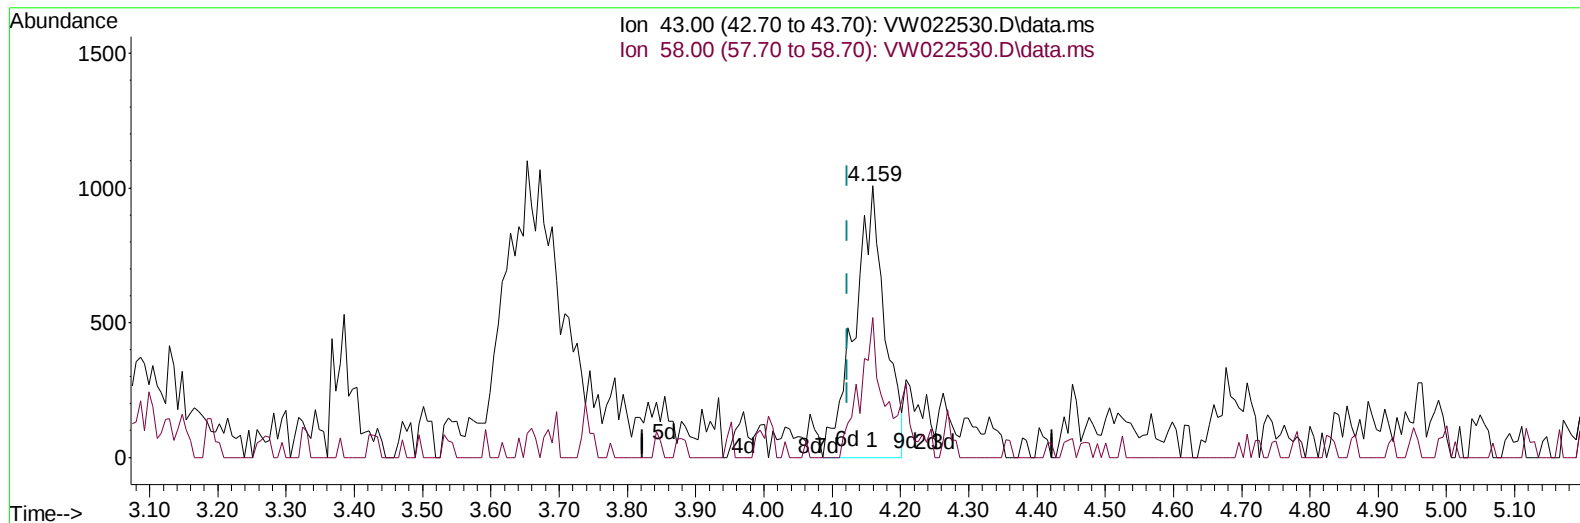

TIC: VW022530.D\data.ms

(13) Acetone (T)

4.159min (+ 0.037) 5.08 ug/L m

response 3114

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	27.17
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041322\
 Data File : VW022530.D
 Acq On : 13 Apr 2022 14:35
 Operator : SY/VA
 Sample : N2373-07
 Misc : 5.65g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFD8

Manual IntegrationsAPPROVED

Quant Time: Apr 14 01:33:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 14 01:27:44 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/14/2022
 Supervised By :Mahesh Dadoda 04/18/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	233171	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	163504	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	46439	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	100228	19.444	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery =	77.760%		
7) Chloroethane-d5	2.879	69	70313	21.765	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery =	87.040%		
11) 1,1-Dichloroethene-d2	4.013	63	90866	13.591	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery =	54.360%		
21) 2-Butanone-d5	7.086	46	43618	48.468	ug/L	0.01
Spiked Amount 50.000	Range 20	- 135	Recovery =	96.940%		
24) Chloroform-d	7.646	84	164841	22.618	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery =	90.480%		
26) 1,2-Dichloroethane-d4	8.305	65	100053	24.027	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery =	96.120%		
32) Benzene-d6	8.274	84	282814	28.311	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery =	113.240%		
36) 1,2-Dichloropropane-d6	9.274	67	90890	31.441	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery =	125.760%#		
41) Toluene-d8	10.323	98	215017	21.977	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery =	87.920%		
43) trans-1,3-Dichloroprop...	10.579	79	30960	22.693	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery =	90.760%		
47) 2-Hexanone-d5	10.926	63	35769	66.504	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery =	133.000%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	65617	26.695	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery =	106.760%		
66) 1,2-Dichlorobenzene-d4	13.853	152	37232	22.635	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery =	90.560%		
Target Compounds						
13) Acetone	4.159	43	3114m	5.082	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041322\
Data File : VW022530.D
Acq On : 13 Apr 2022 14:35
Operator : SY/VA
Sample : N2373-07
Misc : 5.65g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFFD8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/14/2022
Supervised By :Mahesh Dadoda 04/18/2022

Quant Time: Apr 14 01:33:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 14 01:27:44 2022
Response via : Initial Calibration

