




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041322\
 Data File : VW022533.D
 Acq On : 13 Apr 2022 15:48
 Operator : SY/VA
 Sample : N2373-07RE
 Misc : 4.97g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFD8RE

Manual IntegrationsAPPROVED

Quant Time: Apr 14 01:33:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 14 01:27:44 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/14/2022
 Supervised By :Mahesh Dadoda 04/18/2022

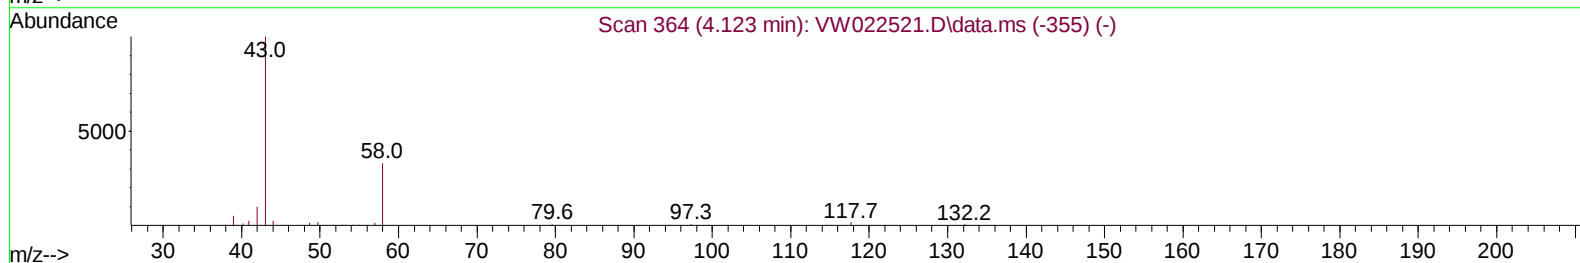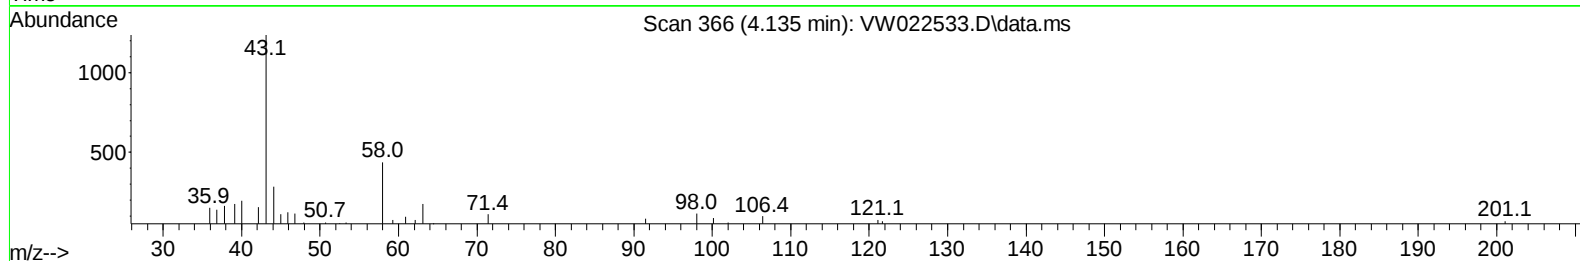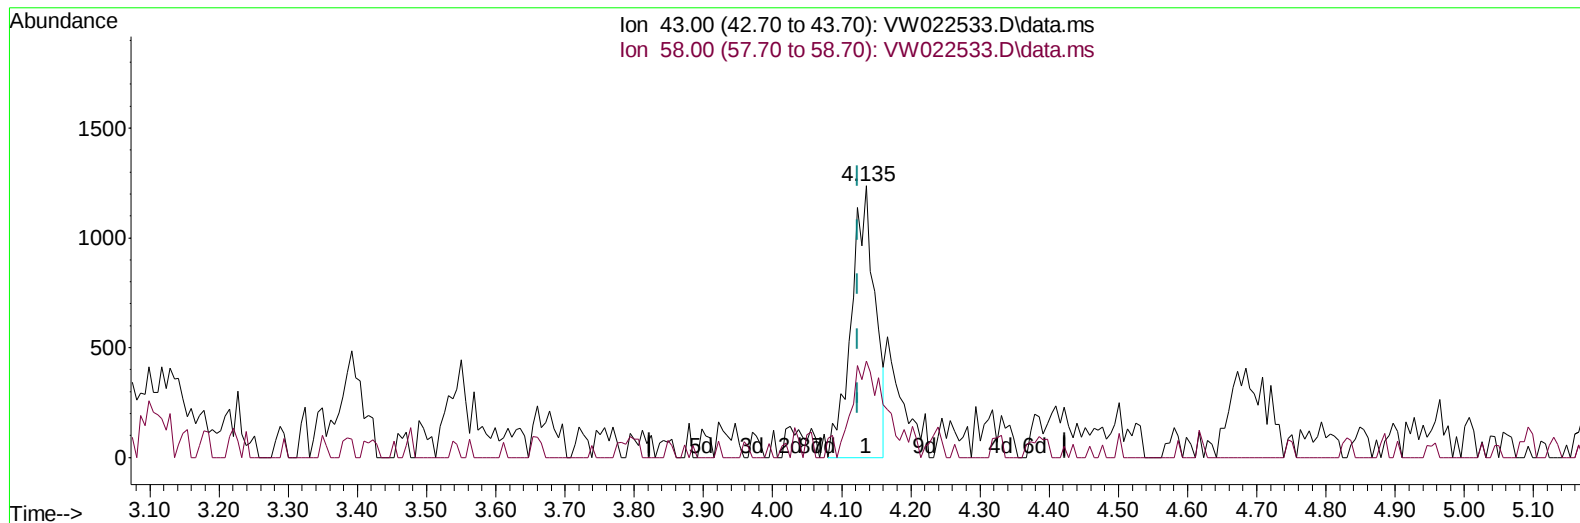

TIC: VW022533.D\data.ms

(13) Acetone (T)

4.135min (+ 0.013) 3.94 ug/L

response 2937

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	31.22
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041322\
 Data File : VW022533.D
 Acq On : 13 Apr 2022 15:48
 Operator : SY/VA
 Sample : N2373-07RE
 Misc : 4.97g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFD8RE

Manual IntegrationsAPPROVED

Quant Time: Apr 14 01:33:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 14 01:27:44 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/14/2022
 Supervised By :Mahesh Dadoda 04/18/2022

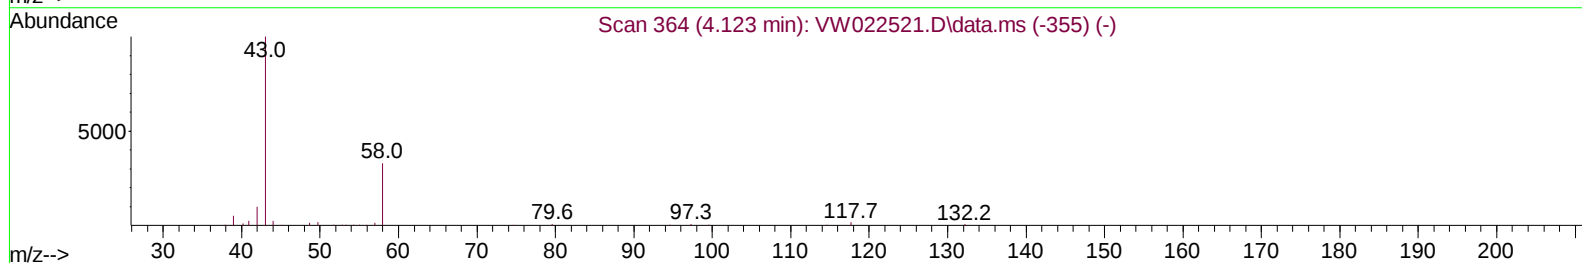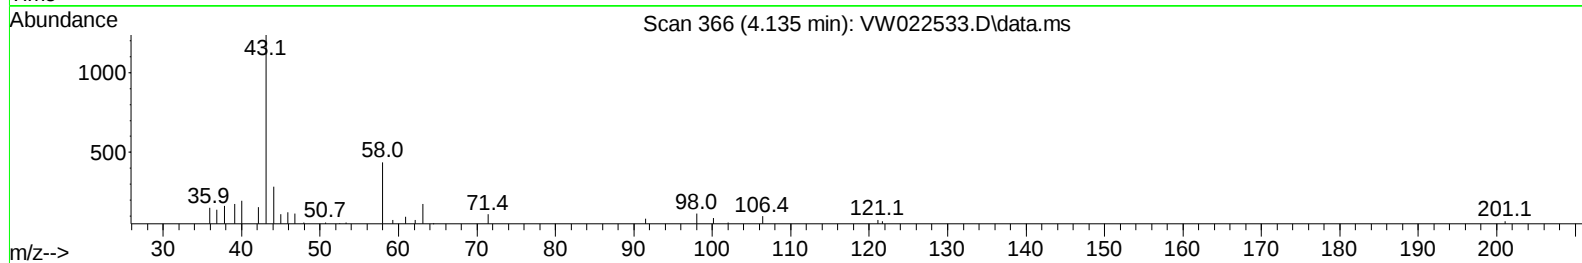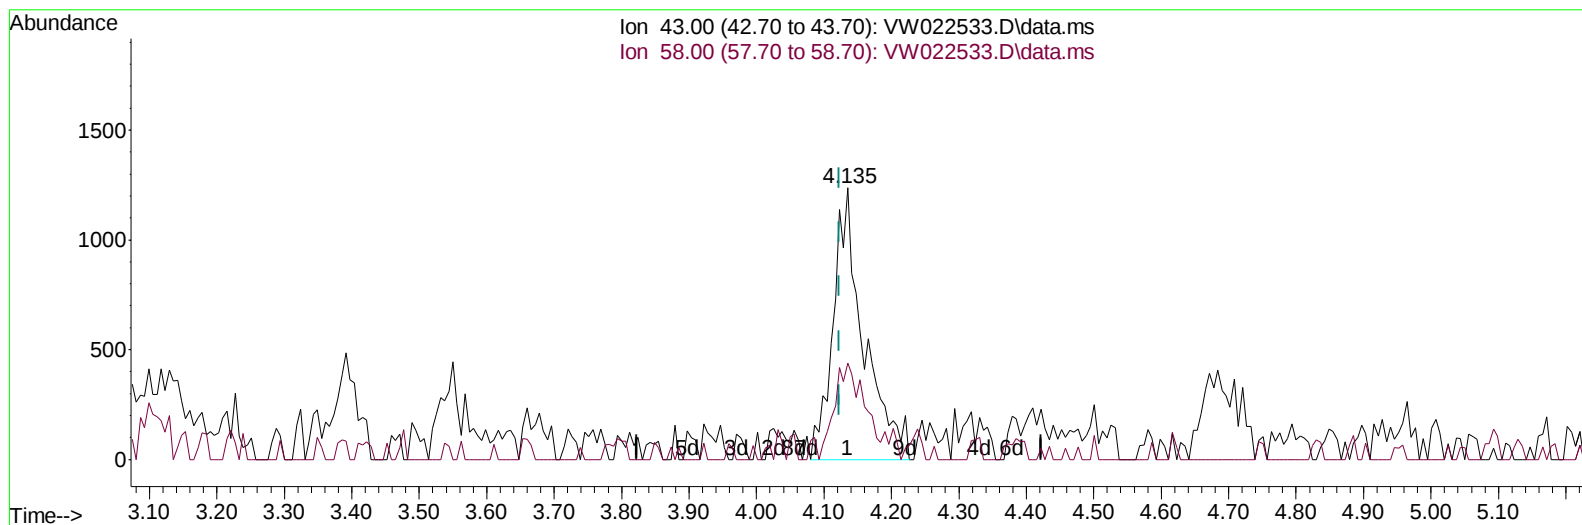

TIC: VW022533.D\data.ms

(13) Acetone (T)

4.135min (+ 0.013) 5.21 ug/L m

response 3890

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.50	23.57
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041322\
 Data File : VW022533.D
 Acq On : 13 Apr 2022 15:48
 Operator : SY/VA
 Sample : N2373-07RE
 Misc : 4.97g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFD8RE

Manual IntegrationsAPPROVED

Quant Time: Apr 14 01:33:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 14 01:27:44 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/14/2022
 Supervised By :Mahesh Dadoda 04/18/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	283947	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	231355	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	83327	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	108061	17.215	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	68.840%	
7) Chloroethane-d5	2.885	69	83034	21.106	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	84.440%	
11) 1,1-Dichloroethene-d2	4.019	63	109291	13.424	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	53.680%	
21) 2-Butanone-d5	7.080	46	71674	65.401	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	130.800%	
24) Chloroform-d	7.647	84	198750	22.394	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	89.560%	
26) 1,2-Dichloroethane-d4	8.305	65	125425	24.734	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	98.920%	
32) Benzene-d6	8.275	84	351433	24.863	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	99.440%	
36) 1,2-Dichloropropane-d6	9.275	67	109594	26.792	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	107.160%	
41) Toluene-d8	10.323	98	289755	20.931	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	83.720%	
43) trans-1,3-Dichloroprop...	10.579	79	42269	21.896	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	87.600%	
47) 2-Hexanone-d5	10.921	63	56964	74.850	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	149.700%#	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	105362	30.293	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	121.160%#	
66) 1,2-Dichlorobenzene-d4	13.853	152	70137	23.764	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	95.040%	
Target Compounds						
13) Acetone	4.135	43	3890m	5.213	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041322\
Data File : VW022533.D
Acq On : 13 Apr 2022 15:48
Operator : SY/VA
Sample : N2373-07RE
Misc : 4.97g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFFD8RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/14/2022
Supervised By :Mahesh Dadoda 04/18/2022

Quant Time: Apr 14 01:33:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 14 01:27:44 2022
Response via : Initial Calibration

