

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041322\
 Data File : VW022529.D
 Acq On : 13 Apr 2022 14:05
 Operator : SY/VA
 Sample : N2373-09
 Misc : 5.49g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFE2

Quant Time: Apr 14 01:32:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 14 01:27:44 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	368196	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	287263	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	92041	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	122158	15.008	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	60.040%
7) Chloroethane-d5	2.885	69	92431	18.119	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	72.480%
11) 1,1-Dichloroethene-d2	4.019	63	132027	12.506	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	50.040%
21) 2-Butanone-d5	7.080	46	63124	44.420	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	88.840%
24) Chloroform-d	7.647	84	238469	20.721	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	82.880%
26) 1,2-Dichloroethane-d4	8.305	65	142016	21.598	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	86.400%
32) Benzene-d6	8.275	84	422602	24.079	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	96.320%
36) 1,2-Dichloropropane-d6	9.274	67	133197	26.225	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	104.920%
41) Toluene-d8	10.323	98	366552	21.325	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.280%
43) trans-1,3-Dichloroprop...	10.579	79	44295	18.479	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	73.920%
47) 2-Hexanone-d5	10.926	63	47132	49.878	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.760%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	106093	24.567	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.280%
66) 1,2-Dichlorobenzene-d4	13.853	152	72186	22.142	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	88.560%
Target Compounds						
13) Acetone	4.129	43	3987	4.121	ug/L	Qvalue 83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041322\
Data File : VW022529.D
Acq On : 13 Apr 2022 14:05
Operator : SY/VA
Sample : N2373-09
Misc : 5.49g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFFE2

Quant Time: Apr 14 01:32:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 14 01:27:44 2022
Response via : Initial Calibration

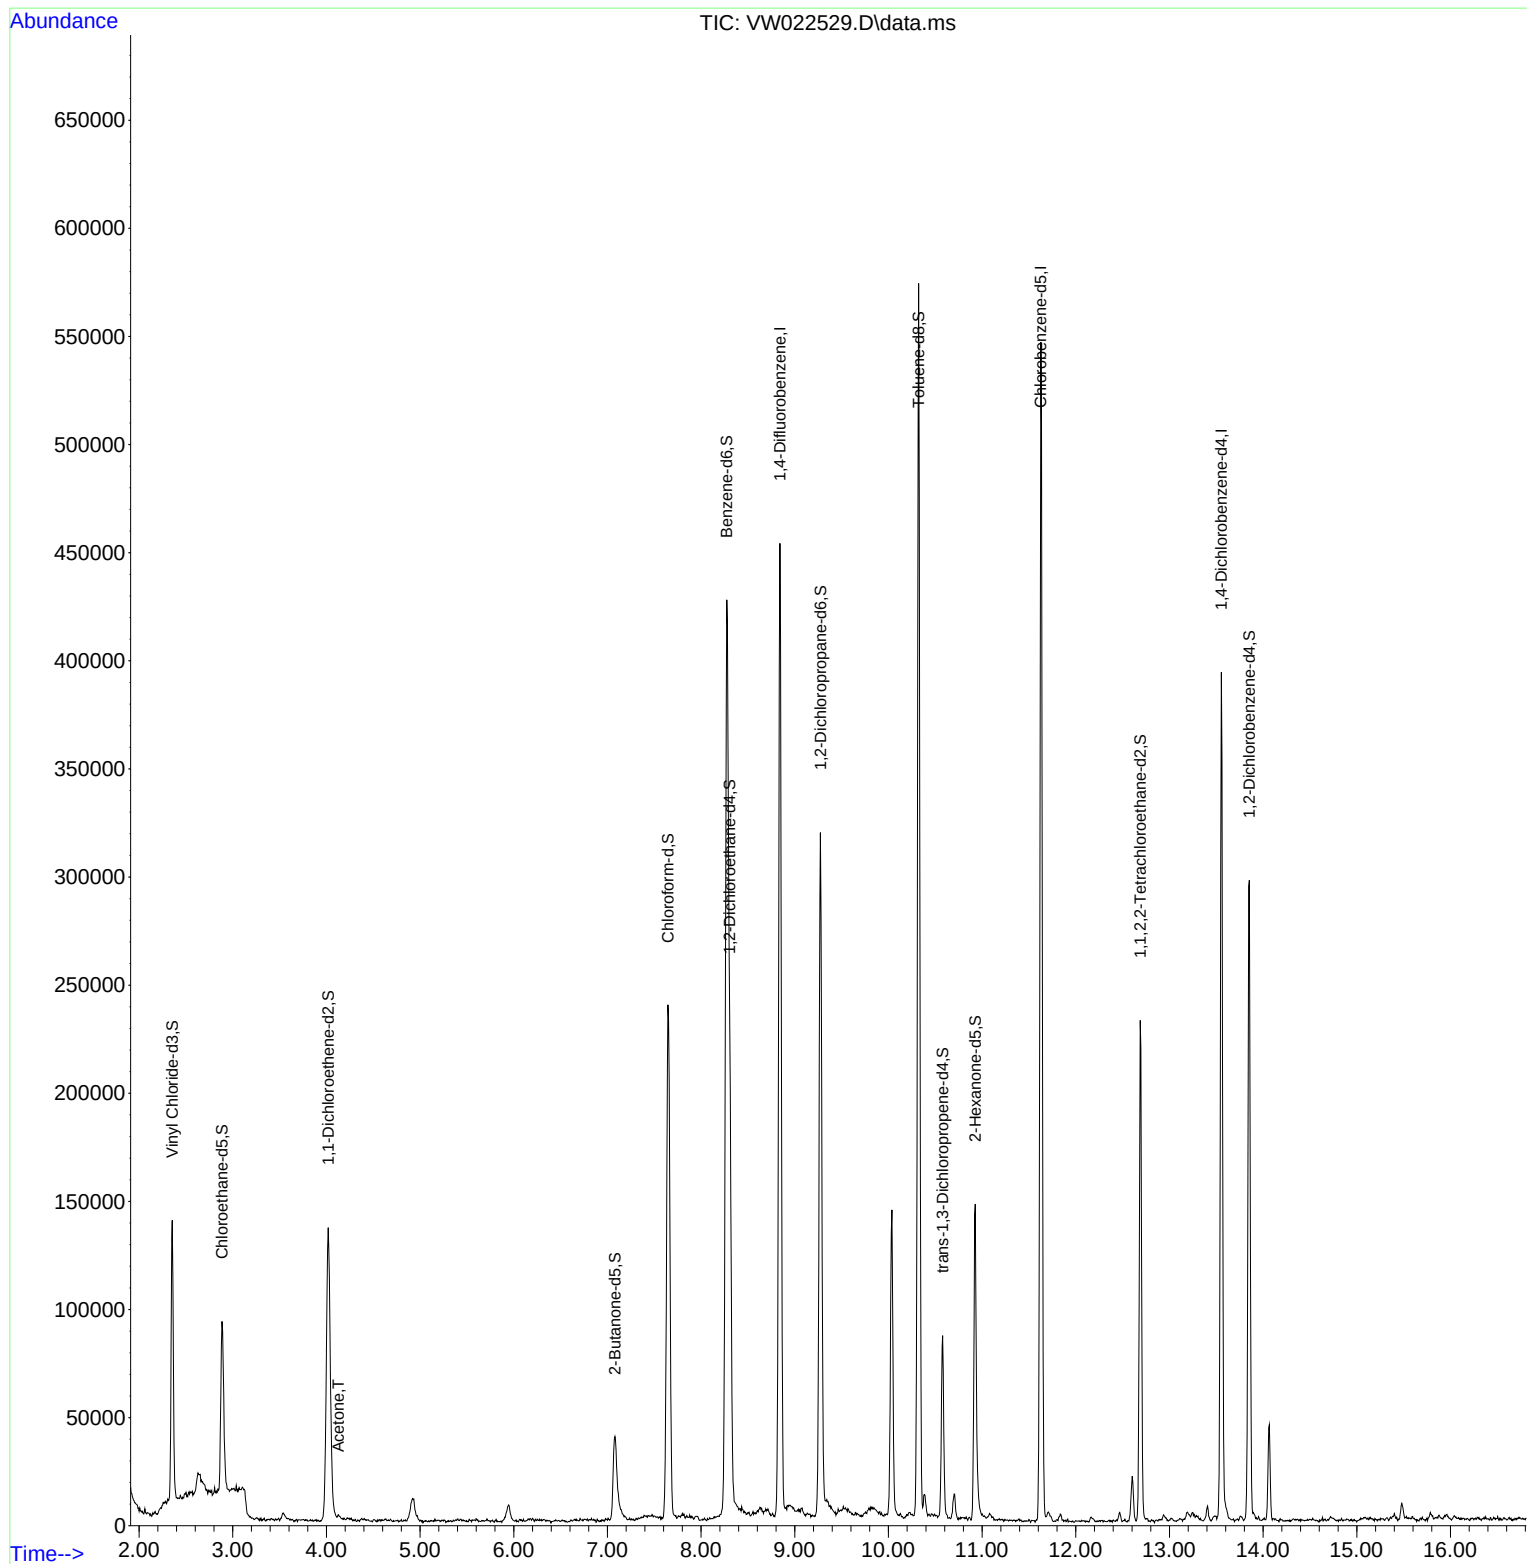

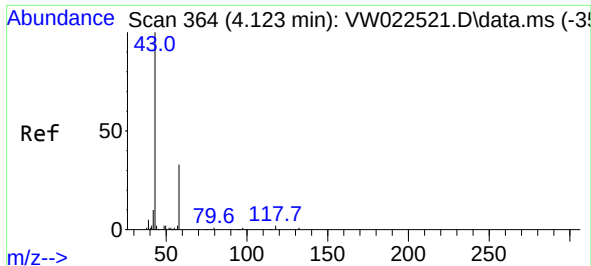

#13
 Acetone
 Concen: 4.121 ug/L
 RT: 4.129 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW022529.D
 Acq: 13 Apr 2022 14:05

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFE2

Tgt Ion: 43 Resp: 3987
 Ion Ratio Lower Upper
 43 100
 58 19.6 0.0 57.0

