

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041322\
 Data File : VW022530.D
 Acq On : 13 Apr 2022 14:35
 Operator : SY/VA
 Sample : N2373-07
 Misc : 5.65g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFD8

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/14/2022
 Supervised By :Mahesh Dadoda 04/18/2022

Quant Time: Apr 14 01:33:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 14 01:27:44 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	233171	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	163504	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	46439	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	100228	19.444	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.760%
7) Chloroethane-d5	2.879	69	70313	21.765	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.040%
11) 1,1-Dichloroethene-d2	4.013	63	90866	13.591	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	54.360%
21) 2-Butanone-d5	7.086	46	43618	48.468	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.940%
24) Chloroform-d	7.646	84	164841	22.618	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.480%
26) 1,2-Dichloroethane-d4	8.305	65	100053	24.027	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.120%
32) Benzene-d6	8.274	84	282814	28.311	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	113.240%
36) 1,2-Dichloropropane-d6	9.274	67	90890	31.441	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	125.760%#
41) Toluene-d8	10.323	98	215017	21.977	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.920%
43) trans-1,3-Dichloroprop...	10.579	79	30960	22.693	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	90.760%
47) 2-Hexanone-d5	10.926	63	35769	66.504	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	133.000%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	65617	26.695	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	106.760%
66) 1,2-Dichlorobenzene-d4	13.853	152	37232	22.635	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.560%
Target Compounds					Qvalue	
13) Acetone	4.159	43	3114m	5.082	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041322\
Data File : VW022530.D
Acq On : 13 Apr 2022 14:35
Operator : SY/VA
Sample : N2373-07
Misc : 5.65g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
BFFD8

Quant Time: Apr 14 01:33:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 14 01:27:44 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 04/14/2022
Supervised By :Mahesh Dadoda 04/18/2022

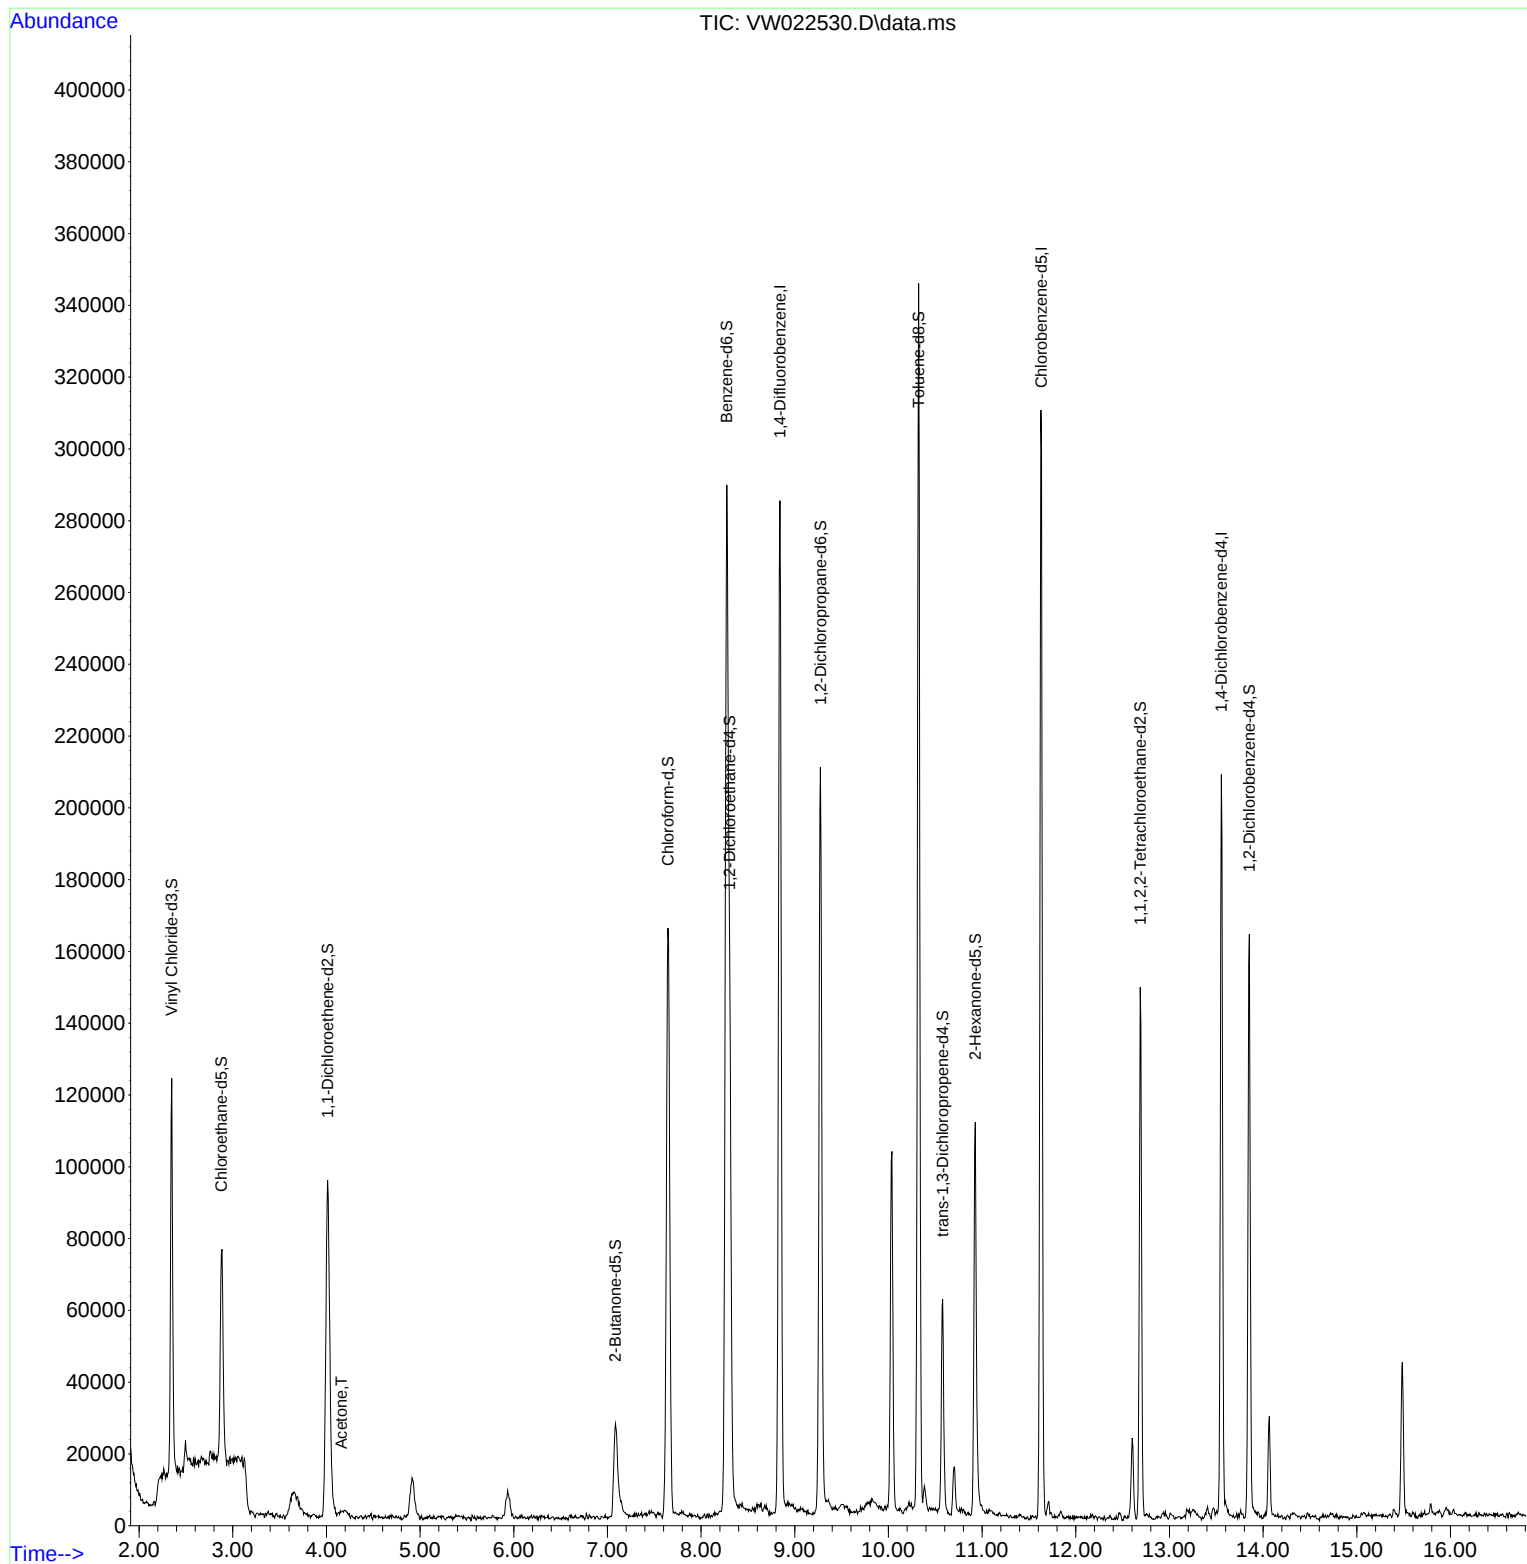

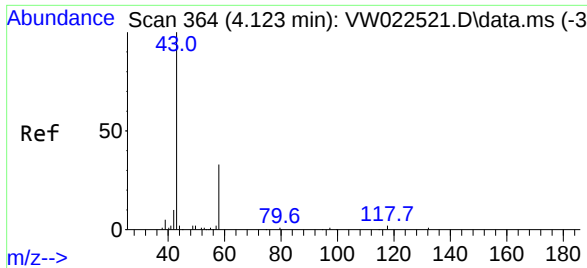

#13
 Acetone
 Concen: 5.082 ug/L m
 RT: 4.159 min Scan# 31
 Delta R.T. 0.037 min
 Lab File: VW022530.D
 Acq: 13 Apr 2022 14:35

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFD8

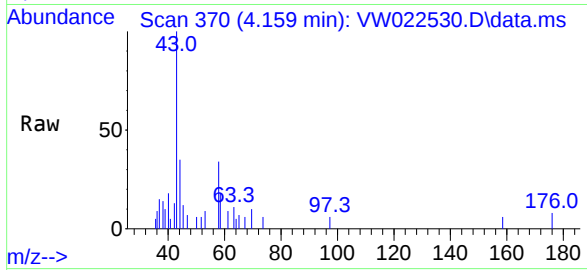

Tgt Ion: 43 Resp: 3114
 Ion Ratio Lower Upper
 43 100
 58 27.2 0.0 57.0

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/14/2022
 Supervised By :Mahesh Dadoda 04/18/2022

