

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041322\
 Data File : VW022533.D
 Acq On : 13 Apr 2022 15:48
 Operator : SY/VA
 Sample : N2373-07RE
 Misc : 4.97g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFFD8RE

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 04/14/2022
 Supervised By :Mahesh Dadoda 04/18/2022

Quant Time: Apr 14 01:33:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 14 01:27:44 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	283947	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	231355	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	83327	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	108061	17.215	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	68.840%
7) Chloroethane-d5	2.885	69	83034	21.106	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.440%
11) 1,1-Dichloroethene-d2	4.019	63	109291	13.424	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	53.680%
21) 2-Butanone-d5	7.080	46	71674	65.401	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	130.800%
24) Chloroform-d	7.647	84	198750	22.394	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.560%
26) 1,2-Dichloroethane-d4	8.305	65	125425	24.734	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.920%
32) Benzene-d6	8.275	84	351433	24.863	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	99.440%
36) 1,2-Dichloropropane-d6	9.275	67	109594	26.792	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	107.160%
41) Toluene-d8	10.323	98	289755	20.931	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	83.720%
43) trans-1,3-Dichloroprop...	10.579	79	42269	21.896	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.600%
47) 2-Hexanone-d5	10.921	63	56964	74.850	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	149.700%#
56) 1,1,2,2-Tetrachloroeth...	12.689	84	105362	30.293	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	121.160%#
66) 1,2-Dichlorobenzene-d4	13.853	152	70137	23.764	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.040%
Target Compounds					Qvalue	
13) Acetone	4.135	43	3890m	5.213	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041322\
Data File : VW022533.D
Acq On : 13 Apr 2022 15:48
Operator : SY/VA
Sample : N2373-07RE
Misc : 4.97g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
BFFD8RE

Quant Time: Apr 14 01:33:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 14 01:27:44 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 04/14/2022
Supervised By :Mahesh Dadoda 04/18/2022

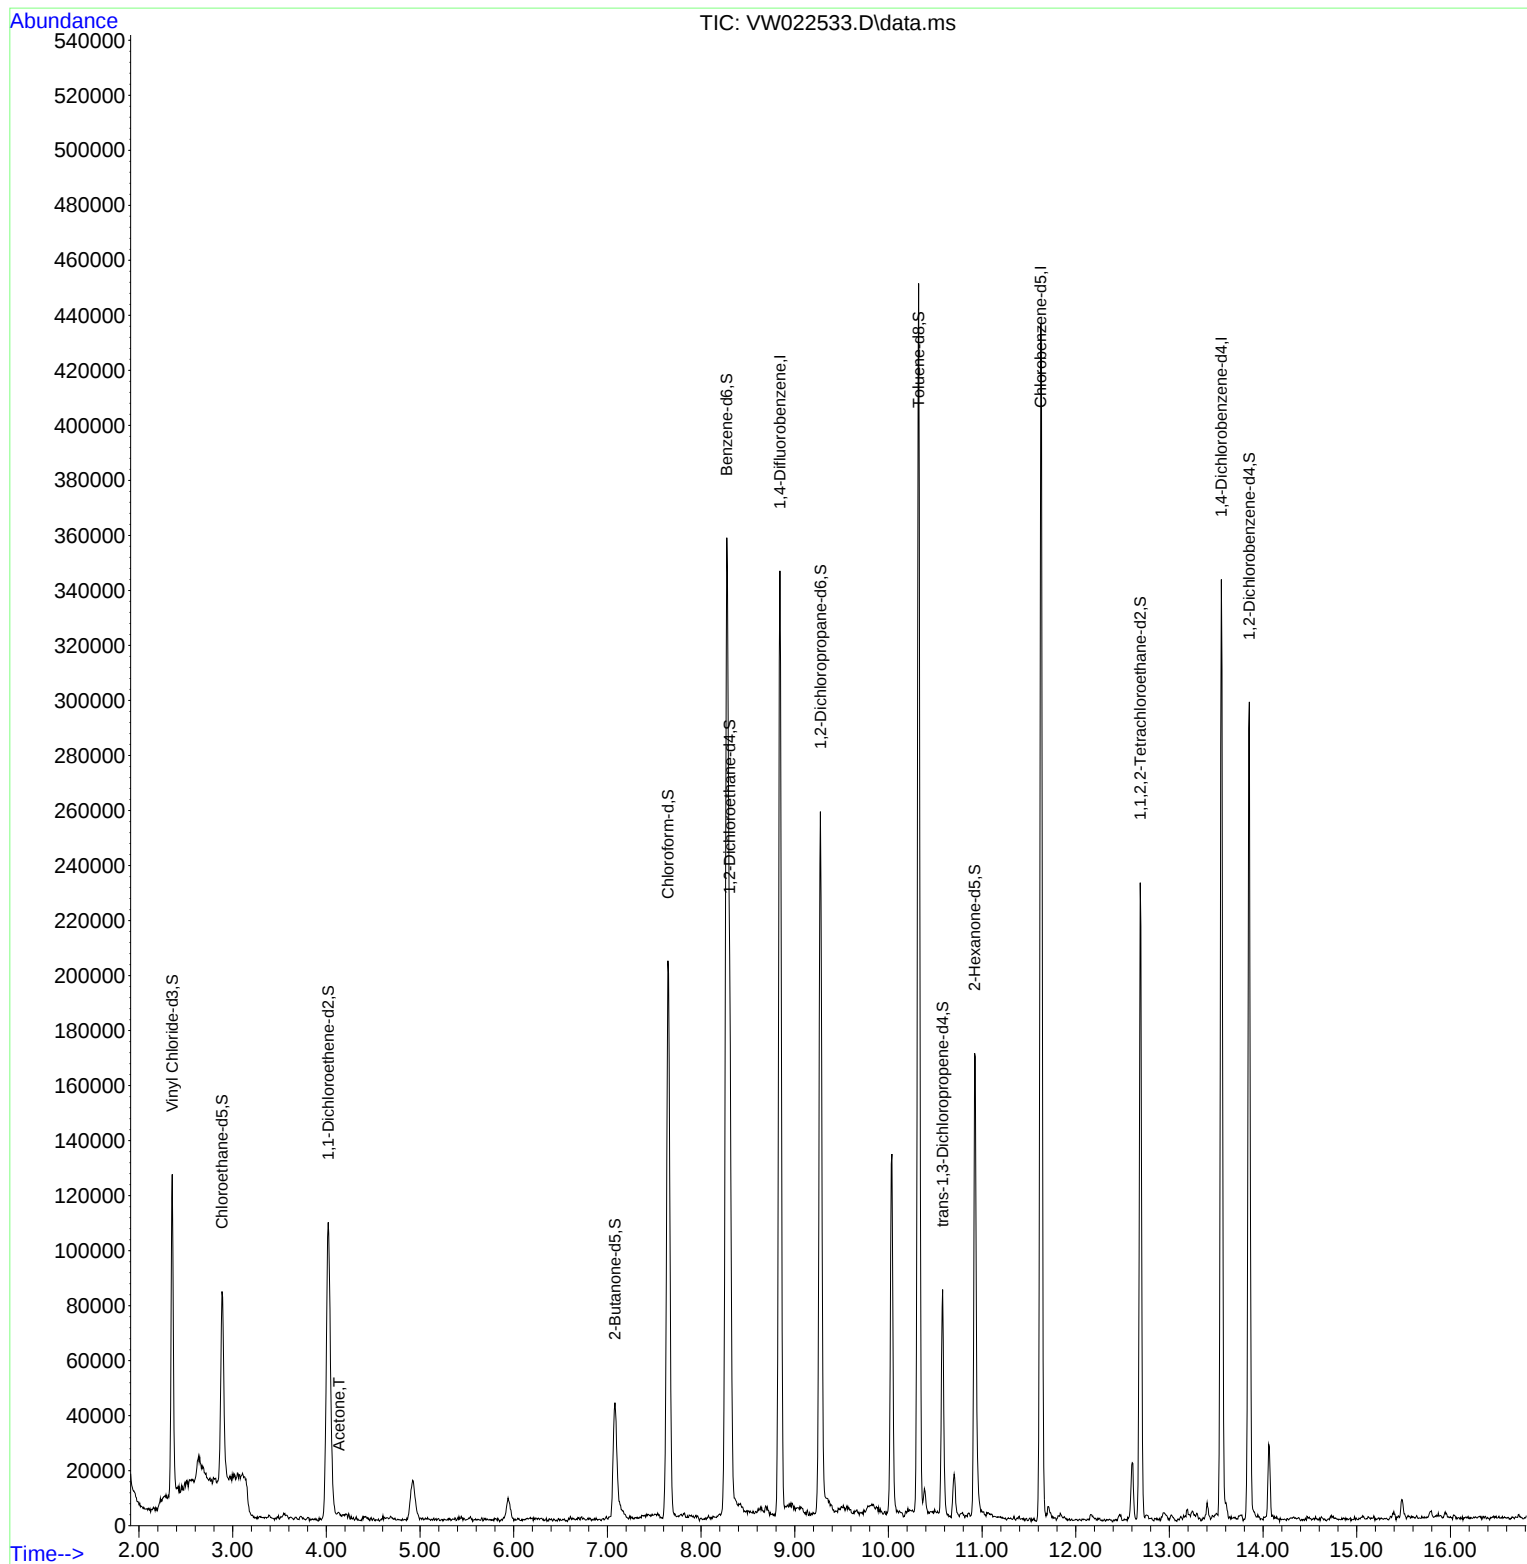

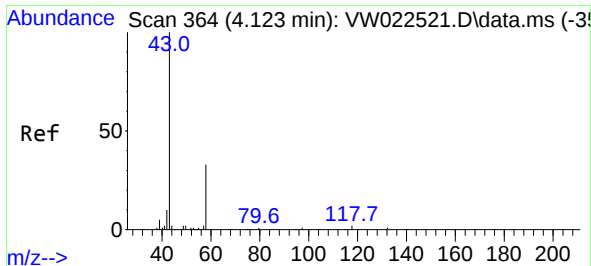

#13
Acetone
Concen: 5.213 ug/L m
RT: 4.135 min Scan# 30
Delta R.T. 0.013 min
Lab File: VW022533.D
Acq: 13 Apr 2022 15:48

Instrument :
MSVOA_W
ClientSampleId :
BFFD8RE

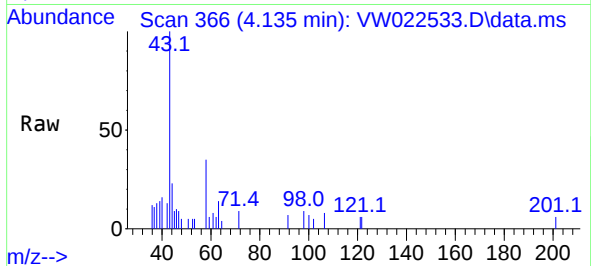

Tgt Ion: 43 Resp: 3890
Ion Ratio Lower Upper
43 100
58 23.6 0.0 57.0

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 04/14/2022
Supervised By :Mahesh Dadoda 04/18/2022

