


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041422\
 Data File : VW022540.D
 Acq On : 14 Apr 2022 09:03
 Operator : SY/VA
 Sample : BFB534
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB534

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Title : SFAM01.0
 Last Update : Fri Apr 15 23:17:23 2022

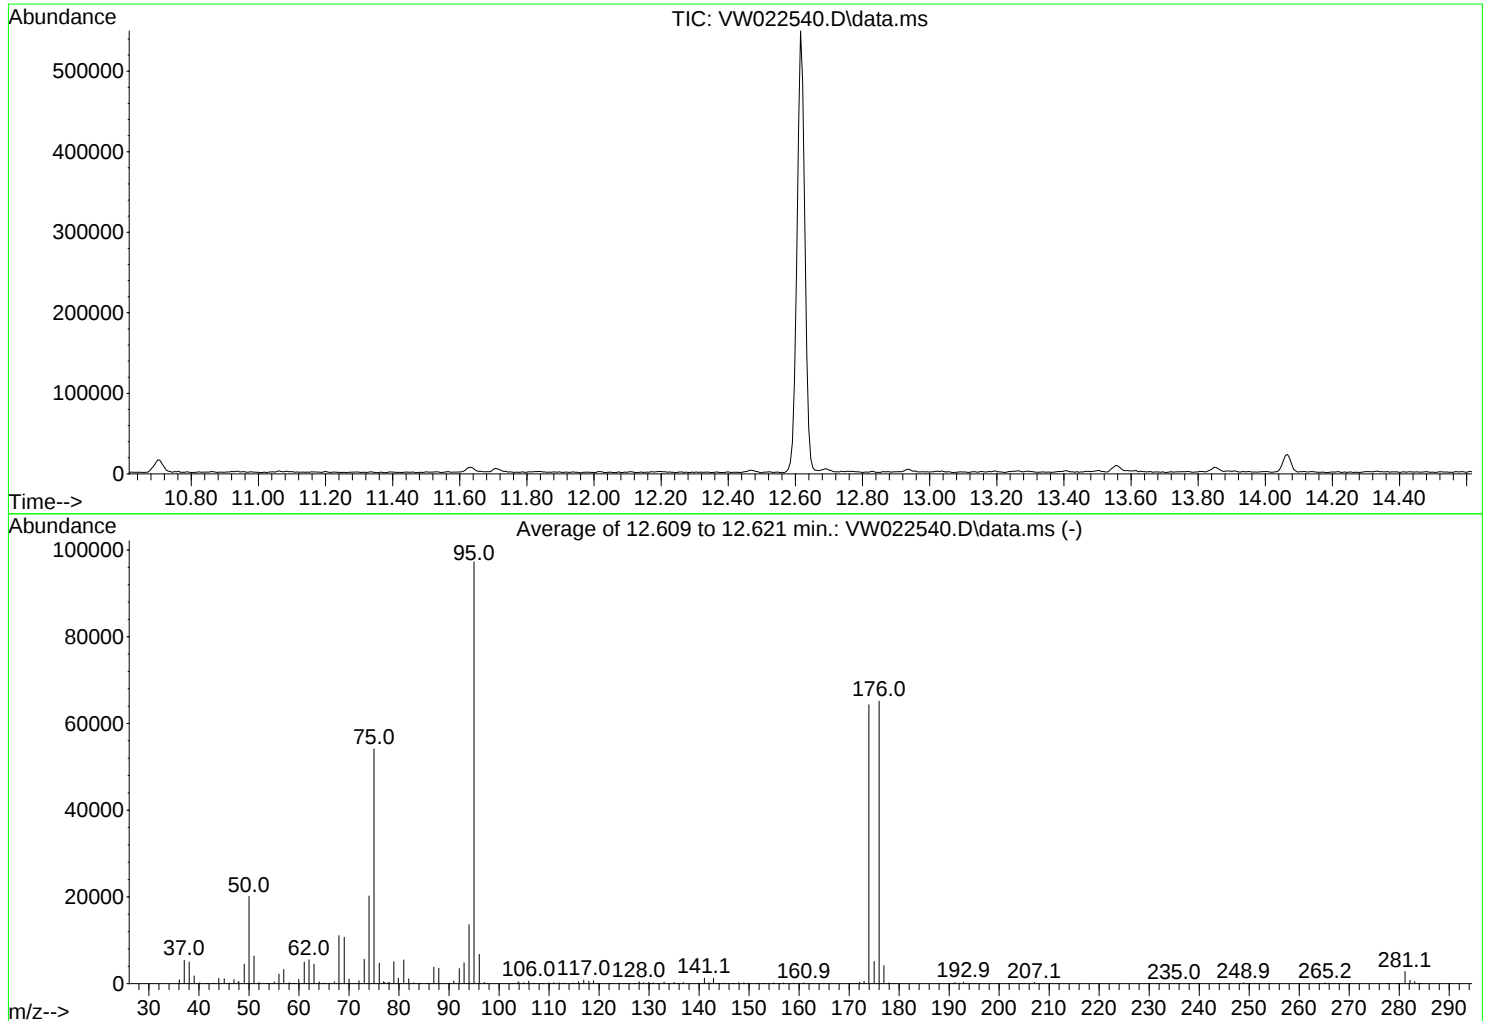

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	20099	PASS
75	95	30	80	55.6	54120	PASS
95	95	100	100	100.0	97272	PASS
96	95	5	9	6.9	6745	PASS
173	174	0.00	2	0.8	541	PASS
174	95	50	120	66.1	64301	PASS
175	174	5	9	8.0	5133	PASS
176	174	95	105	101.3	65125	PASS
177	176	5	10	6.4	4164	PASS

m/z	Abundance
36.40	65.0
37.10	52.0
38.60	101.0
39.20	97.0
40.00	201.0
40.80	172.0
42.00	94.0
43.90	204.0
50.20	77.0
51.50	81.0
56.90	100.0
57.50	58.0
69.40	51.0
74.20	52.0
78.60	57.0
116.70	60.0
162.00	58.0
178.70	57.0

Instrument :
MSVOA_W
ClientSampleId :
BFB534

m/z	Abundance
36.10	954.0
37.00	5113.0
38.10	4686.0
39.00	1570.0
39.90	135.0
41.50	99.0
43.00	122.0
44.00	1218.0
45.00	1034.0
45.80	263.0
47.00	856.0
47.80	789.0
49.10	3779.0
50.00	19144.0
51.00	6185.0
52.00	346.0
53.60	79.0
55.10	380.0
56.00	2209.0
57.00	3228.0
58.10	146.0
58.90	185.0
60.00	959.0
61.00	4265.0
62.00	5346.0
63.00	4180.0
64.10	356.0
64.90	207.0
65.40	84.0
66.10	62.0
67.10	466.0
68.00	10580.0
69.00	9797.0
70.00	1041.0
72.00	687.0
73.00	5347.0
74.00	18416.0
75.00	49344.0
76.00	3912.0
76.90	678.0
78.00	484.0
78.90	4196.0
79.90	1241.0
80.90	5181.0
82.00	845.0
82.90	200.0
84.10	55.0
86.00	156.0
87.00	3717.0
87.90	3985.0
90.10	157.0
91.00	582.0
92.10	3196.0
93.00	4145.0
94.00	11699.0
95.00	84592.0
96.00	5840.0
97.10	389.0
97.70	78.0
103.70	521.0
105.00	258.0
105.90	461.0
106.90	104.0
108.70	55.0
110.00	209.0
111.00	195.0
112.10	174.0
112.70	57.0
113.20	107.0
114.80	217.0
116.00	349.0
116.90	616.0
117.90	654.0
118.90	752.0
122.10	56.0
124.20	83.0
124.80	167.0
125.60	105.0
128.10	418.0
129.00	220.0
130.00	428.0
130.70	254.0
133.10	435.0
135.00	353.0
135.70	87.0
137.00	174.0
139.80	82.0
141.00	1271.0
142.00	155.0
142.90	1153.0
144.10	131.0
144.90	78.0

Instrument :
MSVOA_W
ClientSampleId :
BFB534

145.40	142.0
147.10	170.0
147.90	216.0
148.90	148.0
152.70	78.0
155.10	107.0
156.00	59.0
156.90	84.0
159.10	63.0
161.00	221.0
162.80	135.0
165.00	63.0
170.30	86.0
171.50	262.0
173.90	49000.0
175.00	4084.0
176.00	54600.0
177.00	3684.0
177.90	273.0
178.90	254.0
191.10	428.0
191.90	55.0
193.00	605.0
194.00	80.0
194.70	93.0
202.50	51.0
205.20	107.0
207.00	310.0
208.20	99.0
208.90	100.0
235.00	64.0
248.90	300.0
250.30	166.0
251.00	84.0
265.00	230.0
266.90	110.0
279.60	112.0
281.20	4133.0
282.10	1237.0
283.10	515.0
283.70	128.0
284.50	82.0

Instrument :
MSVOA_W
ClientSampleId :
BFB534

m/z	Abundance
36.00	844.0
37.10	5649.0
38.00	5371.0
39.10	2290.0
40.10	335.0
40.80	53.0
41.70	71.0
42.80	113.0
43.90	1531.0
45.10	1276.0
46.10	252.0
47.00	1074.0
48.00	854.0
49.00	5658.0
50.00	22272.0
51.00	6780.0
52.20	336.0
55.00	440.0
56.00	2448.0
57.00	3557.0
58.00	290.0
59.10	102.0
60.00	1023.0
61.10	6114.0
62.00	6193.0
63.00	4935.0
64.00	444.0
65.10	158.0
66.90	413.0
68.00	11890.0
69.10	11965.0
70.00	1281.0
72.00	674.0
73.00	6158.0
74.00	22952.0
75.00	60320.0
76.10	5517.0
77.10	770.0
77.70	298.0
78.90	5655.0
79.90	1396.0
81.00	6346.0
81.90	1143.0
82.90	173.0
85.70	249.0
86.90	4374.0
88.00	3800.0
90.80	583.0
92.00	4163.0
93.00	5648.0
94.00	15528.0
95.00	109624.0
96.10	8054.0
97.00	330.0
102.70	88.0
103.10	112.0
103.90	700.0
104.90	258.0
105.90	716.0
106.90	113.0
110.00	146.0
111.00	270.0
112.00	210.0
113.00	212.0
114.60	153.0
115.30	101.0
115.90	396.0
116.90	1018.0
118.00	599.0
118.90	740.0
124.00	72.0
125.20	123.0
128.00	427.0
128.90	221.0
129.90	523.0
130.90	245.0
132.90	486.0
135.00	288.0
136.80	331.0
139.70	86.0
141.00	1510.0
141.90	294.0
142.90	1251.0
143.80	154.0
145.00	174.0
145.80	110.0
146.90	95.0
148.00	242.0
149.00	203.0
149.80	158.0
151.80	155.0
152.90	138.0

Instrument :
MSVOA_W
ClientSampleId :
BFB534

154.00	105.0
154.80	260.0
156.00	93.0
156.90	201.0
158.90	139.0
160.90	200.0
170.30	97.0
171.00	165.0
172.10	500.0
174.00	75904.0
175.00	5994.0
176.00	70664.0
176.90	4555.0
178.00	153.0
190.80	185.0
191.20	217.0
192.00	138.0
192.80	502.0
194.10	66.0
194.80	52.0
202.60	63.0
204.60	52.0
205.10	84.0
207.10	386.0
208.10	96.0
208.90	97.0
248.80	157.0
251.00	157.0
265.20	338.0
266.00	75.0
279.60	167.0
281.10	3417.0
282.20	822.0
283.10	684.0
284.10	204.0

Instrument :
MSVOA_W
ClientSampleId :
BFB534

m/z	Abundance
36.00	849.0
37.00	5572.0
38.00	4858.0
39.00	1730.0
40.20	251.0
41.20	85.0
41.80	97.0
43.10	238.0
44.10	1529.0
45.00	966.0
46.20	152.0
47.00	854.0
47.90	728.0
49.00	4034.0
50.00	19112.0
51.00	6239.0
51.90	347.0
54.00	56.0
55.00	431.0
56.00	2003.0
57.00	3229.0
58.00	160.0
58.50	63.0
59.10	69.0
59.90	952.0
61.00	4606.0
62.00	4965.0
63.00	4434.0
64.10	272.0
64.90	115.0
67.10	411.0
68.00	10697.0
69.00	10276.0
70.00	903.0
71.10	97.0
72.00	677.0
73.10	5360.0
74.00	19512.0
75.00	52696.0
76.00	4712.0
76.90	564.0
77.80	426.0
78.10	423.0
79.00	5282.0
79.80	1254.0
81.00	4879.0
81.90	1332.0
83.00	141.0
86.00	69.0
86.90	3319.0
88.00	2814.0
89.10	73.0
91.00	729.0
92.00	3028.0
93.00	4614.0
94.00	13581.0
95.00	97600.0
96.10	6342.0
97.10	138.0
102.60	71.0
104.00	525.0
104.90	171.0
106.00	494.0
107.00	168.0
109.80	195.0
110.90	271.0
112.10	134.0
112.70	140.0
114.90	189.0
115.80	517.0
117.00	860.0
117.90	445.0
118.90	547.0
119.80	76.0
121.70	64.0
122.90	73.0
123.90	160.0
125.30	141.0
127.00	56.0
127.90	482.0
128.80	279.0
130.20	262.0
130.90	276.0
131.70	50.0
133.00	152.0
135.00	264.0
136.00	87.0
136.90	270.0
139.90	151.0
141.10	995.0
142.00	253.0
142.90	1318.0

Instrument :
MSVOA_W
ClientSampleId :
BFB534

143.90	128.0
144.90	141.0
146.00	146.0
146.80	55.0
147.80	259.0
148.90	164.0
149.90	134.0
151.80	135.0
152.50	60.0
153.10	80.0
153.90	56.0
154.90	254.0
156.00	65.0
156.90	212.0
159.00	146.0
160.90	246.0
169.30	75.0
170.60	176.0
171.10	121.0
172.10	401.0
173.00	1622.0
174.00	68000.0
175.00	5320.0
176.00	70112.0
177.00	4254.0
177.80	81.0
178.20	114.0
191.20	110.0
192.10	102.0
193.10	265.0
194.00	60.0
194.90	88.0
205.00	72.0
207.00	186.0
249.00	189.0
251.10	65.0
265.20	189.0
267.20	143.0
277.60	53.0
281.10	837.0
282.10	313.0
283.10	288.0
284.20	68.0

Instrument :
MSVOA_W
ClientSampleId :
BFB534