

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041522\
 Data File : VW022555.D
 Acq On : 15 Apr 2022 13:41
 Operator : SY/VA
 Sample : N2373-11
 Misc : 5.55g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Apr 15 23:18:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 15 23:17:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	293089	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.633	117	223032	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	68935	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	100737	15.547	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	62.200%
7) Chloroethane-d5	2.891	69	73370	18.068	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	72.280%
11) 1,1-Dichloroethene-d2	4.019	63	103614	12.329	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	49.320%
21) 2-Butanone-d5	7.079	46	70098	61.968	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	123.940%
24) Chloroform-d	7.652	84	206065	22.494	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.960%
26) 1,2-Dichloroethane-d4	8.305	65	122675	23.437	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	93.760%
32) Benzene-d6	8.280	84	340176	24.965	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	99.840%
36) 1,2-Dichloropropane-d6	9.274	67	113690	28.831	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	115.320%
41) Toluene-d8	10.323	98	275496	20.643	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	82.560%
43) trans-1,3-Dichloroprop...	10.579	79	35323	18.980	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	75.920%
47) 2-Hexanone-d5	10.920	63	45003	61.340	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	122.680%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	100458	29.961	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	119.840%
66) 1,2-Dichlorobenzene-d4	13.852	152	57243	23.444	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.760%
Target Compounds					Qvalue	
13) Acetone	4.129	43	3836	4.981	ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041522\
Data File : VW022555.D
Acq On : 15 Apr 2022 13:41
Operator : SY/VA
Sample : N2373-11
Misc : 5.55g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Apr 15 23:18:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 15 23:17:23 2022
Response via : Initial Calibration

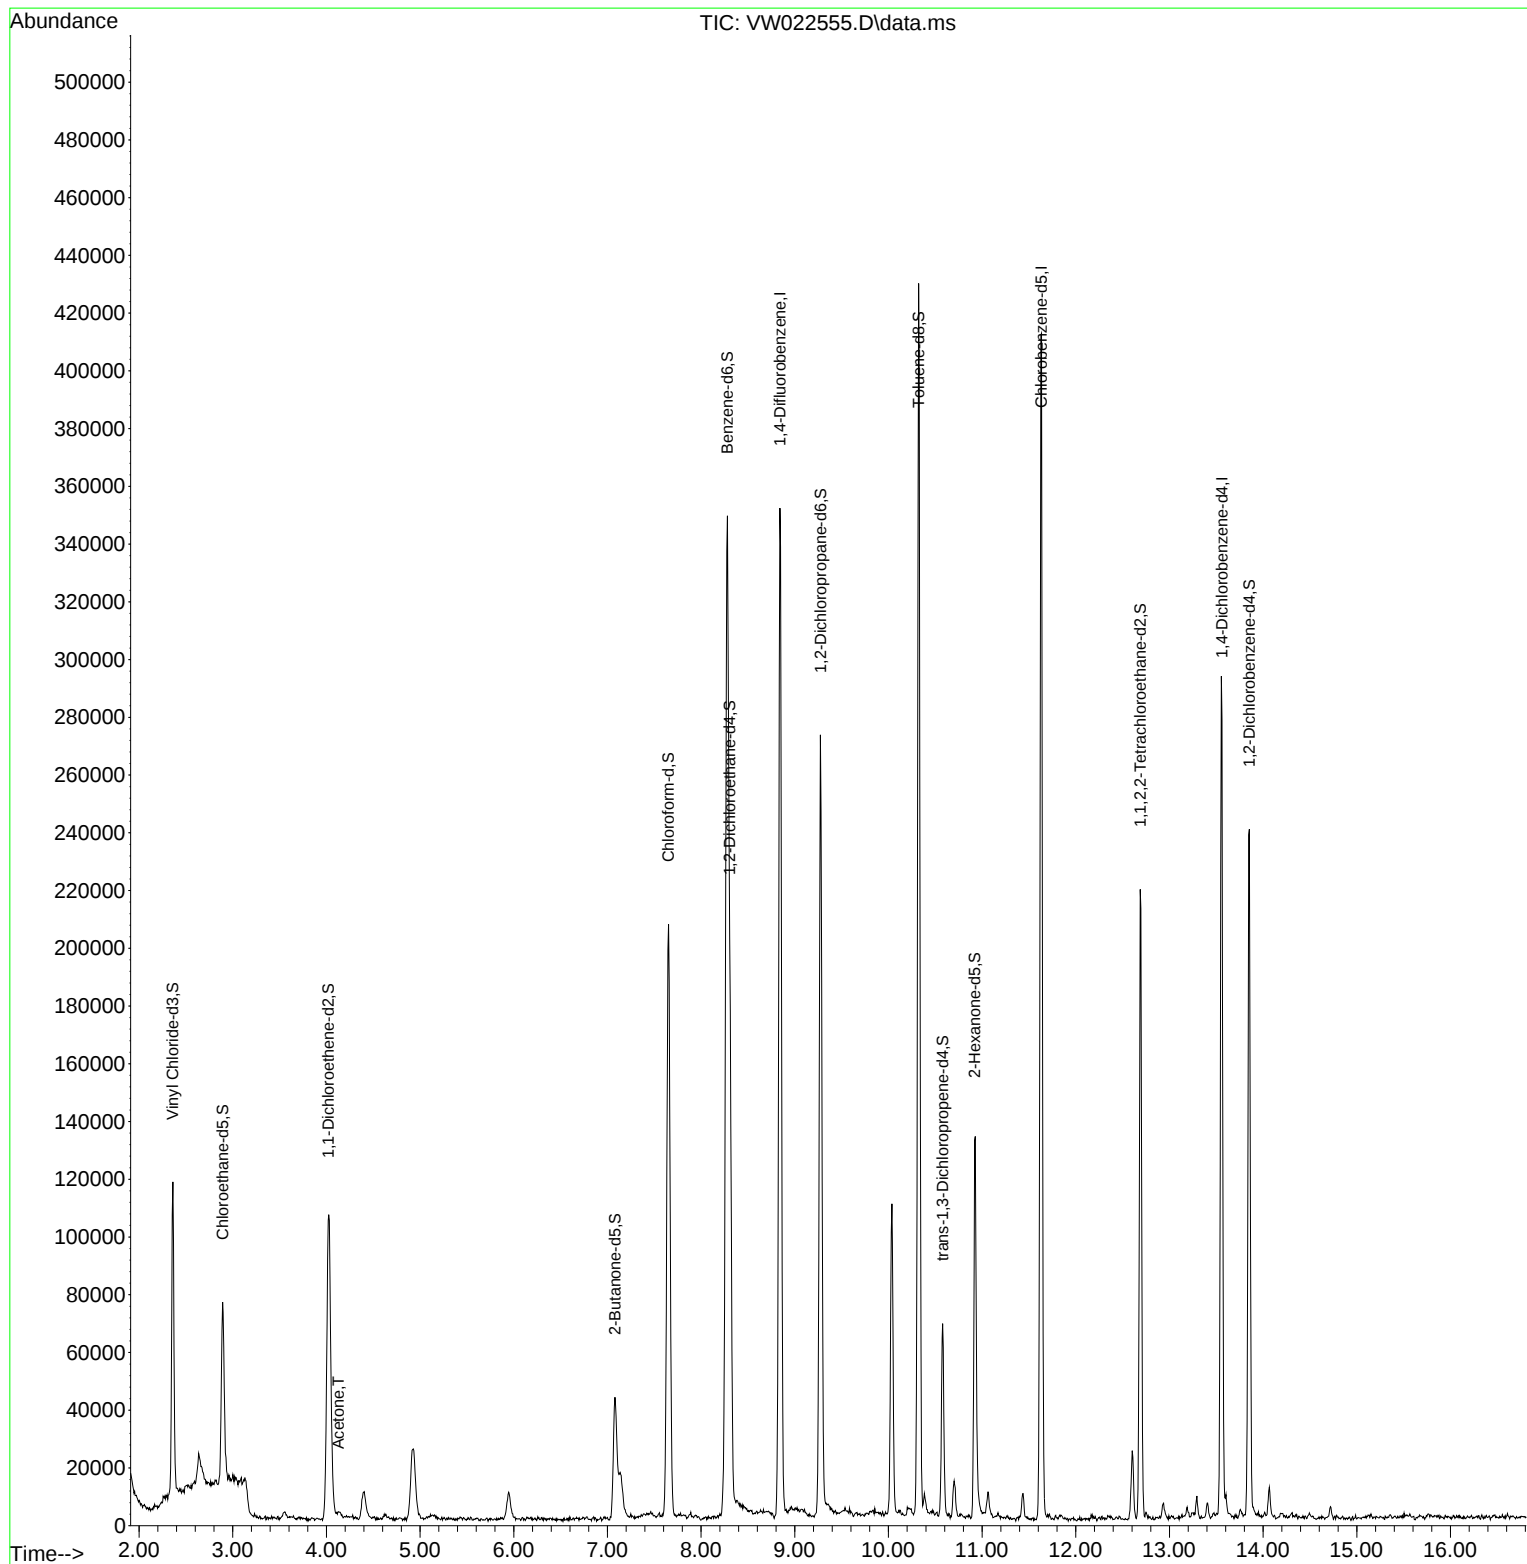

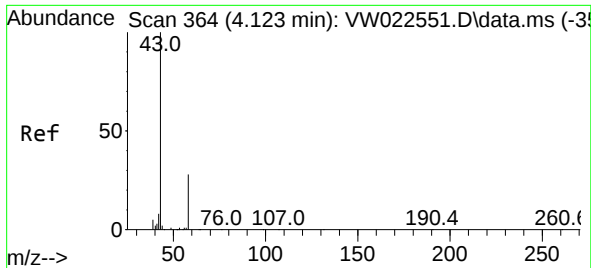

#13

Acetone

Concen: 4.981 ug/L

RT: 4.129 min Scan# 30

Delta R.T. 0.006 min


Lab File: VW022555.D

Acq: 15 Apr 2022 13:41

Instrument :

MSVOA_W

ClientSampleId :

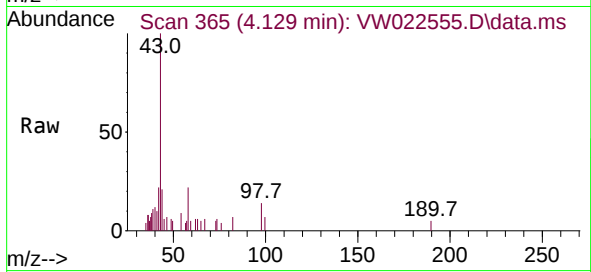

Tgt Ion: 43 Resp: 3836

Ion Ratio Lower Upper

43 100

58 21.4 0.0 57.0

