

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041522\
 Data File : VW022557.D
 Acq On : 15 Apr 2022 14:38
 Operator : SY/VA
 Sample : N2373-11RE
 Misc : 5.58g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Apr 15 23:18:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 15 23:17:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	257390	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	215962	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	80035	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	84402	14.833	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	59.320%
7) Chloroethane-d5	2.885	69	63406	17.780	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.120%
11) 1,1-Dichloroethene-d2	4.013	63	84625	11.466	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	45.880%
21) 2-Butanone-d5	7.080	46	53163	53.515	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	107.040%
24) Chloroform-d	7.647	84	160459	19.945	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	79.760%
26) 1,2-Dichloroethane-d4	8.397	65	168	0.037	ug/L	0.09
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.160%#
32) Benzene-d6	8.275	84	275317	20.866	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	83.480%
36) 1,2-Dichloropropane-d6	9.274	67	89217	23.365	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.480%
41) Toluene-d8	10.323	98	223845	17.322	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	69.280%
43) trans-1,3-Dichloroprop...	10.579	79	32465	18.016	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	72.080%
47) 2-Hexanone-d5	10.921	63	39924	56.199	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	112.400%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	82905	25.535	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	102.160%
66) 1,2-Dichlorobenzene-d4	13.853	152	56758	20.022	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	80.080%
Target Compounds						
39) cis-1,3-Dichloropropene	10.037	75	3630	0.651	ug/L	Qvalue 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041522\
Data File : VW022557.D
Acq On : 15 Apr 2022 14:38
Operator : SY/VA
Sample : N2373-11RE
Misc : 5.58g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Apr 15 23:18:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 15 23:17:23 2022
Response via : Initial Calibration

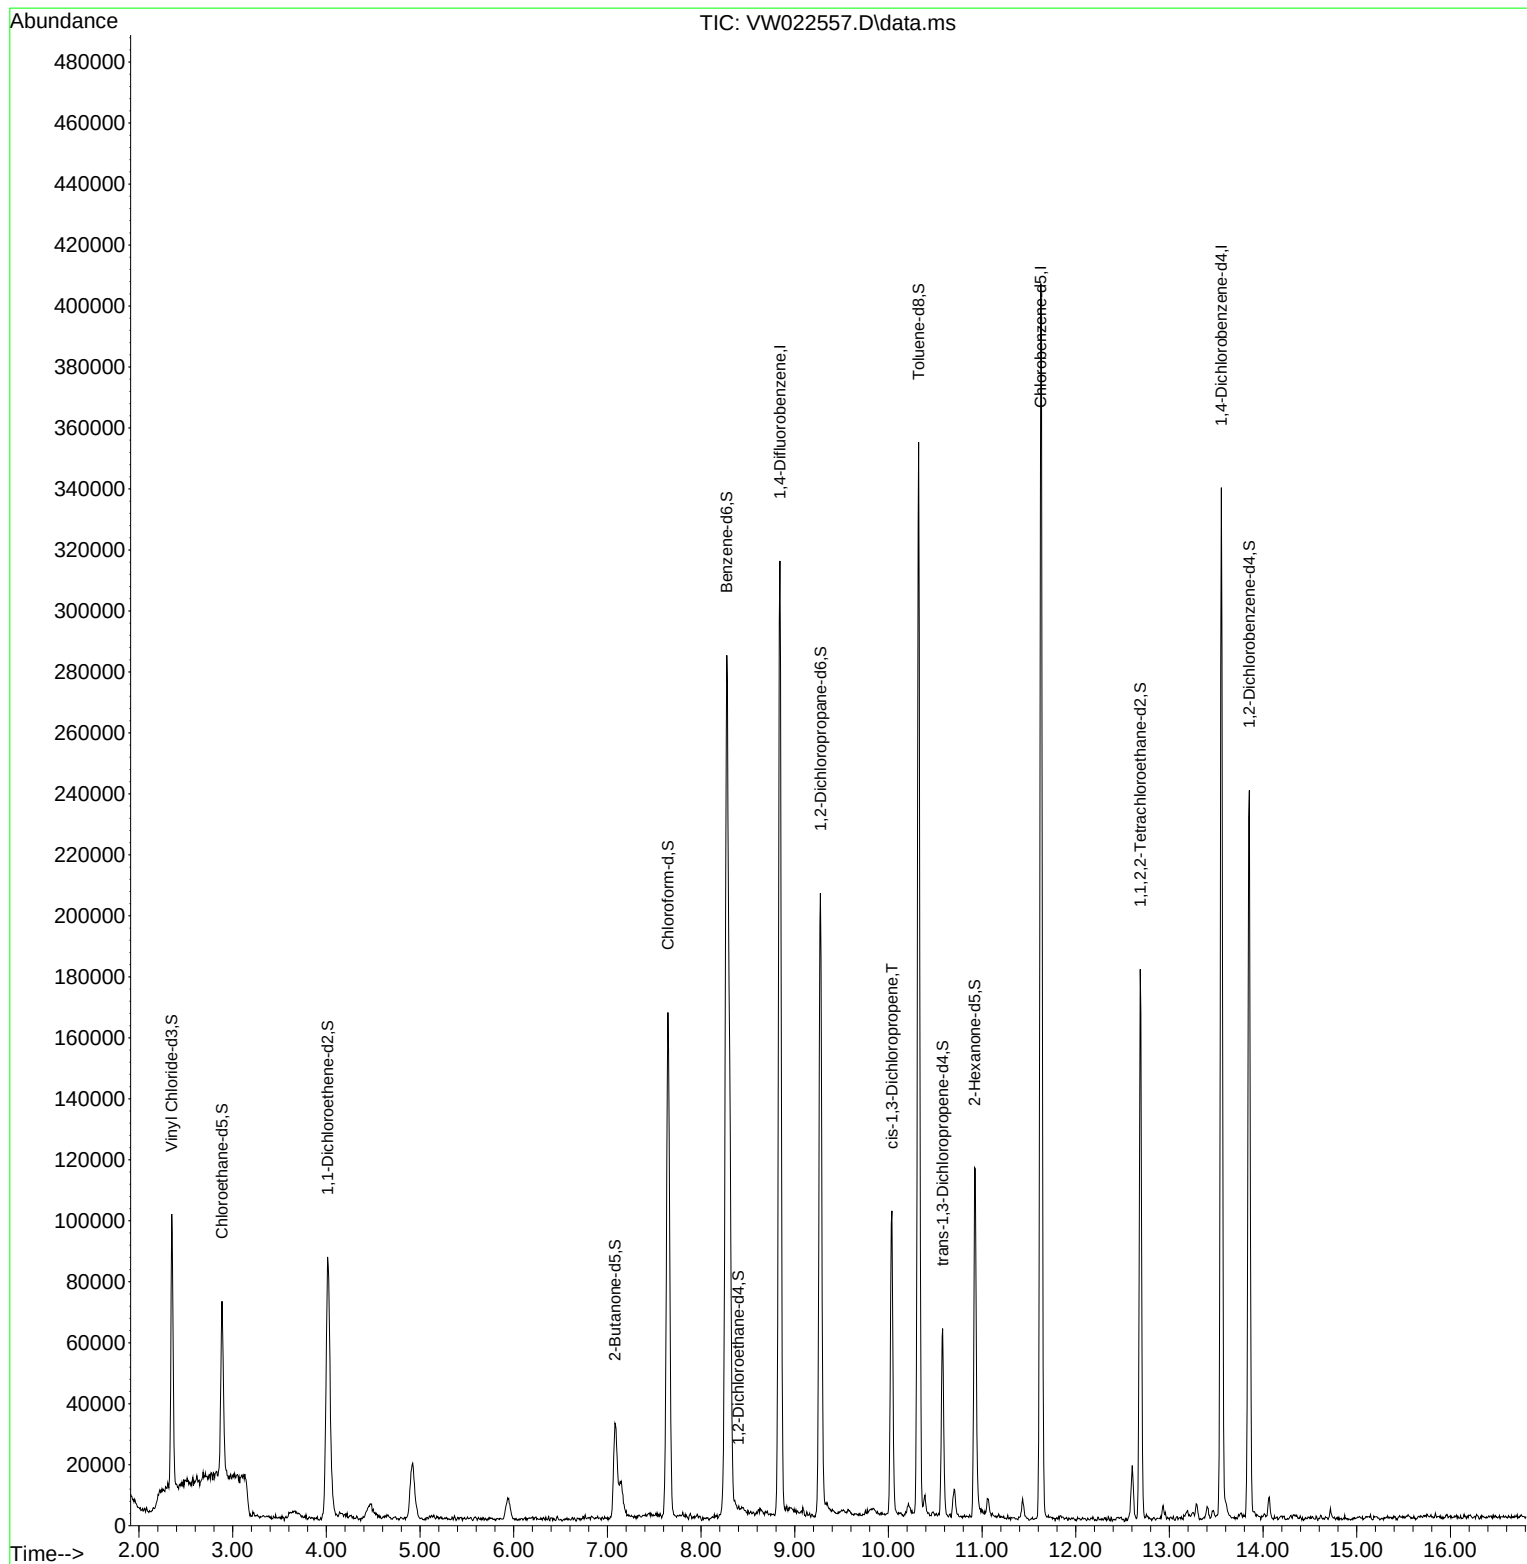

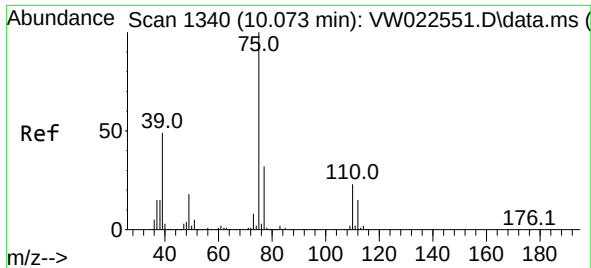

#39
 cis-1,3-Dichloropropene
 Concen: 0.651 ug/L
 RT: 10.037 min Scan# 11
 Delta R.T. -0.036 min
 Lab File: VW022557.D
 Acq: 15 Apr 2022 14:38

Instrument :
 MSVOA_W
 ClientSampleId :

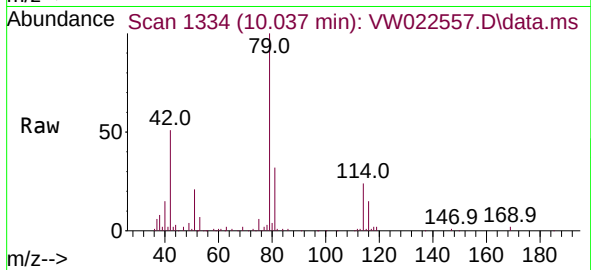

Tgt Ion: 75 Resp: 3630
 Ion Ratio Lower Upper
 75 100
 77 39.2 22.6 42.0

