

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041522\
 Data File : VW022560.D
 Acq On : 15 Apr 2022 16:23
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Apr 15 23:19:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 15 23:17:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.836	114	299931	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	292445	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	151619	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	97937	14.771	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	59.080%
7) Chloroethane-d5	2.891	69	80079	19.271	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.080%
11) 1,1-Dichloroethene-d2	4.019	63	109495	12.732	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	50.920%
21) 2-Butanone-d5	7.074	46	69812	60.307	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	120.620%
24) Chloroform-d	7.647	84	219847	23.451	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.800%
26) 1,2-Dichloroethane-d4	8.305	65	130456	24.355	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	97.440%
32) Benzene-d6	8.275	84	384209	21.504	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	86.000%
36) 1,2-Dichloropropane-d6	9.274	67	123722	23.928	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.720%
41) Toluene-d8	10.323	98	351900	20.110	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	80.440%
43) trans-1,3-Dichloroprop...	10.579	79	48975	20.070	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	80.280%
47) 2-Hexanone-d5	10.921	63	55122	57.299	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	114.600%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	122123	27.778	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	111.120%
66) 1,2-Dichlorobenzene-d4	13.853	152	135951	25.315	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.280%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	4910	0.651	ug/L	# 68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW041522\
Data File : VW022560.D
Acq On : 15 Apr 2022 16:23
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Apr 15 23:19:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM040722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 15 23:17:23 2022
Response via : Initial Calibration

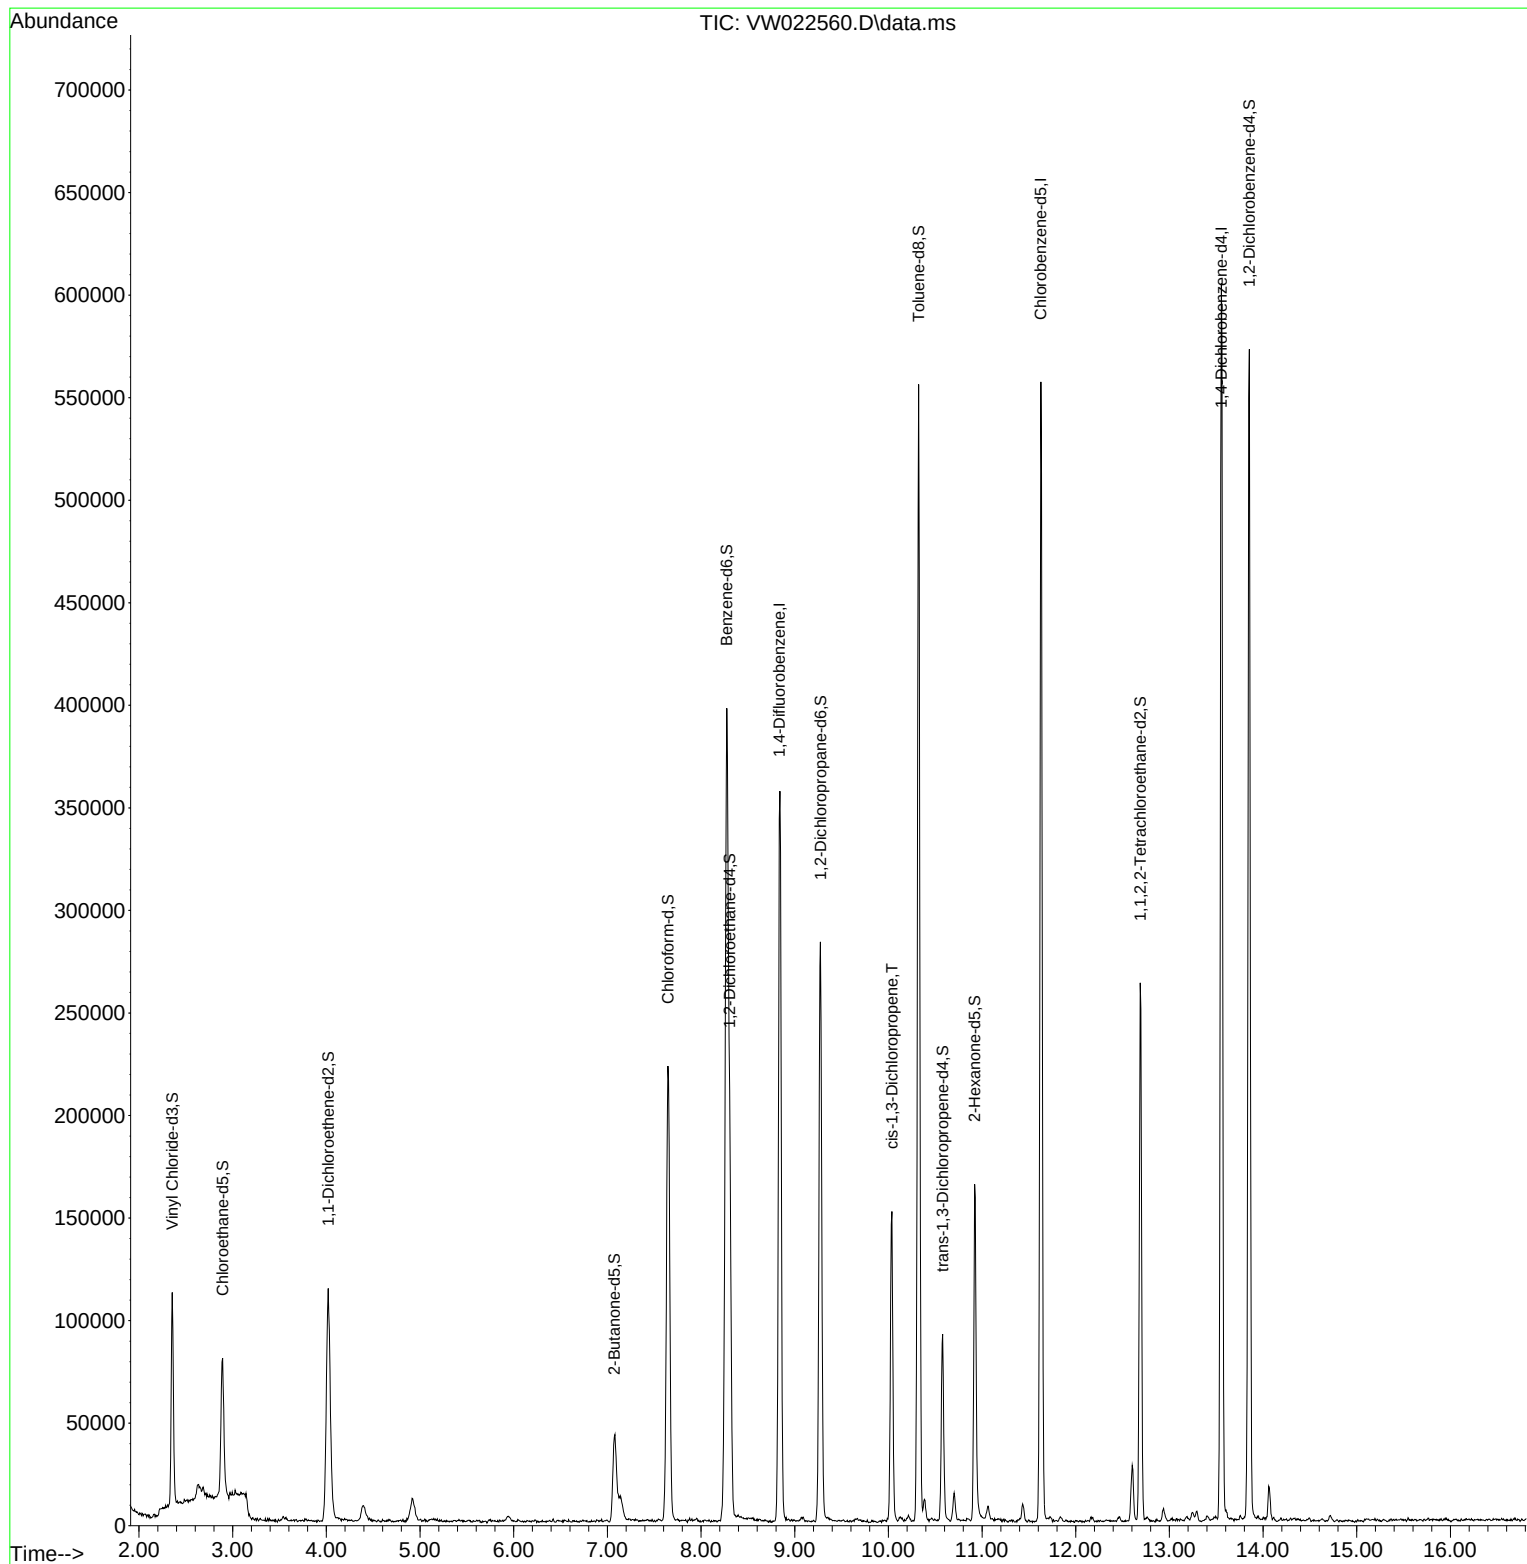

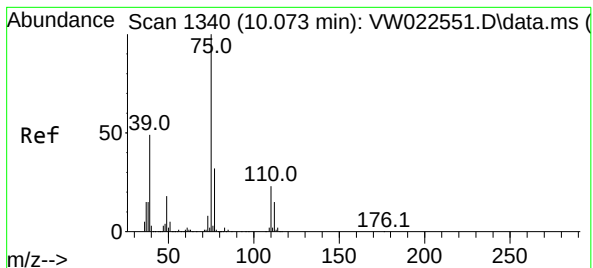

#39
 cis-1,3-Dichloropropene
 Concen: 0.651 ug/L
 RT: 10.037 min Scan# 11
 Delta R.T. -0.036 min
 Lab File: VW022560.D
 Acq: 15 Apr 2022 16:23

Instrument :
 MSVOA_W
 ClientSampleId :

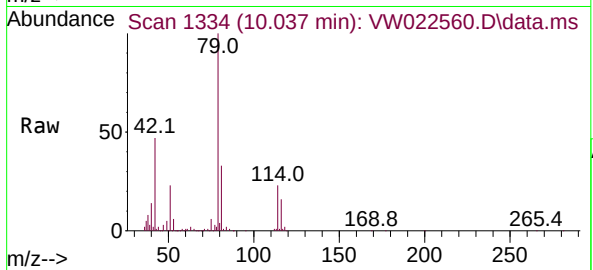

Tgt Ion: 75 Resp: 4910
 Ion Ratio Lower Upper
 75 100
 77 50.0 22.6 42.0#

